

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010289.D
 Acq On : 11 May 2022 15:24
 Operator : CG/JU
 Sample : N2632-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4B5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010289.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	41	45	49	rBV2	18747	24968	0.76%	0.076%
2	3.781	115	118	132	rBV	58506	117784	3.61%	0.360%
3	3.993	151	154	155	rBV3	4823	4791	0.15%	0.015%
4	4.093	168	171	175	rBV4	6376	9033	0.28%	0.028%
5	4.317	206	209	215	rVB7	4291	5450	0.17%	0.017%
6	4.717	275	277	283	rVB7	2748	3747	0.11%	0.011%
7	5.017	322	328	336	rBV4	25017	51086	1.56%	0.156%
8	7.069	670	677	691	rBV	341242	601487	18.41%	1.838%
9	7.234	699	705	717	rBV	297722	487963	14.94%	1.491%
10	7.440	732	740	751	rBV	359105	610178	18.68%	1.864%
11	7.546	753	758	761	rVB6	4397	7270	0.22%	0.022%
12	7.905	811	819	830	rBV	484972	815356	24.96%	2.491%
13	7.981	830	832	837	rVB6	3519	4402	0.13%	0.013%
14	8.616	932	940	952	rBV	424704	754395	23.10%	2.305%
15	8.734	955	960	967	rVB	17216	30214	0.92%	0.092%
16	9.063	1008	1016	1028	rBV	374852	661871	20.26%	2.022%
17	9.234	1043	1045	1049	rVB5	2516	3463	0.11%	0.011%
18	9.510	1086	1092	1097	rBV8	6846	13409	0.41%	0.041%
19	9.787	1132	1139	1151	rBV	307567	547465	16.76%	1.673%
20	10.328	1224	1231	1244	rBV	415833	779515	23.86%	2.382%
21	10.710	1287	1296	1310	rBV	754527	1267802	38.81%	3.874%
22	10.846	1311	1319	1336	rBV	415339	808535	24.75%	2.471%
23	12.304	1558	1567	1574	rBV3	8063	16727	0.51%	0.051%
24	13.287	1728	1734	1739	rVV8	2589	5914	0.18%	0.018%
25	13.375	1744	1749	1754	rVB8	4816	7989	0.24%	0.024%
26	13.945	1839	1846	1857	rBV	1069733	1499430	45.90%	4.582%
27	14.228	1886	1894	1907	rBV	1018377	1585802	48.55%	4.846%
28	14.440	1928	1930	1936	rVB7	3094	4319	0.13%	0.013%
29	14.540	1940	1947	1956	rBV	1255515	1862623	57.02%	5.691%
30	14.734	1973	1980	2005	rBV	274183	614040	18.80%	1.876%
31	14.957	2014	2018	2024	rVB9	12543	22126	0.68%	0.068%
32	15.181	2052	2056	2058	rBV5	2452	3760	0.12%	0.011%
33	15.345	2080	2084	2090	rBV5	8678	17435	0.53%	0.053%
34	15.398	2090	2093	2095	rVB4	3782	4374	0.13%	0.013%
35	15.528	2108	2115	2129	rBV	1405304	2148749	65.78%	6.566%
36	15.651	2129	2136	2149	rVV	425886	672411	20.59%	2.055%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010289.D
 Acq On : 11 May 2022 15:24
 Operator : CG/JU
 Sample : N2632-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4B5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

37	15.775	2152	2157	2166	rVV2	17832	36189	1.11%	0.111%
38	15.845	2166	2169	2174	rVB7	2196	3295	0.10%	0.010%
39	16.322	2246	2250	2252	rVB4	4790	6093	0.19%	0.019%
40	16.834	2333	2337	2343	rVB5	6880	8487	0.26%	0.026%
41	16.969	2358	2360	2363	rVB4	3280	3611	0.11%	0.011%
42	17.286	2408	2414	2421	rVV	1548400	2310124	70.72%	7.059%
43	17.392	2425	2432	2442	rVV	1608805	2478001	75.86%	7.572%
44	17.486	2445	2448	2456	rVB6	24059	39449	1.21%	0.121%
45	17.651	2473	2476	2477	rBV3	5469	4843	0.15%	0.015%
46	17.963	2526	2529	2534	rVB5	9987	11731	0.36%	0.036%
47	18.175	2560	2565	2570	rBV3	27248	47078	1.44%	0.144%
48	18.245	2574	2577	2580	rVB2	7652	11171	0.34%	0.034%
49	19.198	2735	2739	2746	rVB6	28673	43971	1.35%	0.134%
50	19.269	2747	2751	2753	rBV2	21948	32095	0.98%	0.098%
51	19.298	2753	2756	2762	rVB	49722	63422	1.94%	0.194%
52	19.622	2805	2811	2825	rBV	2338876	3266473	100.00%	9.981%
53	21.075	3055	3058	3067	rBV	213028	329521	10.09%	1.007%
54	21.369	3103	3108	3124	rBV	1788196	2557440	78.29%	7.815%
55	23.651	3488	3496	3502	rBV	1443124	2966016	90.80%	9.063%
56	23.804	3515	3522	3532	rVB2	1196018	2431591	74.44%	7.430%


Sum of corrected areas: 32726484

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010289.D
Acq On : 11 May 2022 15:24
Operator : CG/JU
Sample : N2632-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4B5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

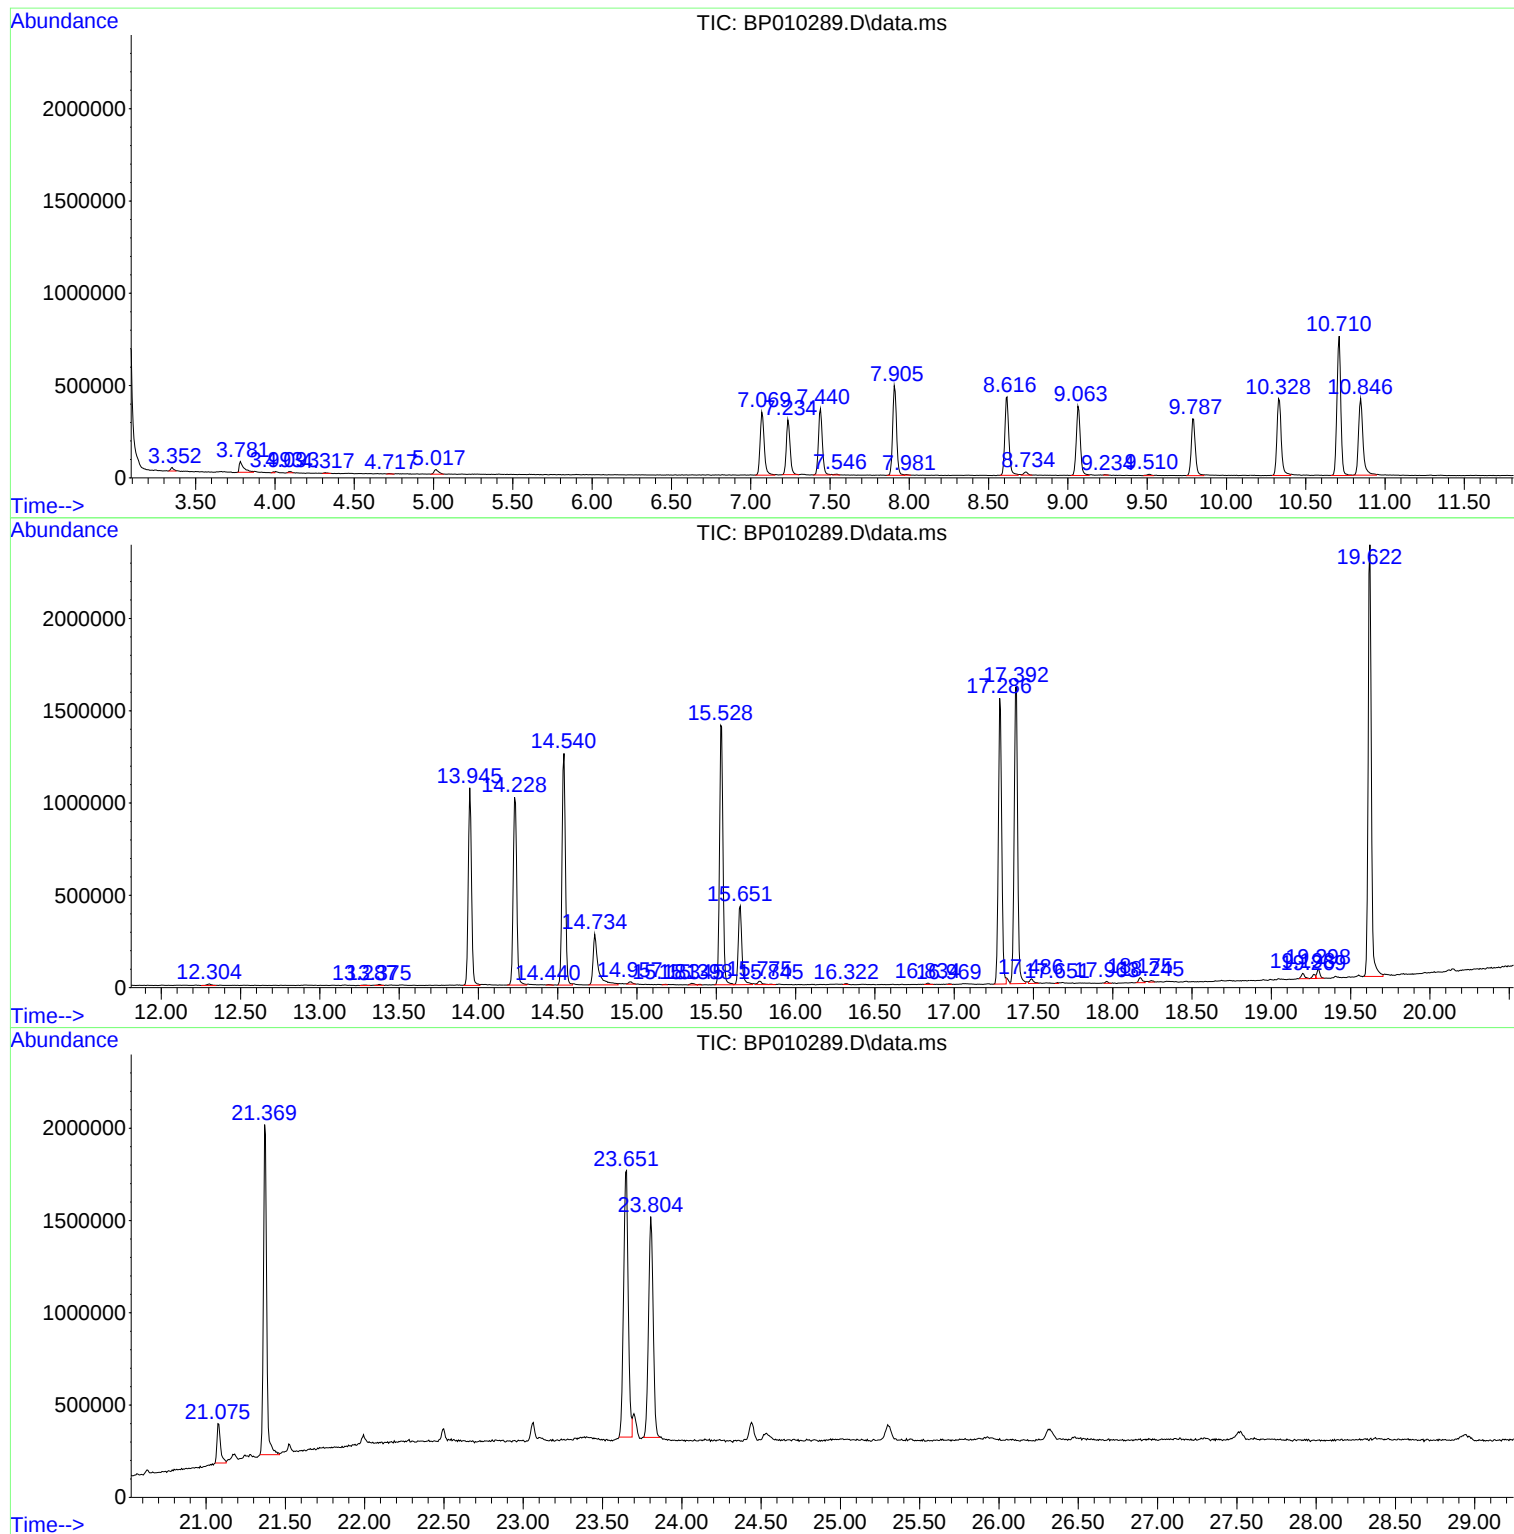

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010289.D
Acq On : 11 May 2022 15:24
Operator : CG/JU
Sample : N2632-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4B5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.075 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.075	2.58 ng/ul	329521	Chrysene-d12	21.375

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cycloeicosane	280	C20H40	000296-56-0	97
2			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
3			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
4			Heptadecyl trifluoroacetate	352	C19H35F3O2	1010351-87-0	94
5			Pentacos-1-ene	350	C25H50	016980-85-1	94

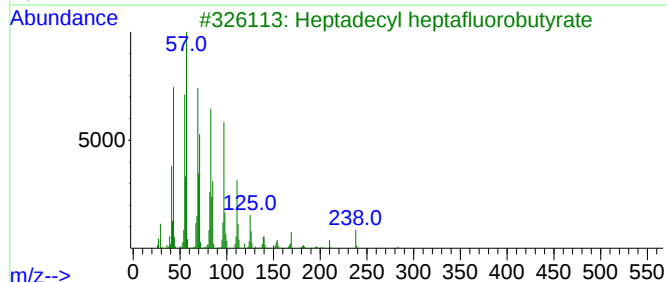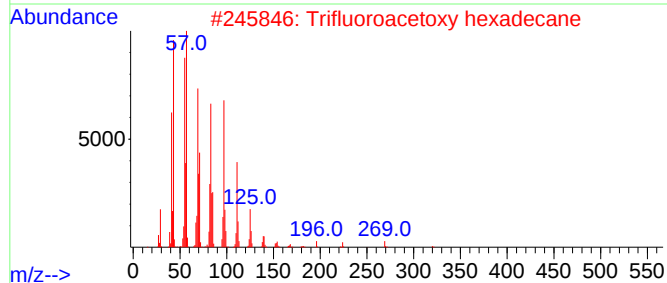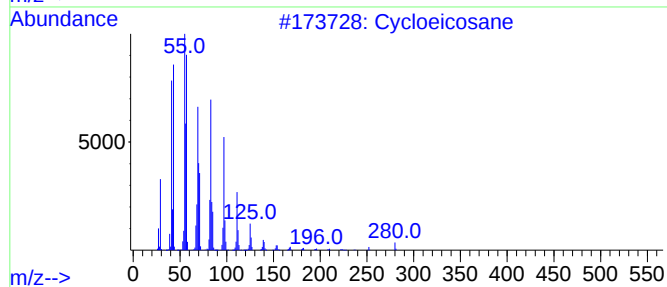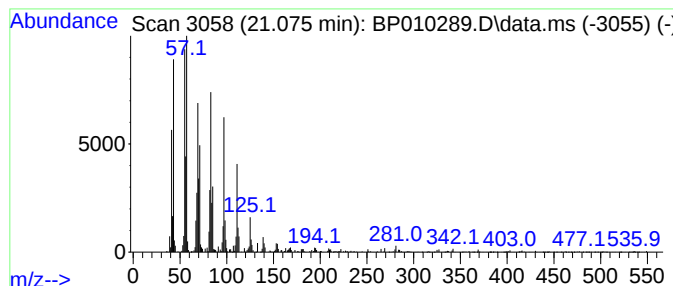

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010289.D
Acq On : 11 May 2022 15:24
Operator : CG/JU
Sample : N2632-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4B5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	21.075	2.6	ng/u1	329521	5	21.375	2557440	20.0