

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010294.D
 Acq On : 11 May 2022 19:24
 Operator : CG/JU
 Sample : PB144657BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK657

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010294.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	41	45	52	rBV	31096	51914	1.34%	0.136%
2	3.764	112	115	134	rBV	400678	760286	19.57%	1.997%
3	4.093	168	171	175	rVB3	8376	10828	0.28%	0.028%
4	4.316	207	209	213	rVB5	3862	4272	0.11%	0.011%
5	7.069	669	677	688	rBV	532094	911290	23.46%	2.393%
6	7.234	698	705	719	rBV	450119	741362	19.09%	1.947%
7	7.440	732	740	756	rBV	568130	937435	24.14%	2.462%
8	7.905	812	819	831	rBV	406073	675846	17.40%	1.775%
9	8.610	932	939	958	rBV	689501	1202572	30.96%	3.158%
10	9.063	1009	1016	1031	rBV	600264	1020382	26.27%	2.680%
11	9.787	1131	1139	1150	rBV	479903	838764	21.59%	2.203%
12	10.328	1222	1231	1243	rBV	651047	1167703	30.06%	3.067%
13	10.710	1287	1296	1308	rBV	596623	1035906	26.67%	2.721%
14	10.846	1311	1319	1337	rBV	667404	1271753	32.74%	3.340%
15	12.310	1563	1568	1576	rVB5	9642	20767	0.53%	0.055%
16	12.916	1666	1671	1674	rBV7	2221	3940	0.10%	0.010%
17	13.281	1728	1733	1737	rBV7	1985	4125	0.11%	0.011%
18	13.945	1839	1846	1858	rBV	1484585	2078172	53.50%	5.458%
19	14.228	1887	1894	1910	rBV	1465082	2241808	57.72%	5.888%
20	14.539	1938	1947	1960	rBV	973230	1500042	38.62%	3.940%
21	14.728	1973	1979	1999	rBV	494267	968110	24.92%	2.543%
22	14.957	2015	2018	2024	rVB8	2627	4059	0.10%	0.011%
23	15.528	2109	2115	2130	rBV	1948396	2915808	75.07%	7.658%
24	15.651	2130	2136	2152	rVV	702889	1064325	27.40%	2.795%
25	15.769	2152	2156	2162	rVB3	24269	42146	1.09%	0.111%
26	16.228	2228	2234	2236	rBV6	2773	4878	0.13%	0.013%
27	16.316	2244	2249	2256	rBV10	8191	14715	0.38%	0.039%
28	16.975	2356	2361	2366	rVB9	4841	7673	0.20%	0.020%
29	17.075	2376	2378	2384	rVB6	2969	5202	0.13%	0.014%
30	17.286	2408	2414	2424	rBV	1301923	1848882	47.60%	4.856%
31	17.386	2424	2431	2446	rVV	2112615	3177245	81.80%	8.344%
32	17.957	2526	2528	2532	rVB4	3721	4005	0.10%	0.011%
33	18.498	2618	2620	2624	rBV5	2965	4433	0.11%	0.012%
34	18.651	2645	2646	2649	rBV3	2911	3892	0.10%	0.010%
35	19.198	2734	2739	2743	rBV2	29101	43945	1.13%	0.115%
36	19.269	2746	2751	2758	rVV	25524	43471	1.12%	0.114%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010294.D
Acq On : 11 May 2022 19:24
Operator : CG/JU
Sample : PB144657BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK657

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Title : SVOA CALIBRATION

37	19.616	2804	2810	2825	rBV	2770804	3884118	100.00%	10.201%
38	21.369	3103	3108	3120	rBV	1478034	2058526	53.00%	5.406%
39	23.645	3488	3495	3501	rBV2	1773053	3535469	91.02%	9.285%
40	23.798	3515	3521	3532	rVB	942372	1966687	50.63%	5.165%




Sum of corrected areas: 38076756

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010294.D
Acq On : 11 May 2022 19:24
Operator : CG/JU
Sample : PB144657BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK657

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

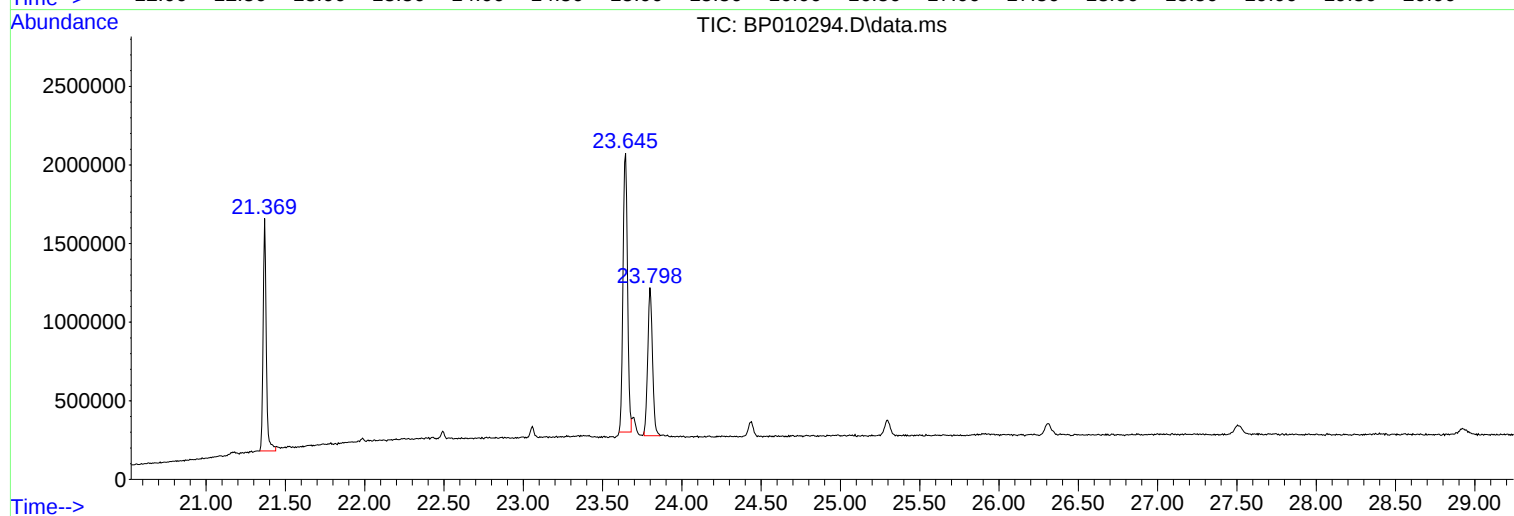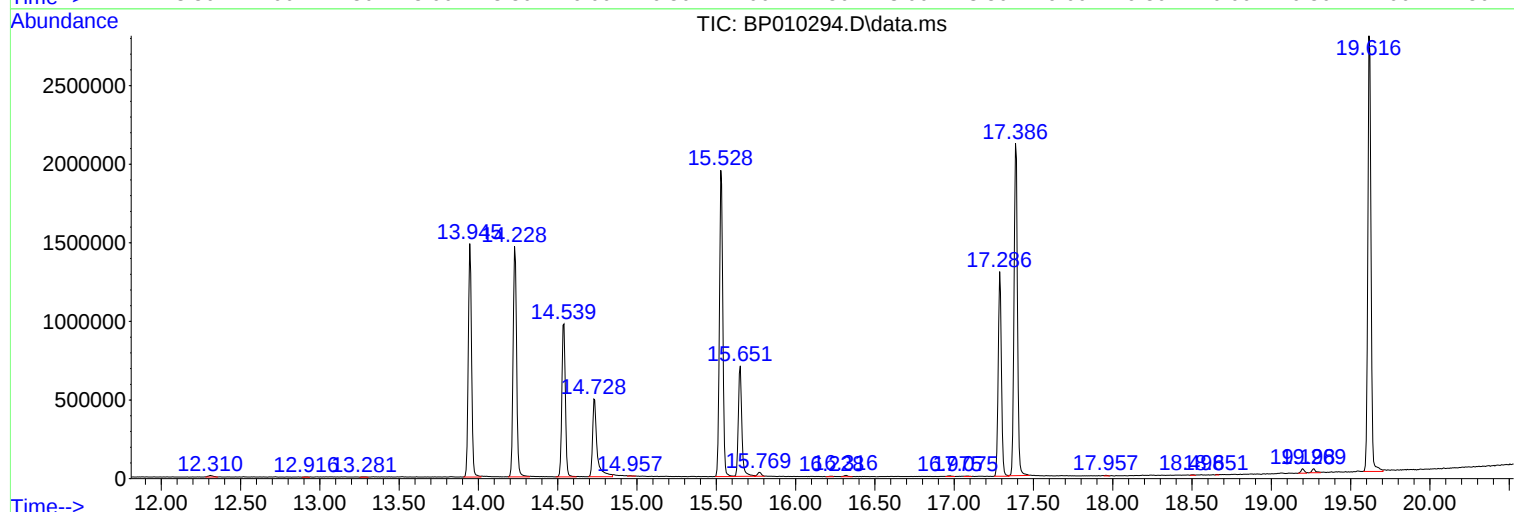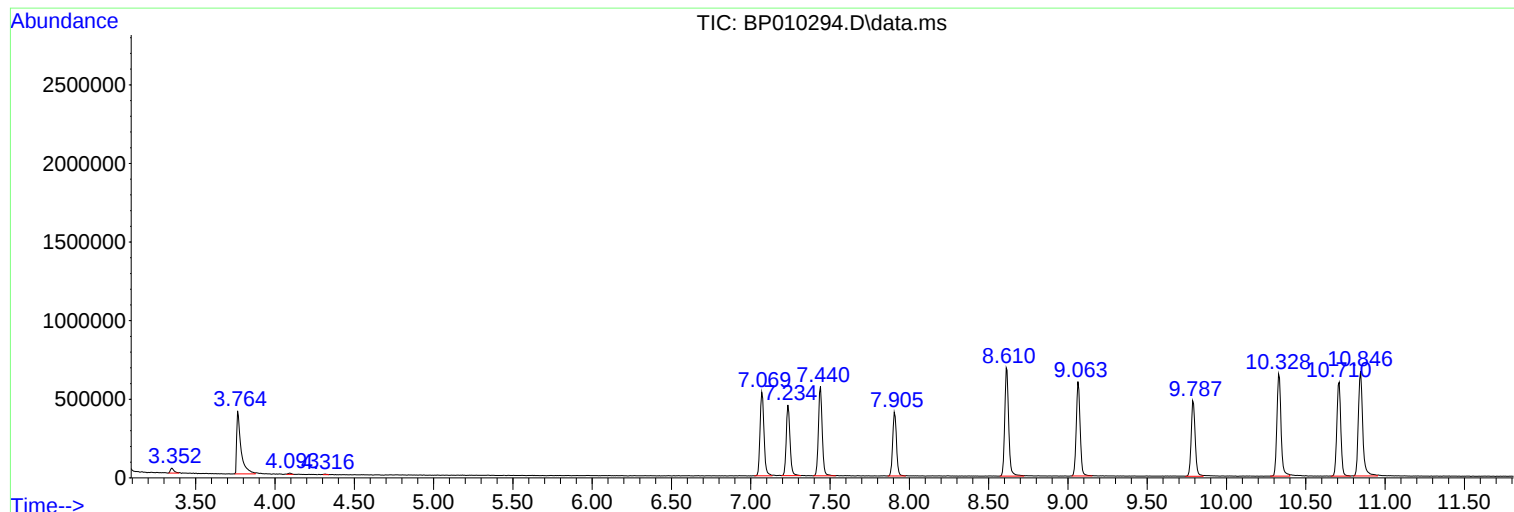

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010294.D
Acq On : 11 May 2022 19:24
Operator : CG/JU
Sample : PB144657BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK657

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010294.D
Acq On : 11 May 2022 19:24
Operator : CG/JU
Sample : PB144657BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK657

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc