

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010302.D
 Acq On : 12 May 2022 01:02
 Operator : CG/JU
 Sample : N2707-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010302.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	41	45	53	rBV	29253	45832	0.73%	0.085%
2	3.781	115	118	133	rBV	81397	178167	2.82%	0.332%
3	4.093	168	171	176	rBV3	9444	13284	0.21%	0.025%
4	4.622	256	261	268	rBV5	23178	41190	0.65%	0.077%
5	7.069	669	677	686	rBV	154243	263284	4.17%	0.491%
6	7.234	698	705	716	rBV	659491	1067029	16.89%	1.988%
7	7.328	719	721	727	rVB5	6190	9033	0.14%	0.017%
8	7.434	732	739	752	rBV	593766	1022539	16.19%	1.905%
9	7.540	753	757	765	rVB10	5001	10734	0.17%	0.020%
10	7.905	812	819	829	rBV	578157	961607	15.22%	1.792%
11	7.969	829	830	839	rVB5	7804	14790	0.23%	0.028%
12	8.610	932	939	952	rBV	481316	827567	13.10%	1.542%
13	9.063	1007	1016	1028	rBV	869494	1489025	23.57%	2.775%
14	9.193	1033	1038	1043	rVV8	3746	7637	0.12%	0.014%
15	9.510	1087	1092	1099	rBV3	17317	28636	0.45%	0.053%
16	9.787	1131	1139	1156	rBV	693339	1202645	19.04%	2.241%
17	10.328	1223	1231	1249	rBV	916349	1601520	25.35%	2.984%
18	10.704	1288	1295	1310	rBV	852995	1484965	23.51%	2.767%
19	10.840	1310	1318	1337	rBV	776334	1478496	23.40%	2.755%
20	11.369	1405	1408	1418	rVB	2800	6547	0.10%	0.012%
21	12.140	1533	1539	1547	rVB3	8749	15098	0.24%	0.028%
22	12.304	1560	1567	1574	rBV2	15044	29306	0.46%	0.055%
23	12.946	1673	1676	1683	rVB9	3326	6414	0.10%	0.012%
24	13.157	1708	1712	1718	rVB8	5261	8748	0.14%	0.016%
25	13.369	1742	1748	1754	rBV2	14662	22180	0.35%	0.041%
26	13.440	1757	1760	1765	rVV7	4537	6979	0.11%	0.013%
27	13.945	1839	1846	1858	rBV	2229513	3072028	48.63%	5.725%
28	14.228	1883	1894	1907	rBV	2291445	3369196	53.33%	6.278%
29	14.534	1940	1946	1961	rBV	1419162	2132387	33.75%	3.974%
30	14.734	1972	1980	1993	rBV	101464	239670	3.79%	0.447%
31	14.957	2014	2018	2025	rVB7	8387	14333	0.23%	0.027%
32	15.357	2079	2086	2090	rBV2	16913	30468	0.48%	0.057%
33	15.528	2108	2115	2127	rBV	2975738	4453639	70.50%	8.299%
34	15.645	2129	2135	2151	rVV	1173252	1774224	28.08%	3.306%
35	15.769	2152	2156	2165	rVB2	37520	67051	1.06%	0.125%
36	15.898	2174	2178	2182	rVB7	5219	7457	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010302.D
 Acq On : 12 May 2022 01:02
 Operator : CG/JU
 Sample : N2707-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

37	16.316	2245	2249	2253	rVB5	13087	18733	0.30%	0.035%
38	16.439	2264	2270	2274	rBV9	3111	6813	0.11%	0.013%
39	16.969	2356	2360	2364	rVB6	5743	7898	0.13%	0.015%
40	17.057	2370	2375	2376	rBV5	6482	7691	0.12%	0.014%
41	17.286	2405	2414	2424	rBV	1773844	2632558	41.67%	4.906%
42	17.386	2424	2431	2455	rVB	3668281	5245686	83.04%	9.775%
43	17.681	2478	2481	2486	rVB6	6300	8258	0.13%	0.015%
44	17.963	2523	2529	2535	rBV	124531	161769	2.56%	0.301%
45	18.169	2559	2564	2573	rBV3	60120	106865	1.69%	0.199%
46	18.651	2642	2646	2649	rBV6	3594	7223	0.11%	0.013%
47	19.086	2716	2720	2724	rVB	107250	115245	1.82%	0.215%
48	19.198	2734	2739	2745	rBV3	45327	73102	1.16%	0.136%
49	19.263	2746	2750	2762	rVV	46650	79325	1.26%	0.148%
50	19.404	2771	2774	2779	rBV4	25244	39395	0.62%	0.073%
51	19.539	2795	2797	2803	rVB6	11626	17467	0.28%	0.033%
52	19.622	2804	2811	2826	rBV	4536259	6317436	100.00%	11.772%
53	21.075	3054	3058	3065	rBV	145000	224727	3.56%	0.419%
54	21.369	3103	3108	3115	rBV	2055925	2744340	43.44%	5.114%
55	23.645	3487	3495	3502	rBV2	2966253	5942338	94.06%	11.073%
56	23.798	3514	3521	3534	rVB2	1334501	2689386	42.57%	5.012%
57	24.433	3625	3629	3637	rVB3	113721	213875	3.39%	0.399%


Sum of corrected areas: 53663835

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010302.D
Acq On : 12 May 2022 01:02
Operator : CG/JU
Sample : N2707-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

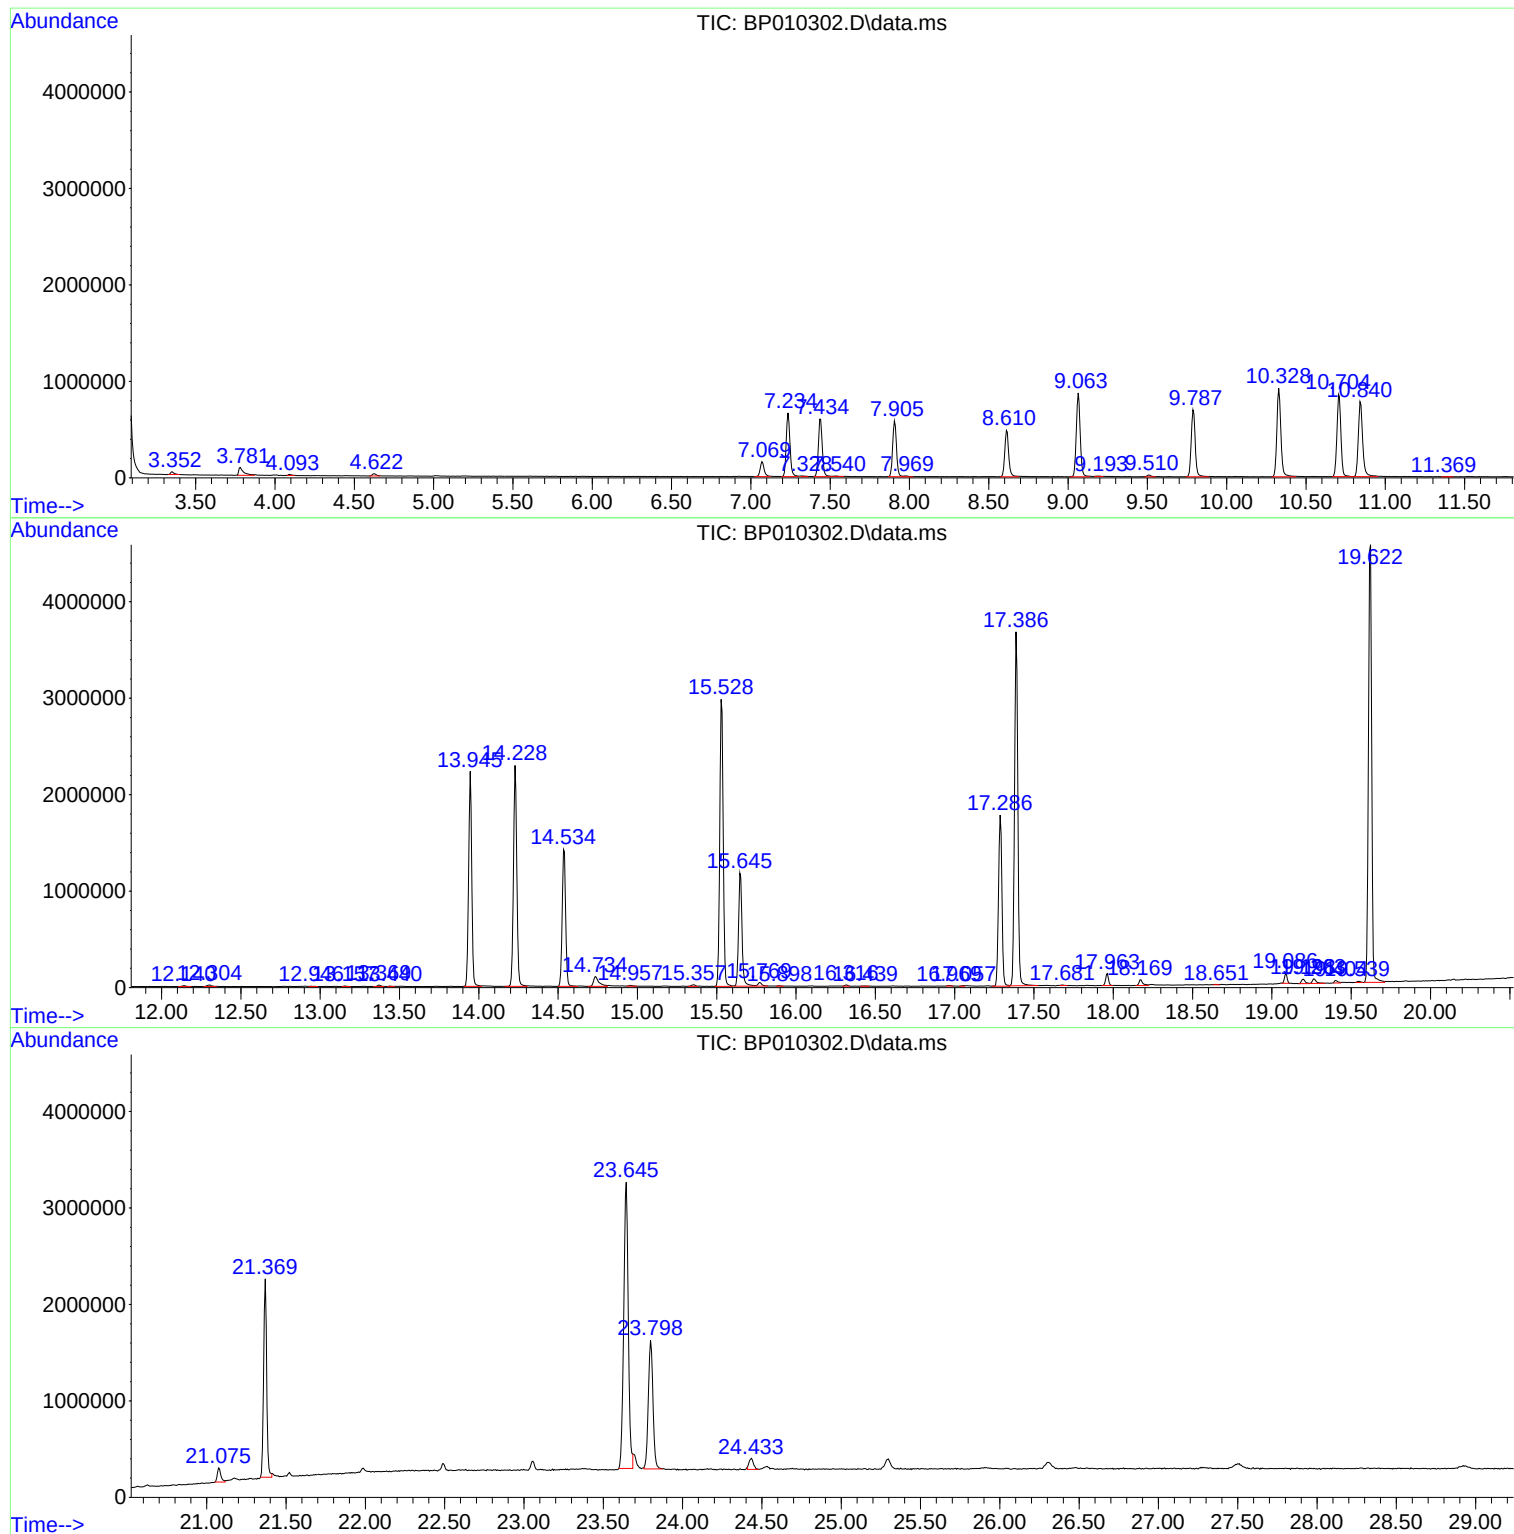

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010302.D
Acq On : 12 May 2022 01:02
Operator : CG/JU
Sample : N2707-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010302.D
Acq On : 12 May 2022 01:02
Operator : CG/JU
Sample : N2707-11
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc