

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010305.D
 Acq On : 12 May 2022 02:43
 Operator : CG/JU
 Sample : N2707-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	41	44	52	rBV	30912	41661	0.84%	0.098%
2	3.775	115	117	132	rBV	70239	138162	2.79%	0.326%
3	4.087	166	170	176	rBV	13955	25469	0.51%	0.060%
4	4.623	256	261	271	rVB2	46944	79866	1.61%	0.189%
5	5.022	325	329	337	rVB2	17099	29675	0.60%	0.070%
6	5.193	350	358	367	rBV2	14844	27350	0.55%	0.065%
7	7.069	671	677	687	rBV	120216	211740	4.27%	0.500%
8	7.234	698	705	717	rBV	496274	818156	16.51%	1.932%
9	7.440	733	740	753	rBV	480350	814202	16.43%	1.923%
10	7.540	756	757	763	rVB6	4886	5114	0.10%	0.012%
11	7.905	812	819	828	rBV	526220	867773	17.51%	2.049%
12	7.975	828	831	837	rVB7	6396	12247	0.25%	0.029%
13	8.611	933	939	953	rBV2	354032	616110	12.43%	1.455%
14	9.063	1007	1016	1028	rBV	658545	1122094	22.64%	2.650%
15	9.510	1086	1092	1101	rVB	23264	41819	0.84%	0.099%
16	9.787	1132	1139	1157	rBV	511702	890604	17.97%	2.103%
17	10.328	1224	1231	1245	rBV	697346	1233777	24.90%	2.914%
18	10.705	1286	1295	1310	rBV	723813	1266117	25.55%	2.990%
19	10.846	1310	1319	1335	rBV	372991	757597	15.29%	1.789%
20	11.540	1431	1437	1442	rBV10	3136	6760	0.14%	0.016%
21	12.134	1534	1538	1544	rVB4	8842	14503	0.29%	0.034%
22	12.234	1548	1555	1562	rBV	196074	351850	7.10%	0.831%
23	12.299	1562	1566	1578	rVB2	16341	38244	0.77%	0.090%
24	13.163	1711	1713	1719	rVB6	4496	6837	0.14%	0.016%
25	13.375	1744	1749	1754	rBV	13934	21358	0.43%	0.050%
26	13.728	1805	1809	1814	rBV7	4574	8532	0.17%	0.020%
27	13.946	1839	1846	1858	rBV	1637665	2304736	46.51%	5.443%
28	14.228	1885	1894	1910	rBV	1689652	2504535	50.54%	5.915%
29	14.440	1928	1930	1937	rVB8	4234	6363	0.13%	0.015%
30	14.534	1939	1946	1959	rBV	1189484	1818177	36.69%	4.294%
31	14.734	1972	1980	1999	rBV2	60967	179030	3.61%	0.423%
32	14.893	2005	2007	2014	rVB8	4377	6541	0.13%	0.015%
33	14.957	2014	2018	2024	rVB9	7737	14264	0.29%	0.034%
34	15.181	2049	2056	2063	rVB9	3276	6850	0.14%	0.016%
35	15.351	2078	2085	2090	rVB2	14926	25200	0.51%	0.060%
36	15.528	2109	2115	2128	rBV	2259986	3362400	67.85%	7.941%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010305.D
 Acq On : 12 May 2022 02:43
 Operator : CG/JU
 Sample : N2707-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXL85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

37	15.651	2129	2136	2150	rVV	854543	1289485	26.02%	3.045%
38	15.775	2152	2157	2163	rVB2	26405	45232	0.91%	0.107%
39	15.898	2172	2178	2183	rBV8	3845	7292	0.15%	0.017%
40	15.957	2183	2188	2192	rVB7	3118	5775	0.12%	0.014%
41	16.316	2245	2249	2254	rVB6	11573	16070	0.32%	0.038%
42	16.969	2355	2360	2363	rBV5	6035	9051	0.18%	0.021%
43	17.075	2376	2378	2384	rVB6	3480	5859	0.12%	0.014%
44	17.287	2407	2414	2424	rBV	1638059	2291052	46.23%	5.411%
45	17.387	2424	2431	2447	rVV	3000407	4145060	83.64%	9.789%
46	17.751	2489	2493	2499	rVB8	3635	6840	0.14%	0.016%
47	17.957	2524	2528	2533	rVB8	5408	8792	0.18%	0.021%
48	18.169	2559	2564	2573	rBV3	45283	87029	1.76%	0.206%
49	18.239	2575	2576	2581	rVB3	10064	11943	0.24%	0.028%
50	18.639	2642	2644	2647	rBV4	4389	5308	0.11%	0.013%
51	19.198	2734	2739	2745	rBV2	36182	53414	1.08%	0.126%
52	19.263	2746	2750	2756	rVV	37004	52388	1.06%	0.124%
53	19.404	2770	2774	2779	rBV7	18200	29536	0.60%	0.070%
54	19.616	2804	2810	2824	rBV	3710814	4955550	100.00%	11.704%
55	21.075	3054	3058	3065	rBV3	135777	204022	4.12%	0.482%
56	21.369	3102	3108	3121	rBV	1792308	2543230	51.32%	6.006%
57	23.645	3487	3495	3502	rBV	2222737	4515972	91.13%	10.665%
58	23.798	3514	3521	3532	rVB2	1172281	2377797	47.98%	5.616%




Sum of corrected areas: 42342410

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010305.D
Acq On : 12 May 2022 02:43
Operator : CG/JU
Sample : N2707-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL85

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

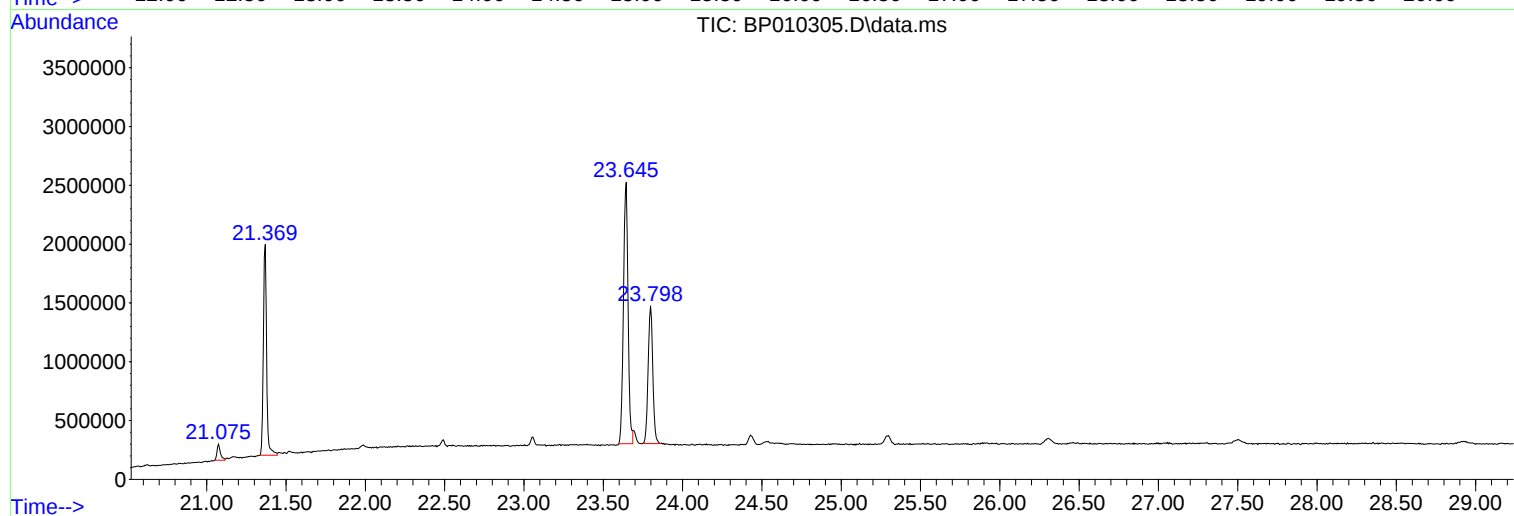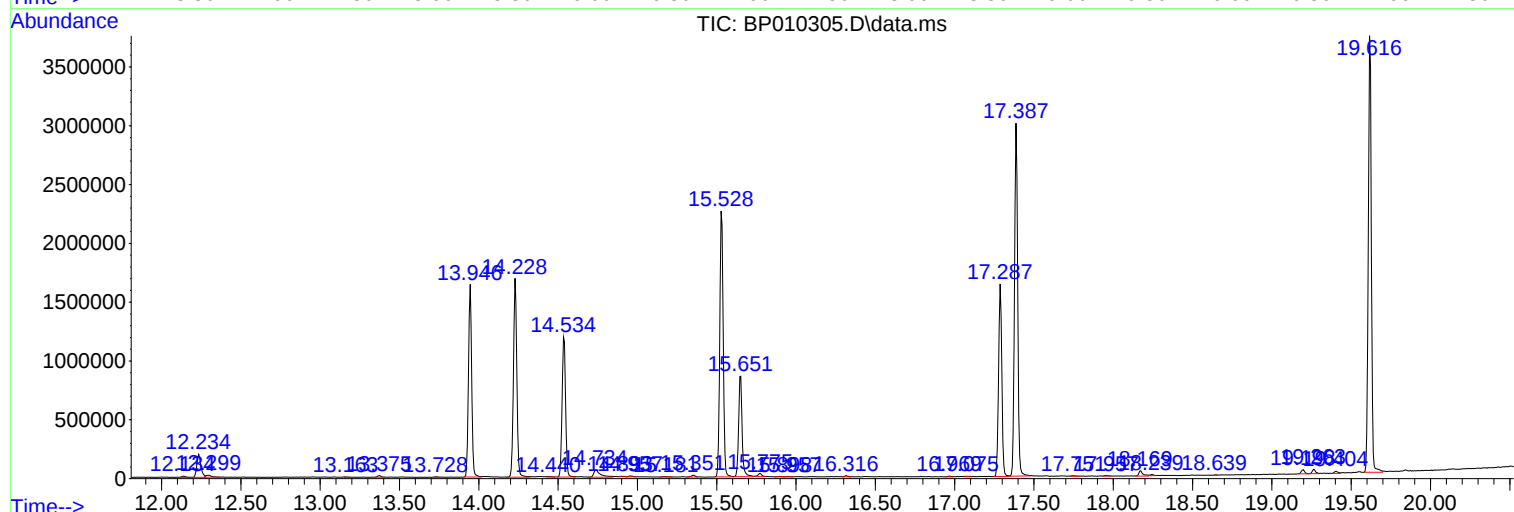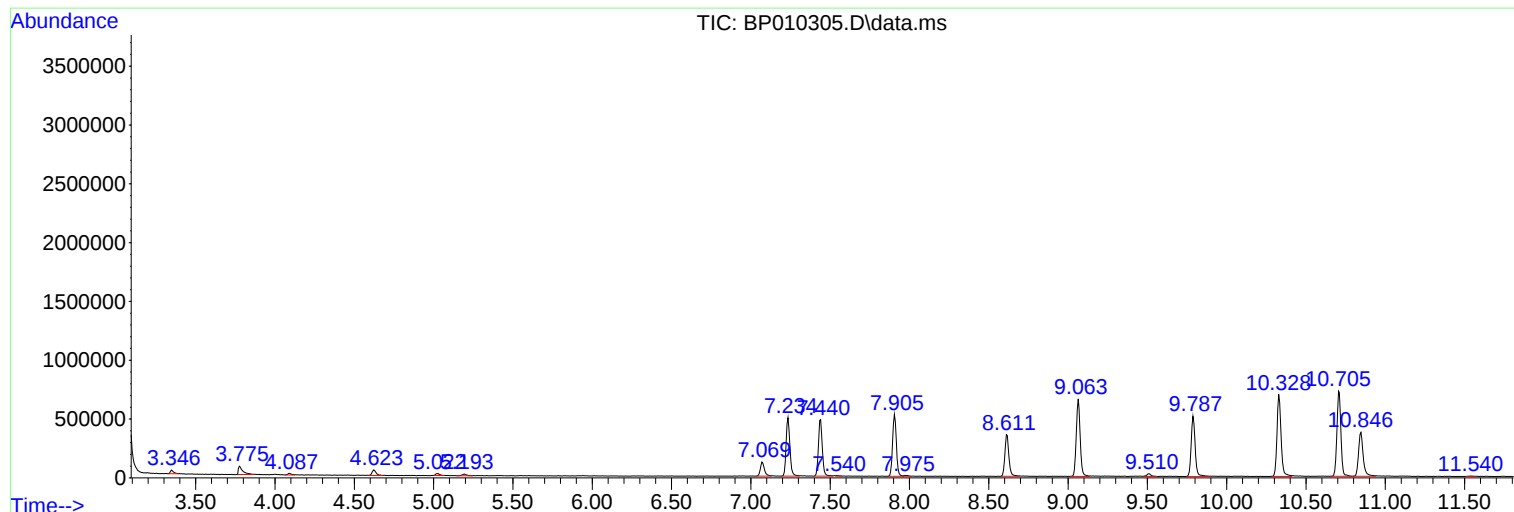

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010305.D
Acq On : 12 May 2022 02:43
Operator : CG/JU
Sample : N2707-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL85










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.234	5.56 ng/ul	351850	Naphthalene-d8	10.704

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	6-Isopropylquinoline		171	C12H13N	000135-79-5	43	
2	1,3-Diaza-5,6-dedihydrocyclohexa...		171	C6H9N3OS	021263-85-4	38	
3	Benzene, 1-chloro-4-methoxy-2-me...		156	C8H9ClO	013334-71-9	32	
4	2-Piperidinone, 1-(trimethylsilyl)-		171	C8H17NOSi	003553-93-3	32	
5	2-Chloro-4,6-dimethyl-3-pyridina...		156	C7H9ClN2	140413-40-7	32	

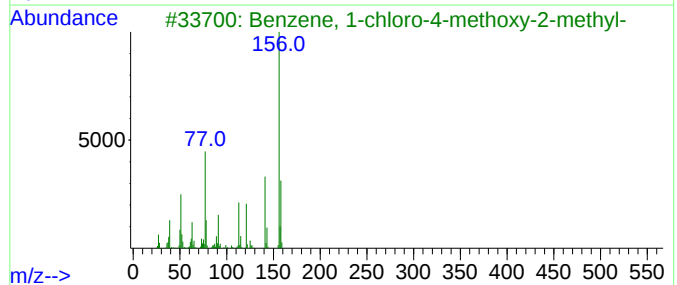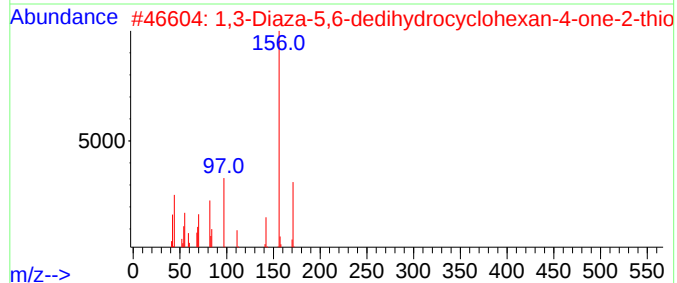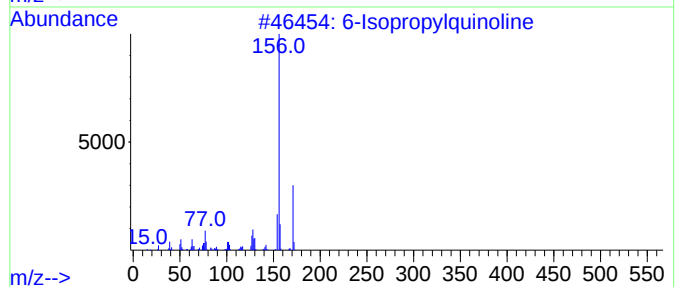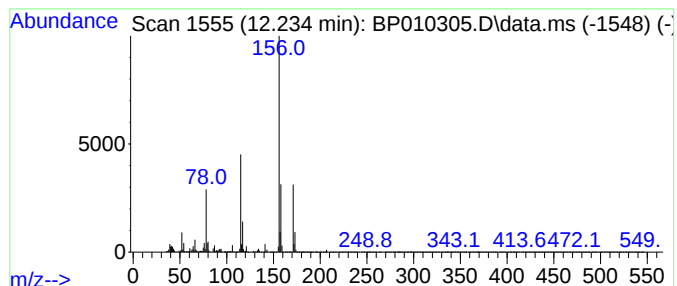

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010305.D
Acq On : 12 May 2022 02:43
Operator : CG/JU
Sample : N2707-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXL85

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	12.234	5.6	ng/u1	351850	2	10.704	1266120	20.0