

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010334.D
 Acq On : 12 May 2022 21:23
 Operator : CG/JU
 Sample : N2746-02
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBSK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	41	44	49	rBV	20027	27591	0.89%	0.083%
2	3.652	95	96	99	rBV3	3709	3869	0.13%	0.012%
3	3.769	112	116	131	rBV	249607	517782	16.75%	1.548%
4	4.087	167	170	179	rVB2	7506	11737	0.38%	0.035%
5	4.905	304	309	313	rBV7	2576	5309	0.17%	0.016%
6	5.016	323	328	335	rBV5	6042	14461	0.47%	0.043%
7	5.193	355	358	363	rVB6	2290	3760	0.12%	0.011%
8	7.069	670	677	689	rBV	387925	667531	21.59%	1.996%
9	7.234	698	705	716	rBV	309586	529205	17.12%	1.583%
10	7.316	716	719	725	rVB3	4906	7826	0.25%	0.023%
11	7.434	731	739	752	rBV	394514	677704	21.92%	2.027%
12	7.904	810	819	828	rBV	445970	757159	24.49%	2.264%
13	8.610	932	939	952	rBV	518080	884111	28.60%	2.644%
14	9.063	1009	1016	1025	rBV	423597	744279	24.08%	2.226%
15	9.240	1041	1046	1052	rVB10	4555	10160	0.33%	0.030%
16	9.504	1087	1091	1098	rVB8	5642	11252	0.36%	0.034%
17	9.787	1128	1139	1154	rBV	348480	618154	20.00%	1.849%
18	10.163	1199	1203	1210	rVB10	1515	4267	0.14%	0.013%
19	10.328	1223	1231	1251	rBV	487737	897640	29.04%	2.684%
20	10.481	1254	1257	1262	rVB7	2485	4068	0.13%	0.012%
21	10.704	1285	1295	1301	rBV	670652	1150162	37.20%	3.440%
22	10.751	1301	1303	1309	rVB	31622	47798	1.55%	0.143%
23	10.840	1311	1318	1335	rBV	474027	932834	30.17%	2.790%
24	10.975	1340	1341	1350	rVB8	3354	6144	0.20%	0.018%
25	11.275	1389	1392	1398	rVB6	2305	4577	0.15%	0.014%
26	11.751	1469	1473	1477	rVB7	1940	3285	0.11%	0.010%
27	12.298	1558	1566	1573	rBV5	7831	18049	0.58%	0.054%
28	12.369	1573	1578	1583	rVB7	3846	7526	0.24%	0.023%
29	12.510	1597	1602	1605	rBV6	3625	7154	0.23%	0.021%
30	12.587	1611	1615	1619	rBV5	4544	7643	0.25%	0.023%
31	12.734	1636	1640	1644	rBV7	1861	3363	0.11%	0.010%
32	13.257	1724	1729	1736	rBV7	2787	6242	0.20%	0.019%
33	13.375	1745	1749	1754	rVB6	7842	10937	0.35%	0.033%
34	13.504	1768	1771	1777	rVB8	4842	6883	0.22%	0.021%
35	13.710	1803	1806	1813	rVB7	6829	10420	0.34%	0.031%
36	13.851	1827	1830	1834	rVB5	2063	3368	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010334.D
 Acq On : 12 May 2022 21:23
 Operator : CG/JU
 Sample : N2746-02
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBSK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

37	13.939	1838	1845	1857	rBV	1110353	1597553	51.68%	4.777%
38	14.228	1883	1894	1904	rBV	1159219	1757223	56.84%	5.255%
39	14.534	1939	1946	1953	rBV	1143834	1669588	54.01%	4.993%
40	14.598	1953	1957	1962	rVB2	25912	38693	1.25%	0.116%
41	14.669	1964	1969	1973	rBV2	13492	20861	0.67%	0.062%
42	14.728	1973	1979	1990	rBV	337687	652619	21.11%	1.952%
43	14.939	2010	2015	2026	rVB2	18426	50989	1.65%	0.152%
44	15.081	2034	2039	2045	rBV	43869	68437	2.21%	0.205%
45	15.163	2049	2053	2059	rVB7	14178	22689	0.73%	0.068%
46	15.281	2066	2073	2077	rBV4	5801	12092	0.39%	0.036%
47	15.345	2080	2084	2089	rVB8	4934	9898	0.32%	0.030%
48	15.528	2108	2115	2121	rBV	1601463	2299003	74.37%	6.875%
49	15.581	2121	2124	2129	rVB2	19731	31221	1.01%	0.093%
50	15.645	2129	2135	2144	rBV	446434	658349	21.30%	1.969%
51	15.769	2150	2156	2162	rVB	18930	29959	0.97%	0.090%
52	15.892	2172	2177	2181	rVB8	4038	5807	0.19%	0.017%
53	15.957	2185	2188	2191	rBV5	2224	3343	0.11%	0.010%
54	16.251	2234	2238	2242	rBV7	4398	7923	0.26%	0.024%
55	16.316	2245	2249	2255	rVB8	8777	13843	0.45%	0.041%
56	16.410	2262	2265	2267	rBV4	2460	3338	0.11%	0.010%
57	16.451	2270	2272	2276	rVB5	2920	4920	0.16%	0.015%
58	16.551	2284	2289	2295	rBV7	3674	7353	0.24%	0.022%
59	16.939	2350	2355	2364	rVB3	46749	83448	2.70%	0.250%
60	17.069	2374	2377	2387	rVB10	5602	13957	0.45%	0.042%
61	17.280	2405	2413	2419	rBV	1377429	2074244	67.10%	6.203%
62	17.380	2424	2430	2443	rVB	1662294	2502573	80.95%	7.484%
63	17.692	2473	2483	2494	rBV	68005	122181	3.95%	0.365%
64	17.851	2507	2510	2515	rBV5	4131	7966	0.26%	0.024%
65	17.904	2515	2519	2524	rVV6	19306	26630	0.86%	0.080%
66	17.951	2524	2527	2531	rVB5	6320	9733	0.31%	0.029%
67	18.169	2559	2564	2574	rBV3	50520	102278	3.31%	0.306%
68	18.569	2629	2632	2633	rBV3	4247	5015	0.16%	0.015%
69	19.033	2709	2711	2712	rBV2	5847	3843	0.12%	0.011%
70	19.192	2734	2738	2742	rBV3	24993	32645	1.06%	0.098%
71	19.263	2746	2750	2753	rBV	19138	28121	0.91%	0.084%
72	19.398	2771	2773	2776	rBV4	10413	12828	0.41%	0.038%
73	19.616	2804	2810	2823	rBV	2321134	3091497	100.00%	9.245%
74	21.074	3054	3058	3063	rBV2	93072	131579	4.26%	0.393%
75	21.363	3102	3107	3123	rBV	1730397	2425820	78.47%	7.254%
76	23.633	3486	3493	3500	rBV2	1419415	2899599	93.79%	8.671%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010334.D
Acq On : 12 May 2022 21:23
Operator : CG/JU
Sample : N2746-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBSK5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Title : SVOA CALIBRATION

77 23.792 3513 3520 3534 rVB2 1085151 2275206 73.60% 6.804%




Sum of corrected areas: 33439114

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010334.D
Acq On : 12 May 2022 21:23
Operator : CG/JU
Sample : N2746-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBSK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

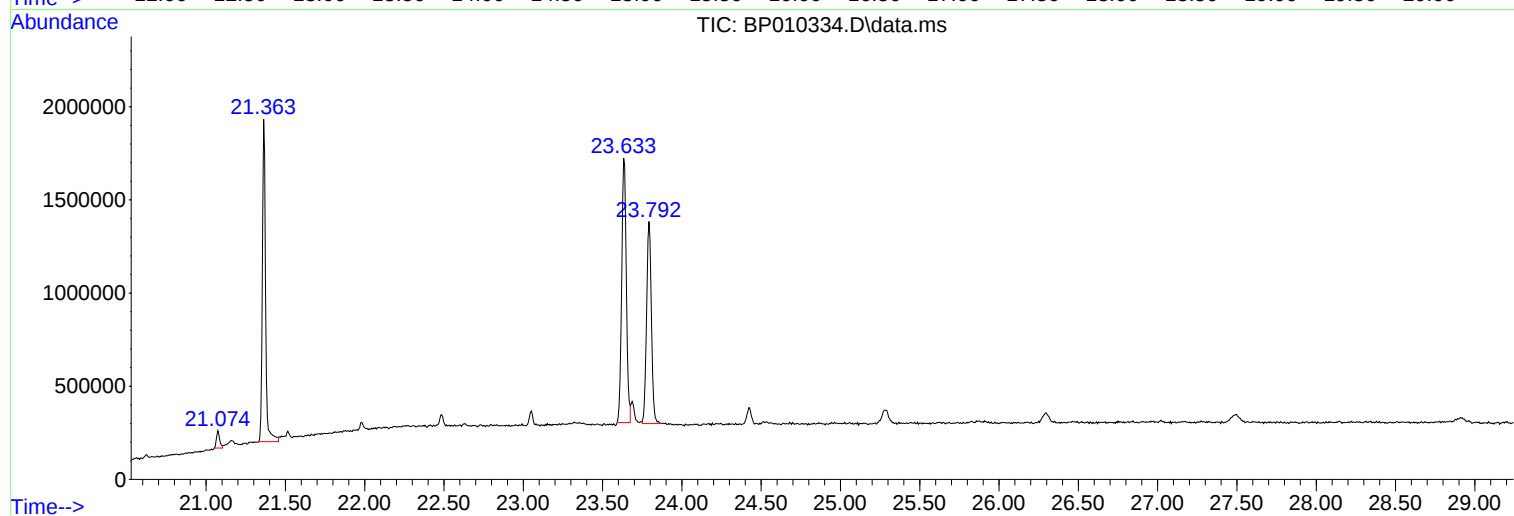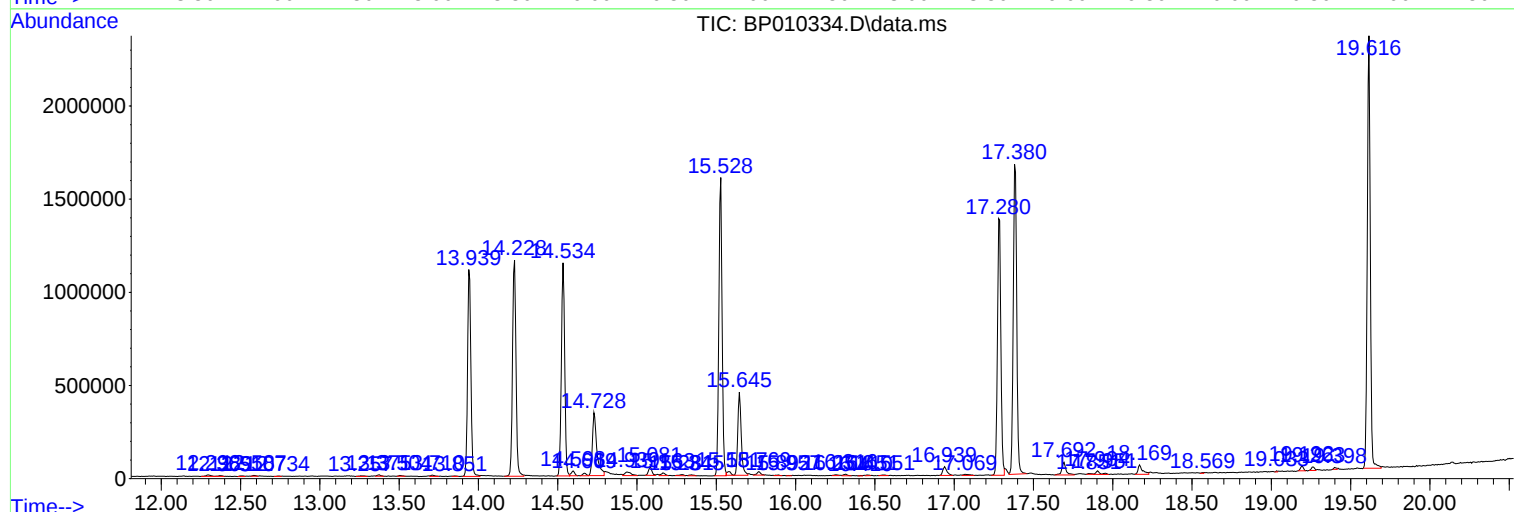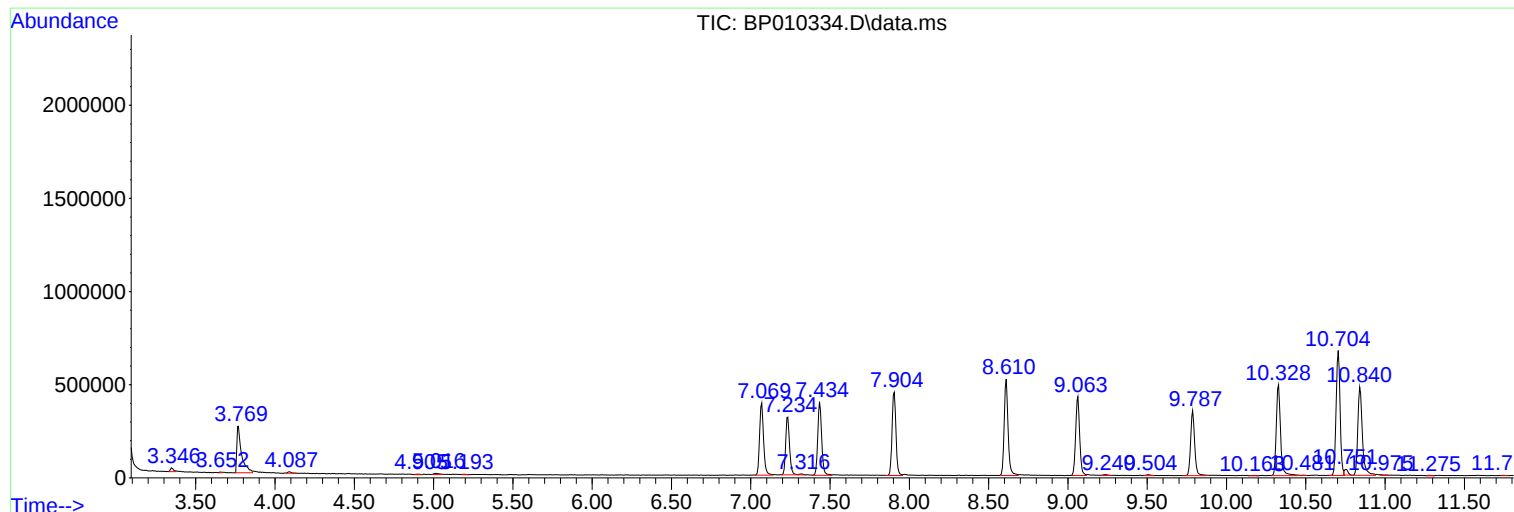

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010334.D
Acq On : 12 May 2022 21:23
Operator : CG/JU
Sample : N2746-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBSK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010334.D
Acq On : 12 May 2022 21:23
Operator : CG/JU
Sample : N2746-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBSK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc