

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010340.D
 Acq On : 13 May 2022 00:46
 Operator : CG/JU
 Sample : N2801-04
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010340.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	40	44	55	rVB	28474	53206	1.00%	0.114%
2	3.775	113	117	139	rBV	116399	266819	5.00%	0.571%
3	4.093	166	171	177	rBV	11046	21242	0.40%	0.045%
4	4.622	255	261	272	rBV	141538	244225	4.58%	0.522%
5	5.017	323	328	333	rBV3	5881	8907	0.17%	0.019%
6	7.069	670	677	692	rBV	129283	246895	4.63%	0.528%
7	7.228	696	704	717	rBV	545911	912971	17.11%	1.952%
8	7.322	717	720	724	rVB3	4309	6782	0.13%	0.015%
9	7.434	731	739	748	rBV	531488	879804	16.49%	1.881%
10	7.905	811	819	828	rBV	504514	854625	16.02%	1.827%
11	7.975	828	831	837	rVB6	7363	12158	0.23%	0.026%
12	8.610	932	939	952	rBV	415748	716963	13.44%	1.533%
13	9.057	1008	1015	1032	rBV	732581	1260961	23.63%	2.696%
14	9.505	1088	1091	1094	rBV3	6182	8006	0.15%	0.017%
15	9.787	1129	1139	1154	rBV	588011	1023012	19.17%	2.187%
16	10.328	1223	1231	1249	rBV	750024	1383062	25.92%	2.957%
17	10.704	1287	1295	1310	rBV	757446	1294478	24.26%	2.768%
18	10.840	1310	1318	1341	rBV	708001	1353643	25.37%	2.894%
19	12.140	1533	1539	1544	rBV5	9210	18034	0.34%	0.039%
20	12.299	1559	1566	1572	rBV3	13774	26670	0.50%	0.057%
21	12.763	1641	1645	1650	rBV7	3393	6707	0.13%	0.014%
22	13.087	1695	1700	1704	rBV8	5336	7267	0.14%	0.016%
23	13.163	1708	1713	1717	rBV7	6121	12033	0.23%	0.026%
24	13.369	1737	1748	1754	rBV	28835	46695	0.88%	0.100%
25	13.940	1839	1845	1857	rBV	1853368	2607969	48.88%	5.576%
26	14.022	1857	1859	1863	rVV5	10562	15596	0.29%	0.033%
27	14.063	1863	1866	1870	rVB6	7300	10847	0.20%	0.023%
28	14.140	1876	1879	1883	rBV5	4190	6543	0.12%	0.014%
29	14.222	1885	1893	1906	rBV	1867954	2888387	54.13%	6.176%
30	14.440	1925	1930	1938	rBV	48572	64639	1.21%	0.138%
31	14.534	1938	1946	1955	rBV	1194258	1845183	34.58%	3.945%
32	14.734	1975	1980	1993	rBV2	71715	180123	3.38%	0.385%
33	14.945	2012	2016	2021	rVB7	9455	13294	0.25%	0.028%
34	15.057	2031	2035	2039	rVB5	11640	16931	0.32%	0.036%
35	15.334	2079	2082	2084	rBV4	5543	7906	0.15%	0.017%
36	15.387	2087	2091	2097	rVB	75241	93215	1.75%	0.199%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010340.D
 Acq On : 13 May 2022 00:46
 Operator : CG/JU
 Sample : N2801-04
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

37	15.528	2108	2115	2127	rBV	2504728	3833741	71.85%	8.197%
38	15.645	2129	2135	2150	rVB	921391	1319267	24.72%	2.821%
39	15.769	2151	2156	2159	rBV2	35273	60325	1.13%	0.129%
40	15.951	2183	2187	2192	rVB6	8439	15068	0.28%	0.032%
41	16.010	2194	2197	2201	rVB5	11008	16131	0.30%	0.034%
42	16.251	2234	2238	2241	rBV	99000	134559	2.52%	0.288%
43	17.045	2369	2373	2377	rBV	84147	110603	2.07%	0.236%
44	17.104	2379	2383	2393	rVB	39616	72258	1.35%	0.155%
45	17.281	2407	2413	2423	rBV	1532233	2252488	42.21%	4.816%
46	17.381	2424	2430	2441	rVB	2998360	4367605	81.85%	9.339%
47	17.786	2495	2499	2504	rVB	84574	105706	1.98%	0.226%
48	17.957	2525	2528	2531	rVB4	30049	35470	0.66%	0.076%
49	18.169	2561	2564	2570	rBV4	26224	35743	0.67%	0.076%
50	18.457	2609	2613	2617	rBV	81348	87911	1.65%	0.188%
51	19.063	2713	2716	2722	rVB	65455	81858	1.53%	0.175%
52	19.192	2734	2738	2742	rBV2	42826	60850	1.14%	0.130%
53	19.263	2747	2750	2757	rVB	37669	64210	1.20%	0.137%
54	19.616	2804	2810	2817	rBV	4048441	5335798	100.00%	11.409%
55	20.139	2897	2899	2904	rVB2	40393	40845	0.77%	0.087%
56	21.075	3054	3058	3066	rBV2	137733	209308	3.92%	0.448%
57	21.363	3102	3107	3121	rBV	1889126	2559273	47.96%	5.472%
58	22.486	3295	3298	3303	rVB2	91251	126022	2.36%	0.269%
59	23.051	3390	3394	3398	rVB	111859	162073	3.04%	0.347%
60	23.639	3486	3494	3500	rBV2	2454943	4962364	93.00%	10.611%
61	23.792	3513	3520	3530	rVB2	1126352	2302496	43.15%	4.923%




Sum of corrected areas: 46767770

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010340.D
Acq On : 13 May 2022 00:46
Operator : CG/JU
Sample : N2801-04
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

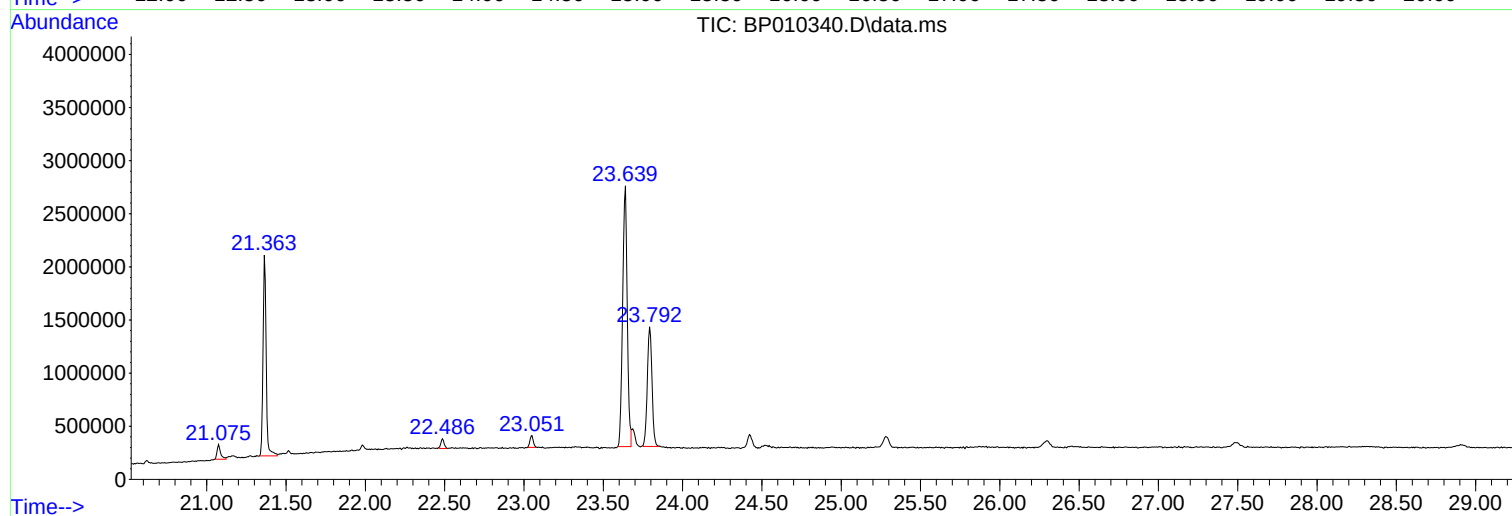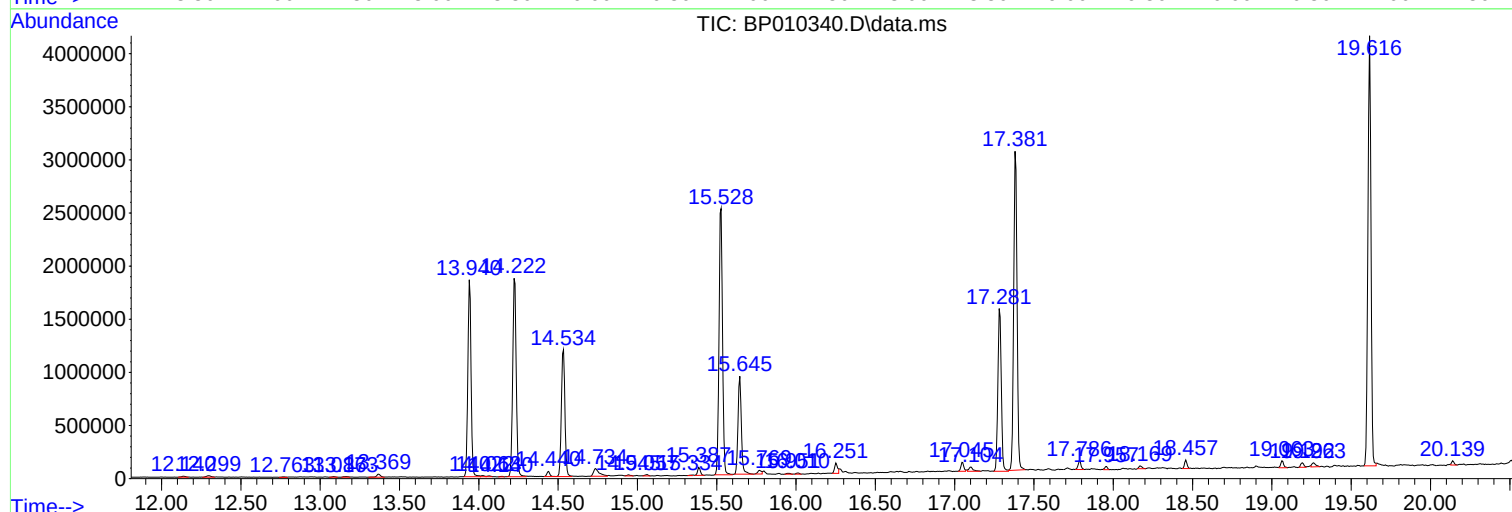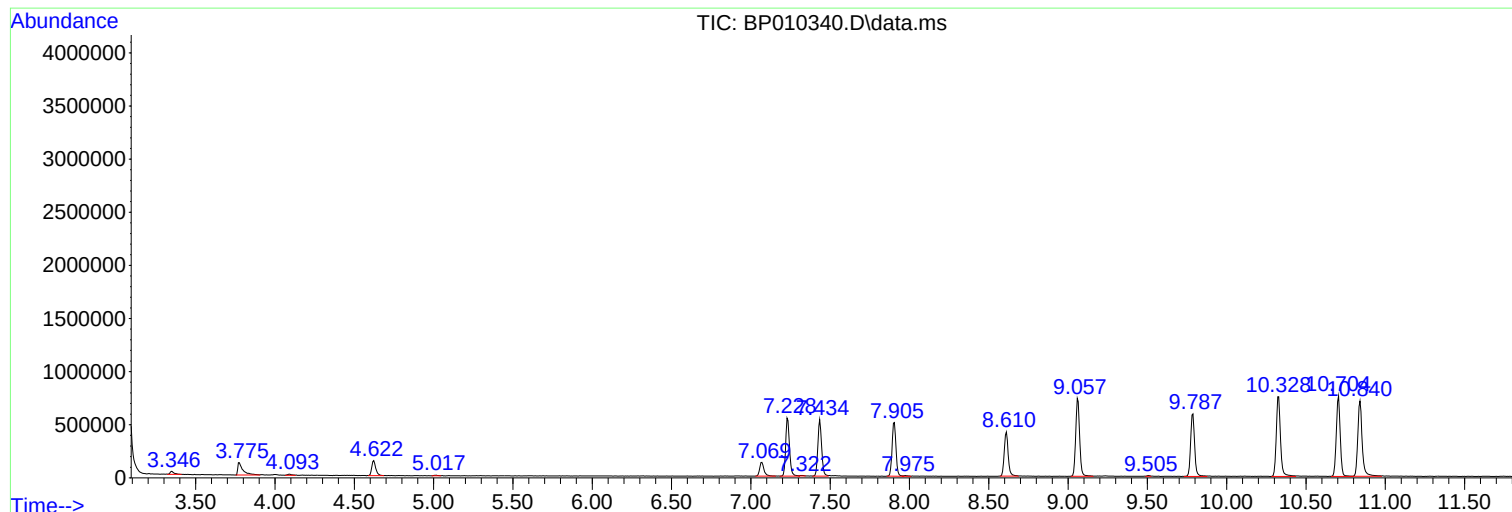

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010340.D
Acq On : 13 May 2022 00:46
Operator : CG/JU
Sample : N2801-04
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010340.D
Acq On : 13 May 2022 00:46
Operator : CG/JU
Sample : N2801-04
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc