

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010341.D
 Acq On : 13 May 2022 01:20
 Operator : CG/JU
 Sample : N2801-05
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	41	44	56	rVB2	29467	52886	0.99%	0.113%
2	3.770	113	116	132	rBV	141905	292828	5.49%	0.625%
3	4.005	152	156	160	rBV5	5969	9886	0.19%	0.021%
4	4.087	167	170	177	rVB2	11342	16061	0.30%	0.034%
5	4.622	256	261	268	rVB4	20871	33976	0.64%	0.073%
6	5.011	324	327	332	rBV2	6508	7474	0.14%	0.016%
7	7.069	669	677	688	rBV	138572	258157	4.84%	0.551%
8	7.228	697	704	717	rBV	561606	938575	17.59%	2.004%
9	7.434	731	739	750	rBV	571279	928202	17.40%	1.982%
10	7.540	753	757	761	rVB7	3956	6092	0.11%	0.013%
11	7.899	811	818	828	rBV	518396	892937	16.74%	1.907%
12	7.975	828	831	840	rVB	7403	14093	0.26%	0.030%
13	8.610	931	939	953	rBV	441739	768297	14.40%	1.641%
14	9.057	1007	1015	1033	rBV	750985	1319657	24.73%	2.818%
15	9.234	1041	1045	1051	rVB9	4457	7991	0.15%	0.017%
16	9.504	1084	1091	1100	rVB5	6505	15979	0.30%	0.034%
17	9.787	1130	1139	1154	rBV	610100	1054520	19.76%	2.252%
18	10.322	1223	1230	1250	rBV	775485	1427753	26.76%	3.049%
19	10.704	1286	1295	1309	rBV	775568	1357485	25.44%	2.899%
20	10.840	1309	1318	1337	rBV	767320	1443654	27.06%	3.083%
21	12.134	1534	1538	1543	rVB6	5223	7834	0.15%	0.017%
22	12.298	1558	1566	1575	rBV2	15540	33950	0.64%	0.072%
23	13.151	1707	1711	1716	rVB6	3969	5850	0.11%	0.012%
24	13.369	1743	1748	1754	rBV	20586	30677	0.57%	0.066%
25	13.940	1839	1845	1857	rBV	1815504	2649604	49.66%	5.658%
26	14.022	1857	1859	1863	rVB4	5210	6761	0.13%	0.014%
27	14.228	1882	1894	1905	rBV	1947745	2961193	55.50%	6.323%
28	14.440	1924	1930	1936	rVB	39032	49900	0.94%	0.107%
29	14.534	1938	1946	1960	rBV	1339105	1928044	36.13%	4.117%
30	14.734	1973	1980	1993	rBV	78226	199291	3.74%	0.426%
31	14.887	2003	2006	2012	rVB6	5326	10550	0.20%	0.023%
32	14.945	2012	2016	2021	rVB8	5199	11330	0.21%	0.024%
33	15.057	2030	2035	2042	rVB7	10023	15786	0.30%	0.034%
34	15.128	2042	2047	2049	rBV6	5098	7056	0.13%	0.015%
35	15.339	2079	2083	2087	rBV6	7222	13769	0.26%	0.029%
36	15.387	2087	2091	2098	rVB	65650	85168	1.60%	0.182%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
 Data File : BP010341.D
 Acq On : 13 May 2022 01:20
 Operator : CG/JU
 Sample : N2801-05
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXLB8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
 Title : SVOA CALIBRATION

37	15.528	2105	2115	2128	rBV	2609004	3897602	73.05%	8.323%
38	15.645	2129	2135	2150	rBV	921517	1301725	24.40%	2.780%
39	15.769	2150	2156	2159	rBV2	34288	58146	1.09%	0.124%
40	15.892	2175	2177	2182	rVB6	7613	8142	0.15%	0.017%
41	15.945	2182	2186	2191	rBV7	9356	15934	0.30%	0.034%
42	16.010	2193	2197	2205	rVB10	12029	20171	0.38%	0.043%
43	16.086	2209	2210	2217	rVB7	3762	6338	0.12%	0.014%
44	16.251	2234	2238	2242	rBV	86131	119774	2.24%	0.256%
45	16.357	2254	2256	2262	rVB7	3969	6981	0.13%	0.015%
46	16.604	2293	2298	2299	rBV5	9134	13514	0.25%	0.029%
47	16.657	2305	2307	2312	rVB5	7033	8274	0.16%	0.018%
48	16.757	2322	2324	2328	rBV4	7002	9262	0.17%	0.020%
49	16.963	2356	2359	2361	rVB4	6230	6532	0.12%	0.014%
50	17.045	2369	2373	2379	rBV	76545	107279	2.01%	0.229%
51	17.104	2379	2383	2387	rVB2	25790	35637	0.67%	0.076%
52	17.281	2407	2413	2422	rBV	1618312	2374367	44.50%	5.070%
53	17.381	2423	2430	2444	rVV2	2892564	4410007	82.65%	9.417%
54	17.475	2444	2446	2451	rVB6	7865	9934	0.19%	0.021%
55	17.592	2461	2466	2468	rBV6	8827	13339	0.25%	0.028%
56	17.786	2495	2499	2504	rBV	71981	86676	1.62%	0.185%
57	17.957	2524	2528	2533	rVB2	33778	42109	0.79%	0.090%
58	18.063	2543	2546	2550	rBV6	6446	10294	0.19%	0.022%
59	18.169	2560	2564	2568	rBV4	24012	37613	0.70%	0.080%
60	18.457	2609	2613	2618	rBV	59682	72020	1.35%	0.154%
61	19.063	2713	2716	2721	rBV	49325	62299	1.17%	0.133%
62	19.192	2734	2738	2745	rBV3	42824	61749	1.16%	0.132%
63	19.263	2746	2750	2754	rBV	35548	53847	1.01%	0.115%
64	19.398	2770	2773	2775	rBV4	10469	13494	0.25%	0.029%
65	19.539	2795	2797	2802	rBV6	8780	8440	0.16%	0.018%
66	19.616	2803	2810	2824	rBV	3911164	5335727	100.00%	11.394%
67	20.139	2896	2899	2903	rVB	28678	28810	0.54%	0.062%
68	21.074	3054	3058	3062	rBV	90688	126645	2.37%	0.270%
69	21.363	3102	3107	3120	rBV	1924830	2678512	50.20%	5.720%
70	23.633	3486	3493	3500	rBV2	2222394	4529237	84.89%	9.672%
71	23.792	3513	3520	3537	rVB2	1133477	2396889	44.92%	5.118%


Sum of corrected areas: 46830585

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010341.D
Acq On : 13 May 2022 01:20
Operator : CG/JU
Sample : N2801-05
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

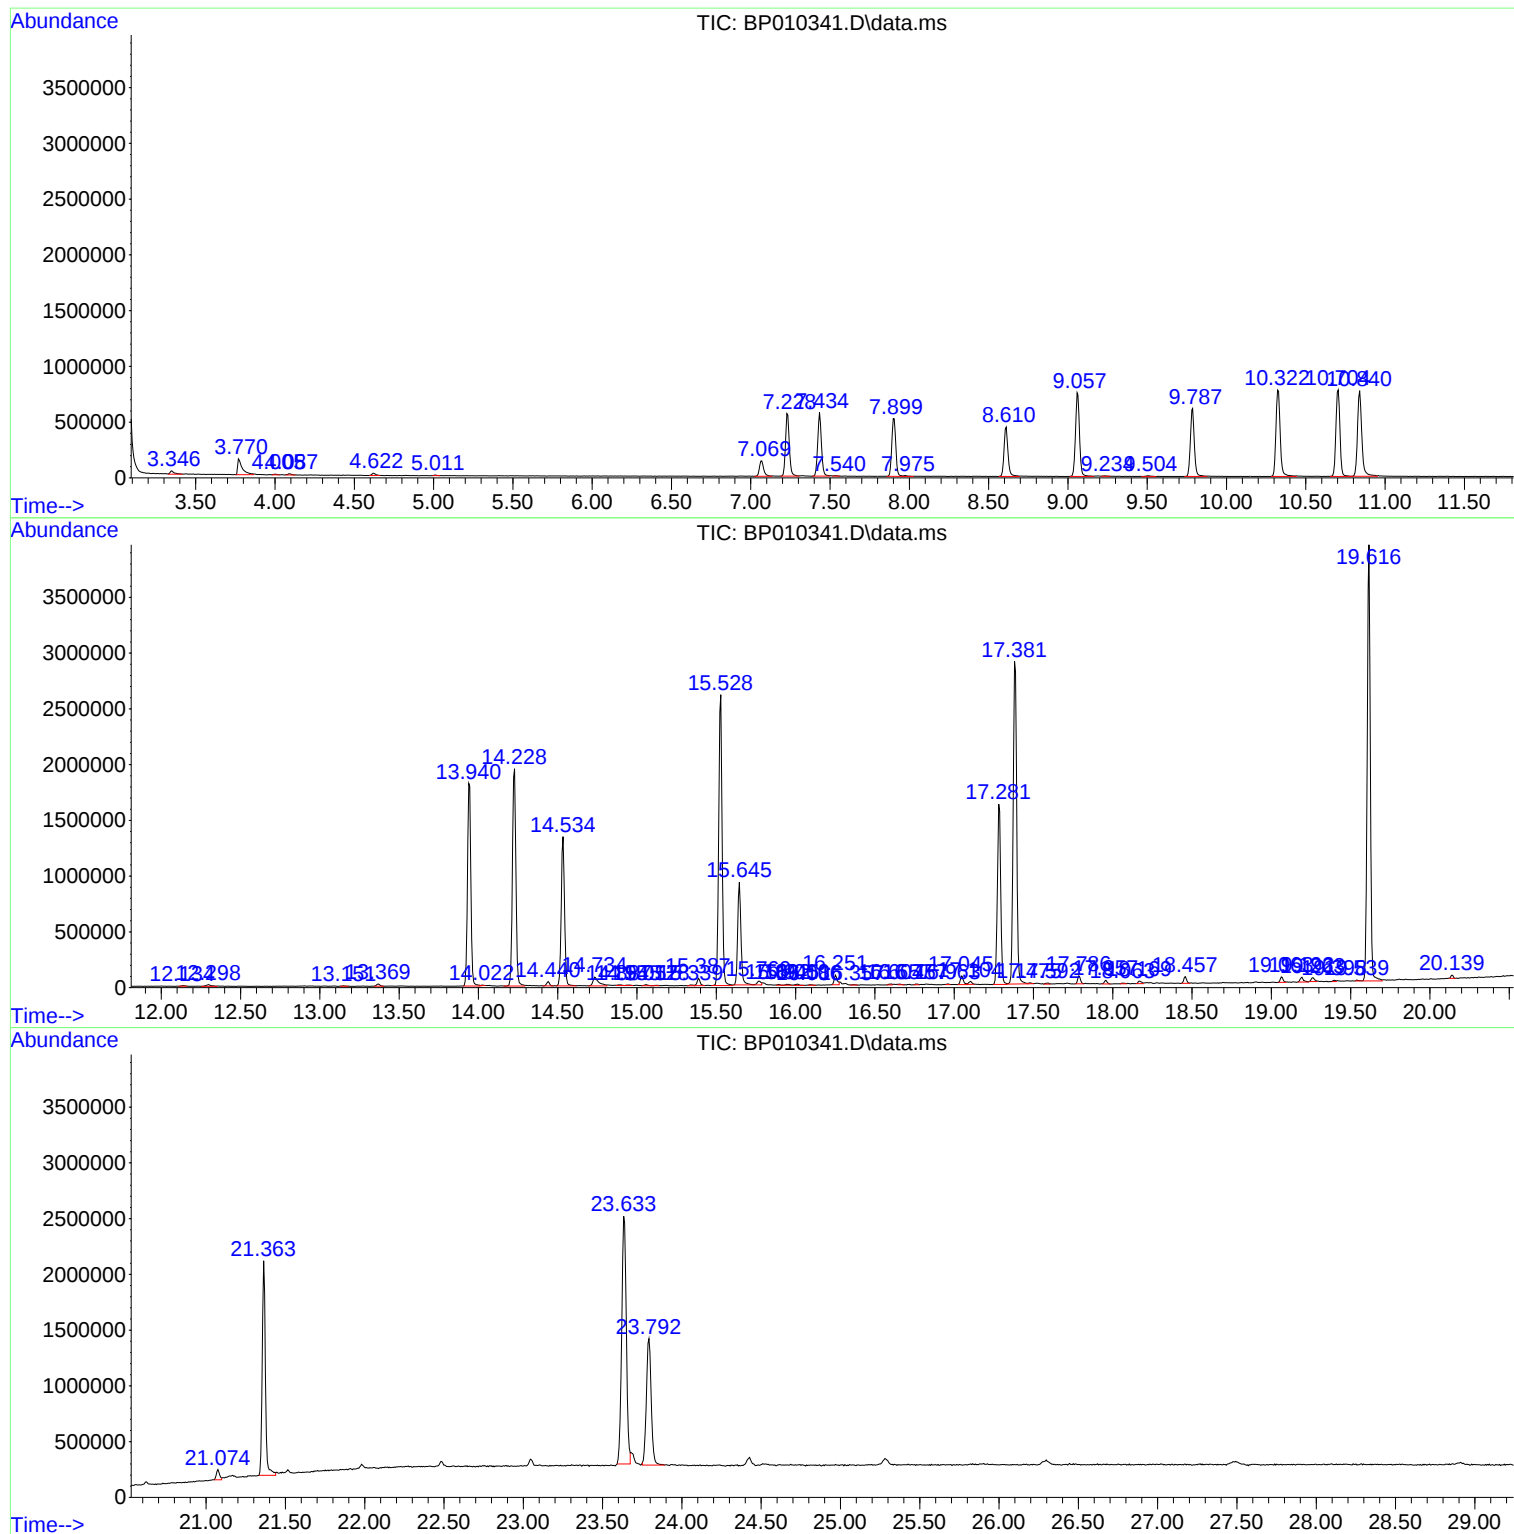

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010341.D
Acq On : 13 May 2022 01:20
Operator : CG/JU
Sample : N2801-05
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051122\
Data File : BP010341.D
Acq On : 13 May 2022 01:20
Operator : CG/JU
Sample : N2801-05
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXLB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------