
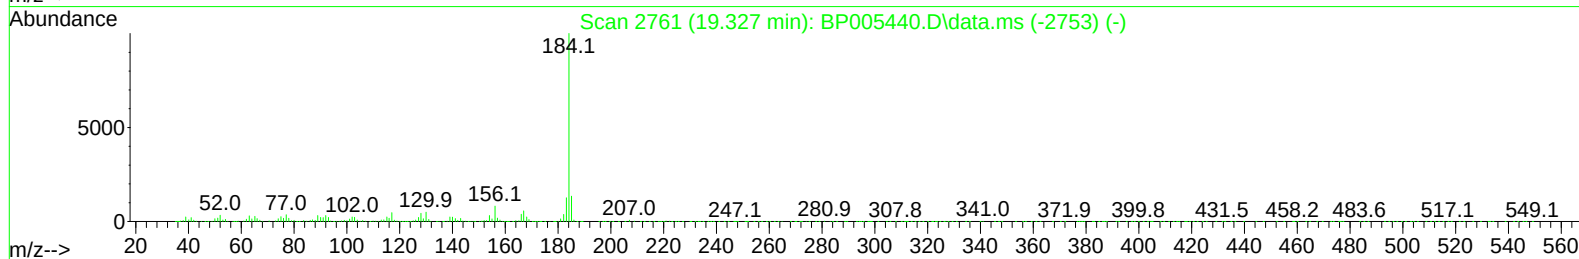
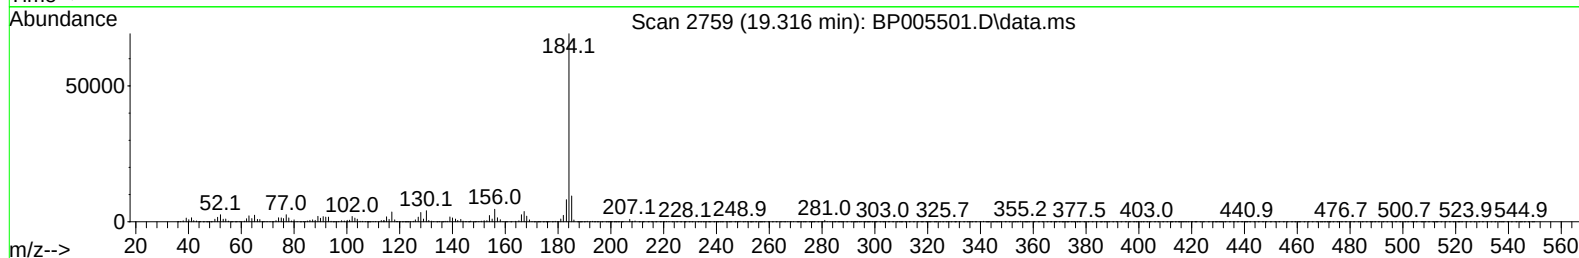


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051221\
Data File : BP005501.D
Acq On : 12 May 2021 13:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 13:58:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 11 11:20:59 2021
Response via : Initial Calibration

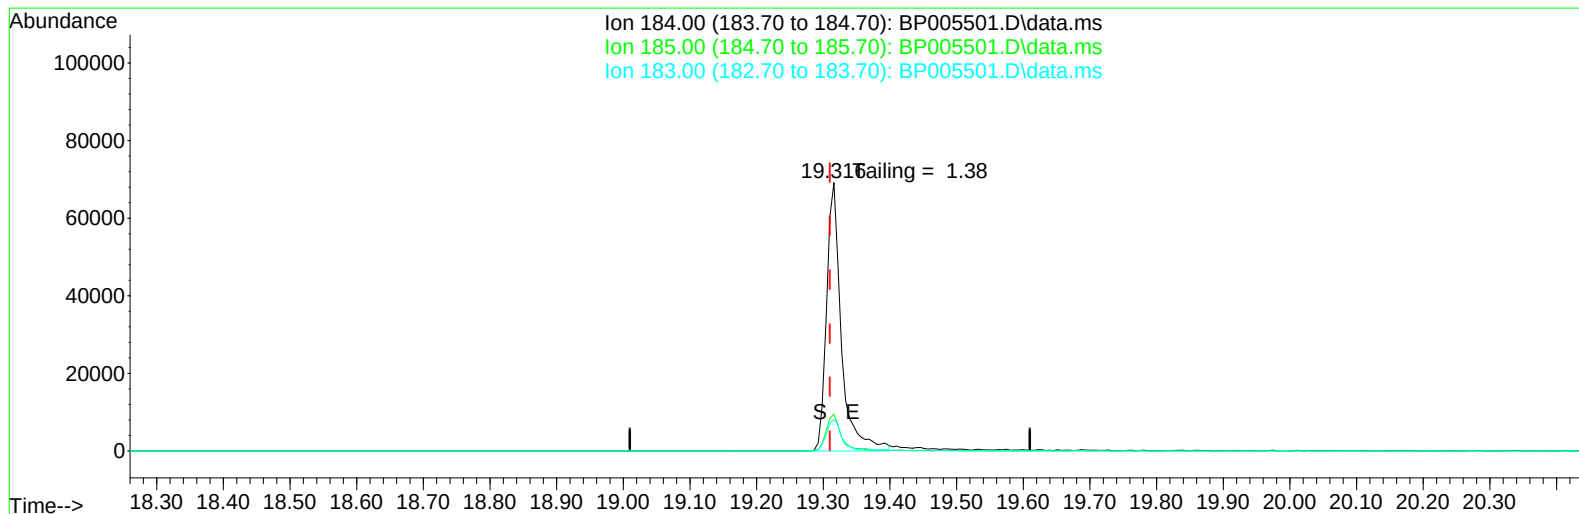

TIC: BP005501.D\data.ms

(77) Benzidine




19.316min (+ 0.006) 251745.45 ng

response 109108

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.73
183.00	12.30	11.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051221\
Data File : BP005501.D
Acq On : 12 May 2021 13:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 13:58:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 11 11:20:59 2021
Response via : Initial Calibration

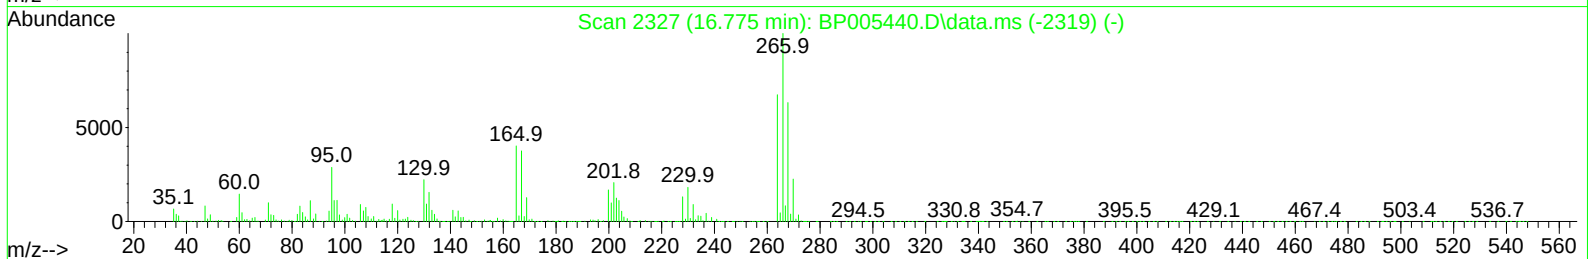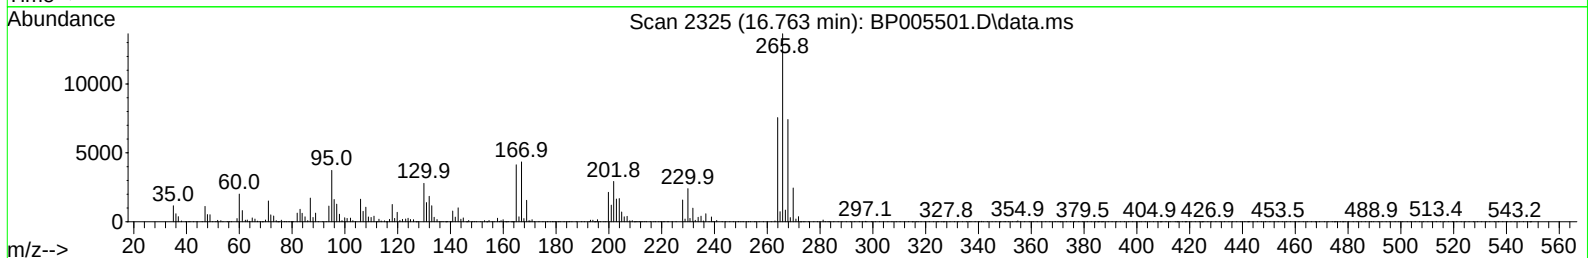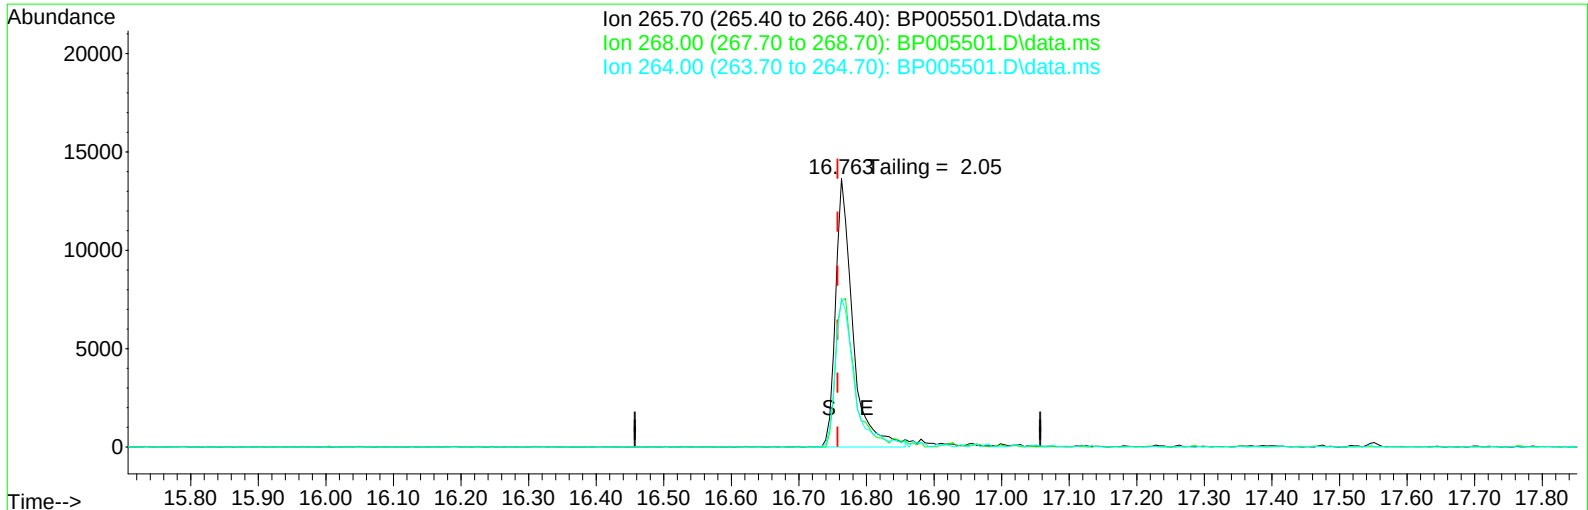

TIC: BP005501.D\data.ms

(70) Pentachlorophenol (C)

16.763min (+ 0.006) 188967.87 ng

response 23818

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	56.61
264.00	67.10	55.37
0.00	0.00	0.00