

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051221\
 Data File : BP005518.D
 Acq On : 12 May 2021 23:04
 Operator : CG/JU
 Sample : M2365-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MW-1

Quant Time: May 13 03:28:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 11 11:20:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.687	152	13277	20.00	ng	-0.01
21) Naphthalene-d8	10.481	136	34119	20.00	ng	#-0.01
39) Acenaphthene-d10	14.339	164	27580	20.00	ng	0.00
64) Phenanthrene-d10	17.098	188	69315	20.00	ng	# 0.00
76) Chrysene-d12	21.192	240	90470	20.00	ng	# 0.00
86) Perylene-d12	23.503	264	115073	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.287	112	47454	68.59	ng	0.00
7) Phenol-d6	6.887	99	22520	26.10	ng	0.00
23) Nitrobenzene-d5	8.857	82	93557	107.93	ng	0.00
42) 2,4,6-Tribromophenol	15.839	330	86792	110.90	ng	0.00
45) 2-Fluorobiphenyl	12.963	172	208756	85.38	ng	0.00
79) Terphenyl-d14	19.668	244	362669	68.08	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.810	163	12916	5.43	ng	Qvalue # 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051221\
Data File : BP005518.D
Acq On : 12 May 2021 23:04
Operator : CG/JU
Sample : M2365-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-1

Quant Time: May 13 03:28:55 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 11 11:20:59 2021
Response via : Initial Calibration




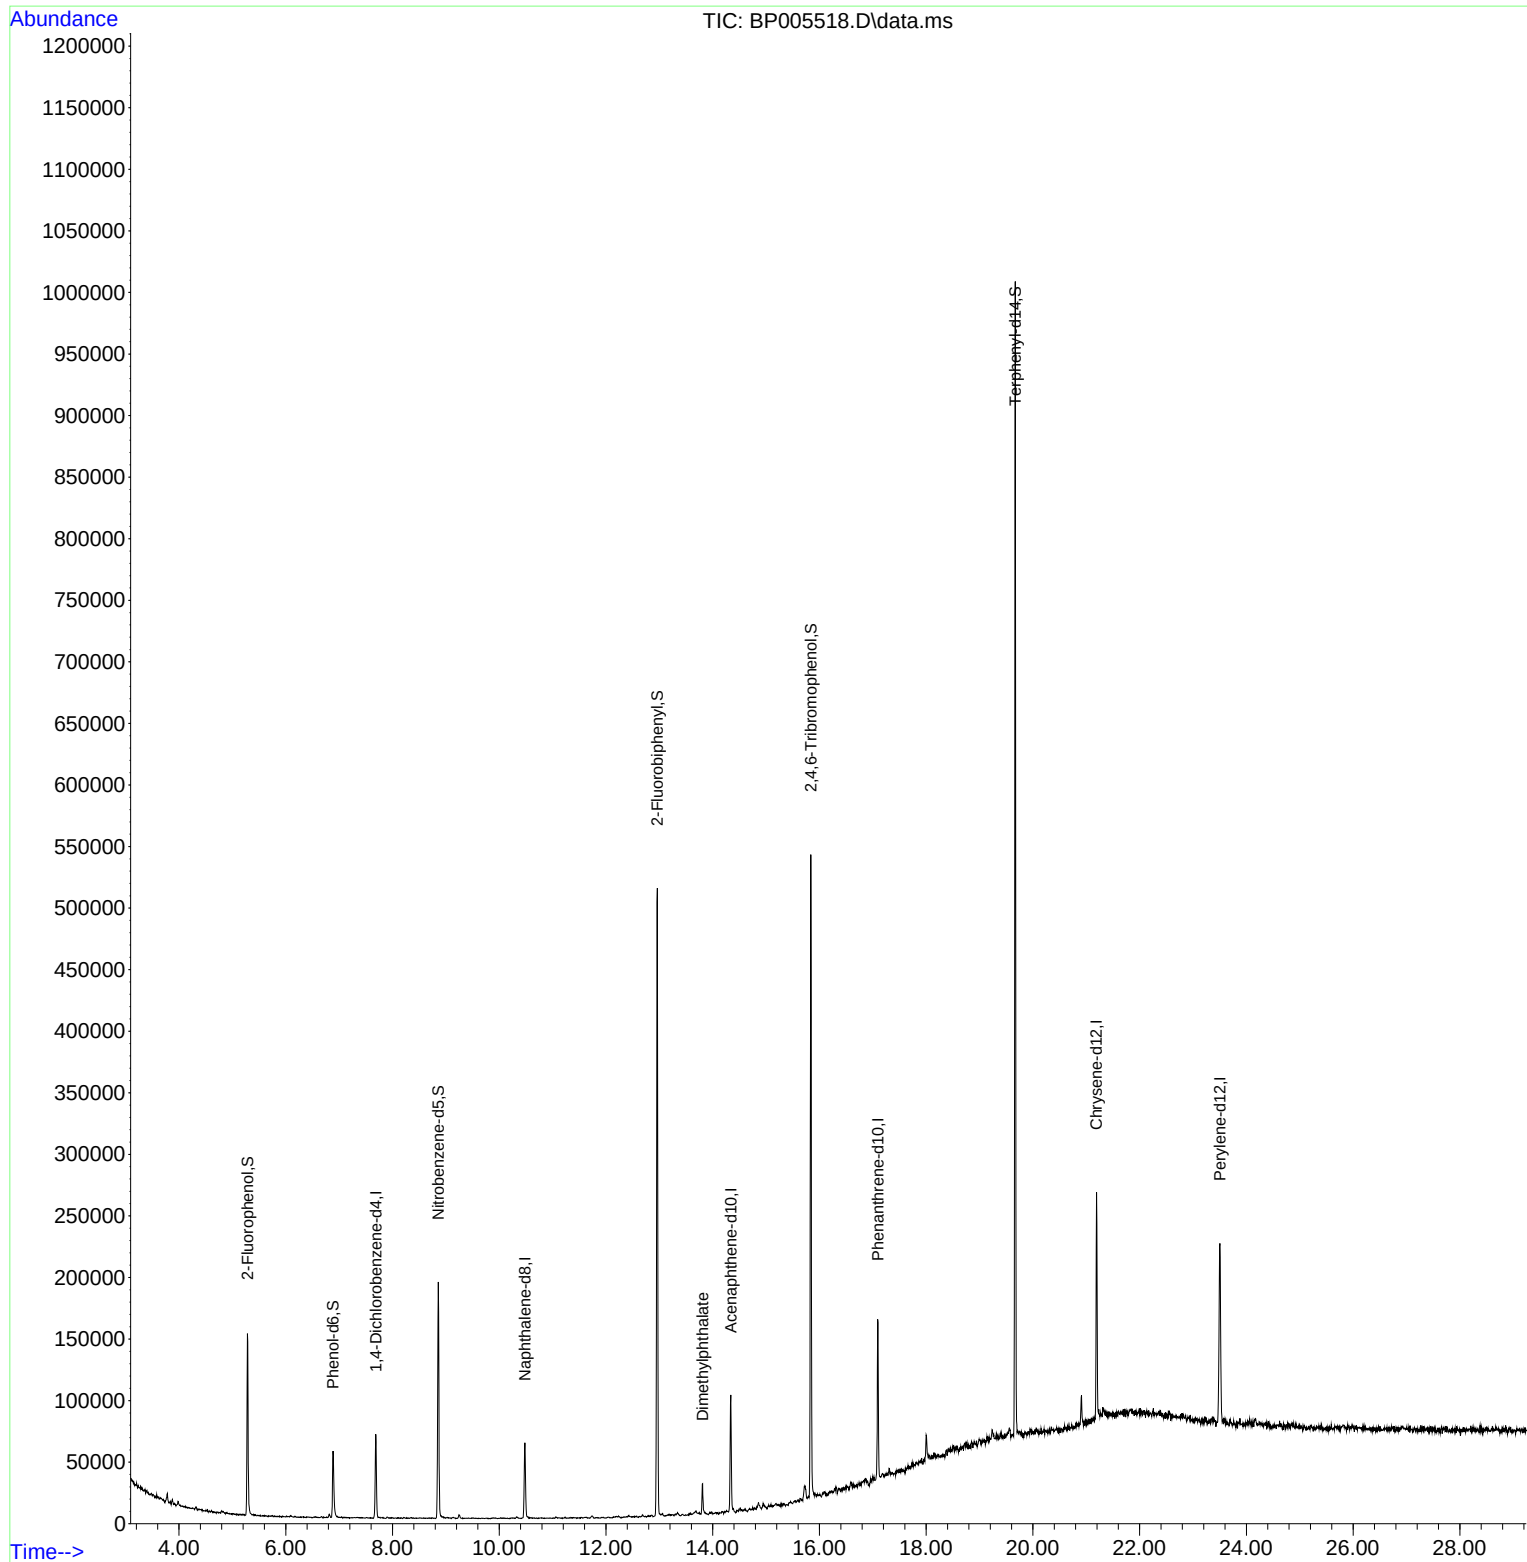




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.687 min Scan# 782
Delta R.T. -0.012 min
Lab File: BP005518.D
Acq: 12 May 2021 23:04




Instrument :
BNA_P
ClientSampleId :
MW-1


Tgt Ion:152 Resp: 13277
Ion Ratio Lower Upper
152 100
150 153.9 119.8 179.8
115 66.6 49.0 73.4

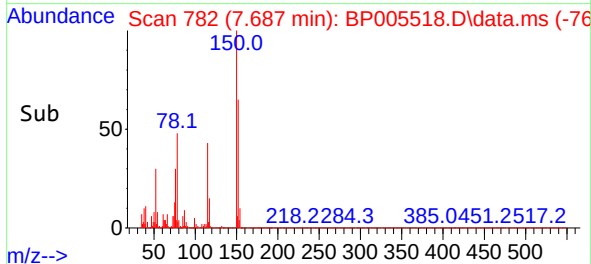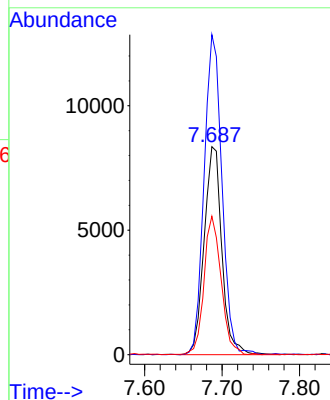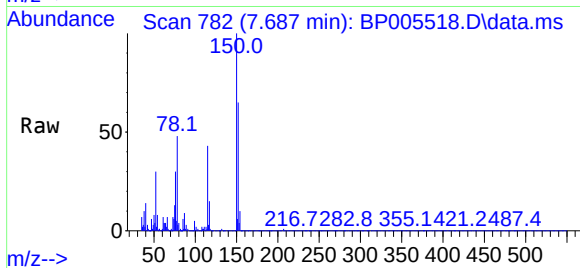

#5
2-Fluorophenol
Concen: 68.59 ng
RT: 5.287 min Scan# 374
Delta R.T. -0.000 min
Lab File: BP005518.D
Acq: 12 May 2021 23:04

Tgt Ion:112 Resp: 47454
Ion Ratio Lower Upper
112 100
64 53.0 33.6 50.4#
63 42.2 18.6 27.8#


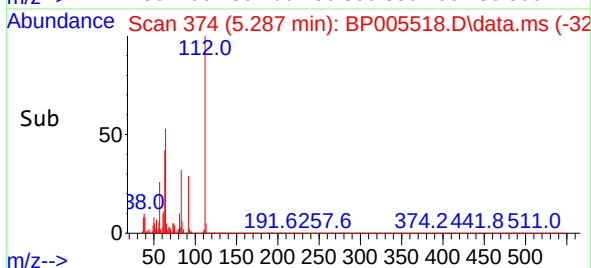
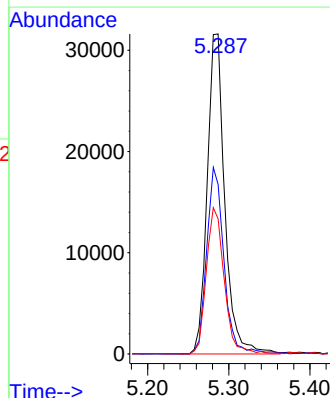
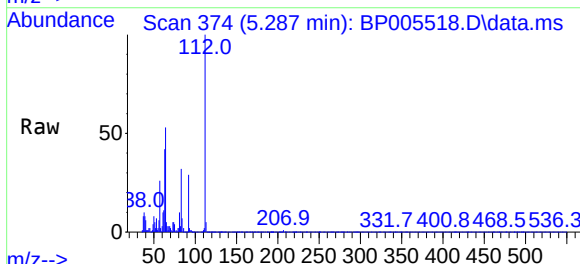


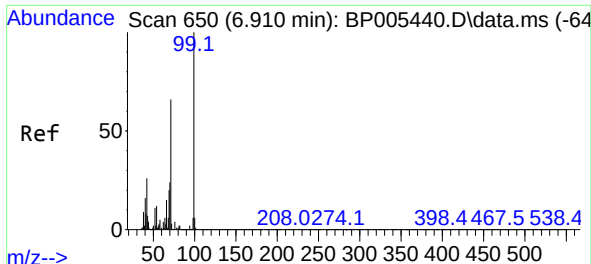

#7
Phenol-d6
Concen: 26.10 ng
RT: 6.887 min Scan# 646
Delta R.T. -0.006 min
Lab File: BP005518.D
Acq: 12 May 2021 23:04




Instrument :
BNA_P
ClientSampleId :
MW-1


Tgt Ion:	99	Resp:	22520
Ion	Ratio	Lower	Upper
99	100		
42	37.9	12.9	19.3#
71	74.6	26.7	40.1#

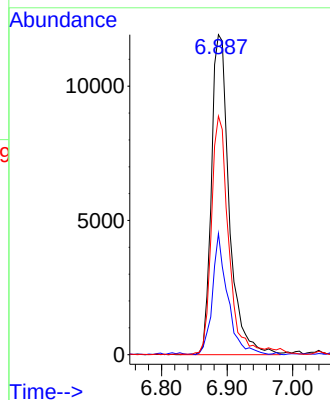

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.481 min Scan# 1257
Delta R.T. -0.012 min
Lab File: BP005518.D
Acq: 12 May 2021 23:04

Tgt Ion:	136	Resp:	34119
Ion	Ratio	Lower	Upper
136	100		
137	13.2	8.9	13.3
54	9.0	5.0	7.4#
68	2.3	3.7	5.5#


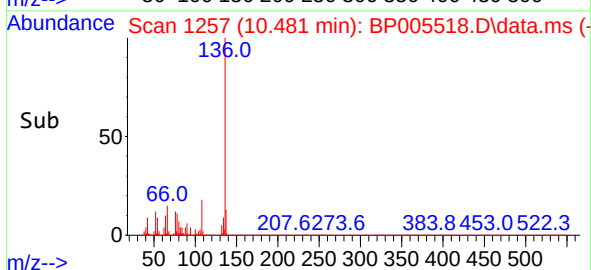
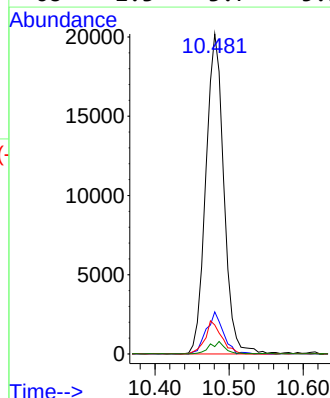
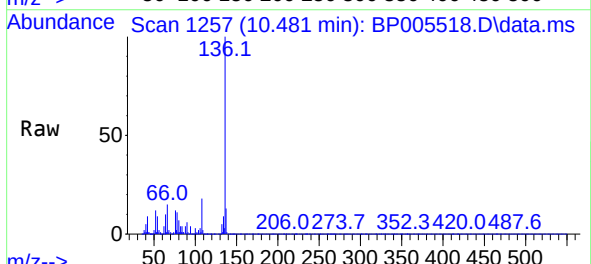


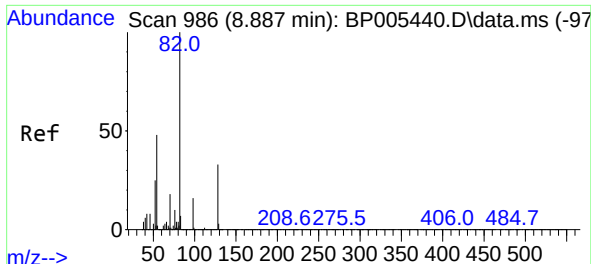

#23
Nitrobenzene-d5
Concen: 107.93 ng
RT: 8.857 min Scan# 981
Delta R.T. -0.006 min
Lab File: BP005518.D
Acq: 12 May 2021 23:04




Instrument :
BNA_P
ClientSampleId :
MW-1


Tgt Ion:	82	Resp:	93557
Ion	Ratio	Lower	Upper
82	100		
128	31.8	30.5	45.7
54	49.8	33.9	50.9

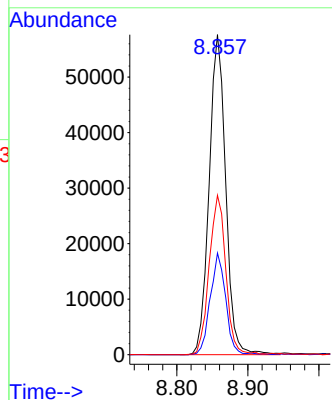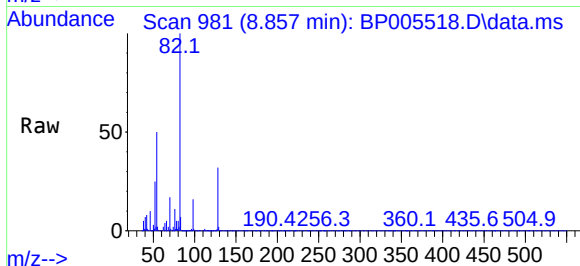

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.339 min Scan# 1913
Delta R.T. -0.000 min
Lab File: BP005518.D
Acq: 12 May 2021 23:04

Tgt Ion:	164	Resp:	27580
Ion	Ratio	Lower	Upper
164	100		
162	102.4	73.5	110.3
160	40.8	40.6	61.0


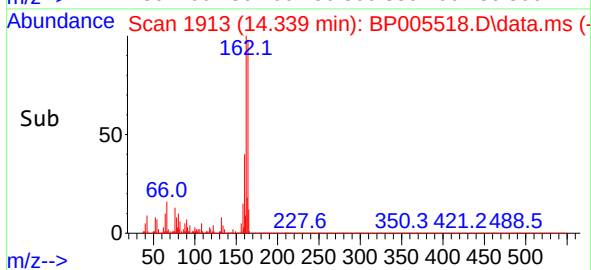
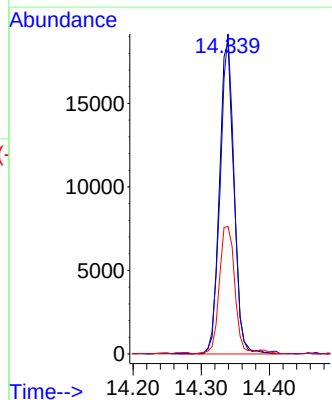
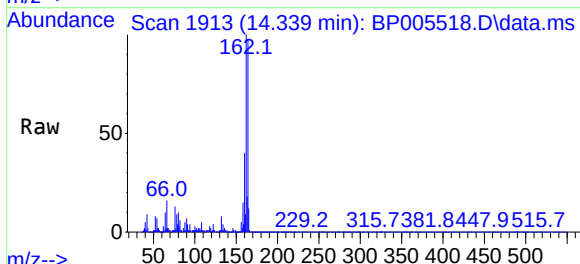


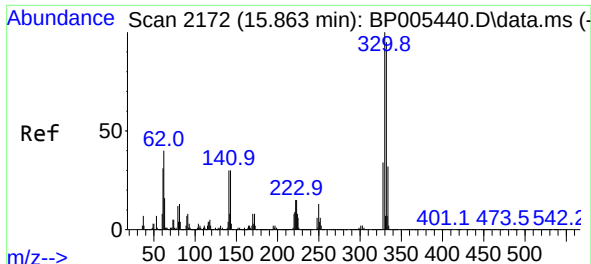

#42
2,4,6-Tribromophenol
Concen: 110.90 ng
RT: 15.839 min Scan# 2168
Delta R.T. -0.000 min
Lab File: BP005518.D
Acq: 12 May 2021 23:04




Instrument :
BNA_P
ClientSampleId :
MW-1


Tgt Ion:330 Resp: 86792
Ion Ratio Lower Upper
330 100
332 98.0 76.3 114.5
141 32.0 22.8 34.2

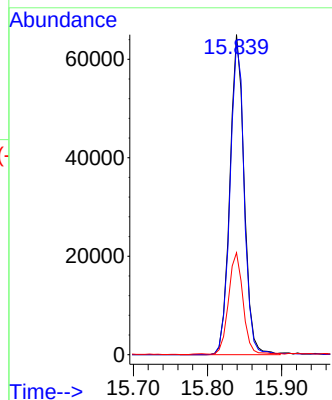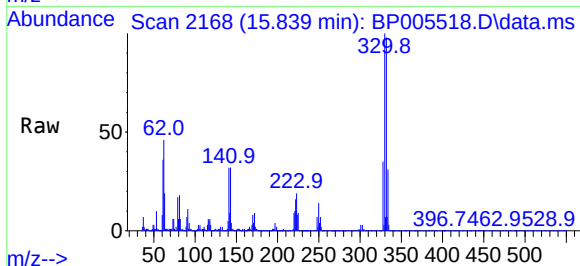

#45
2-Fluorobiphenyl
Concen: 85.38 ng
RT: 12.963 min Scan# 1679
Delta R.T. -0.006 min
Lab File: BP005518.D
Acq: 12 May 2021 23:04

Tgt Ion:172 Resp: 208756
Ion Ratio Lower Upper
172 100
171 35.5 28.1 42.1
170 23.9 19.6 29.4


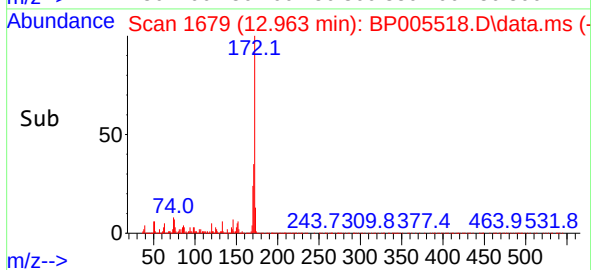
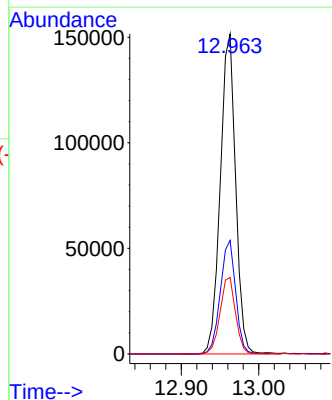
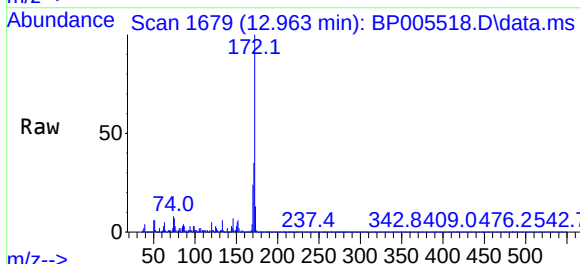




#50
Dimethylphthalate
Concen: 5.43 ng
RT: 13.810 min Scan# 1823
Delta R.T. -0.006 min
Lab File: BP005518.D
Acq: 12 May 2021 23:04




Instrument :
BNA_P
ClientSampleId :
MW-1


Tgt Ion:163 Resp: 12916
Ion Ratio Lower Upper
163 100
194 6.9 3.9 5.9#
164 10.0 8.1 12.1

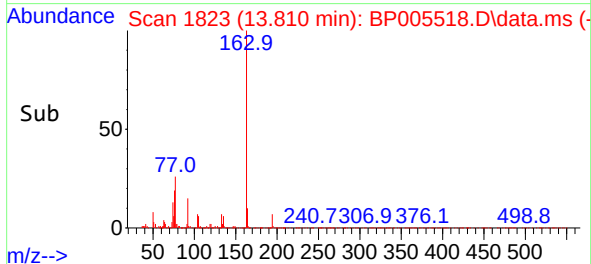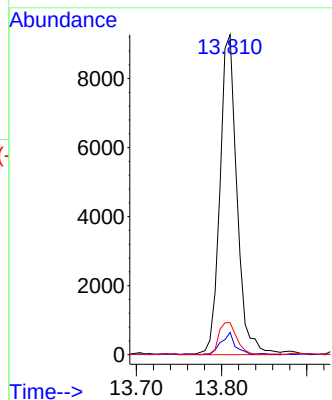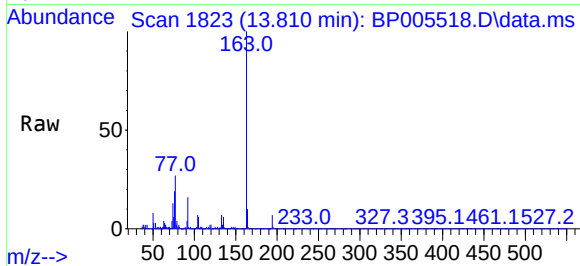

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.098 min Scan# 2382
Delta R.T. -0.000 min
Lab File: BP005518.D
Acq: 12 May 2021 23:04

Tgt Ion:188 Resp: 69315
Ion Ratio Lower Upper
188 100
94 3.8 5.0 7.6#
80 3.9 5.9 8.9#


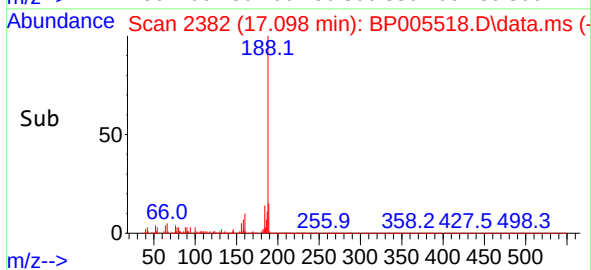
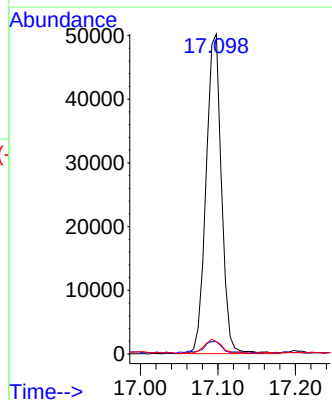
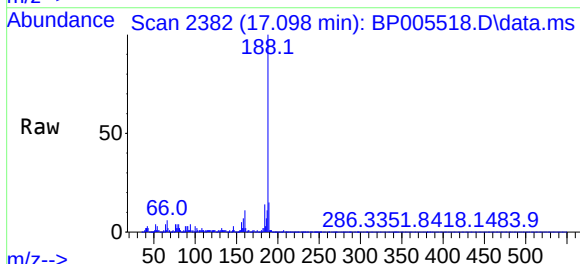




#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.192 min Scan# 3078
Delta R.T. -0.000 min
Lab File: BP005518.D
Acq: 12 May 2021 23:04




Instrument :
BNA_P
ClientSampleId :
MW-1


Tgt Ion:240 Resp: 90470
Ion Ratio Lower Upper
240 100
120 2.5 4.2 6.2#
236 27.4 20.2 30.2

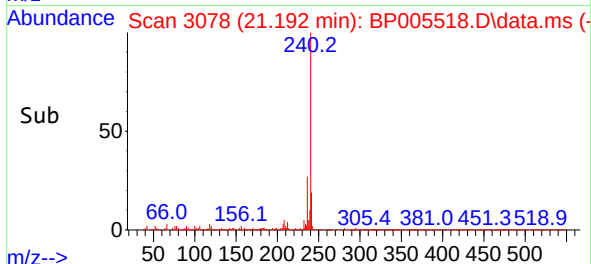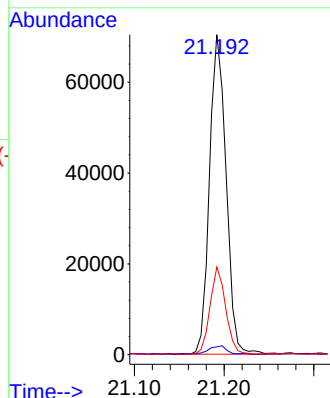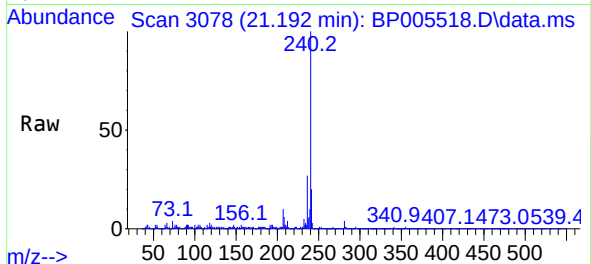

#79
Terphenyl-d14
Concen: 68.08 ng
RT: 19.668 min Scan# 2819
Delta R.T. -0.000 min
Lab File: BP005518.D
Acq: 12 May 2021 23:04

Tgt Ion:244 Resp: 362669
Ion Ratio Lower Upper
244 100
212 7.4 5.8 8.6
122 4.5 5.2 7.8#

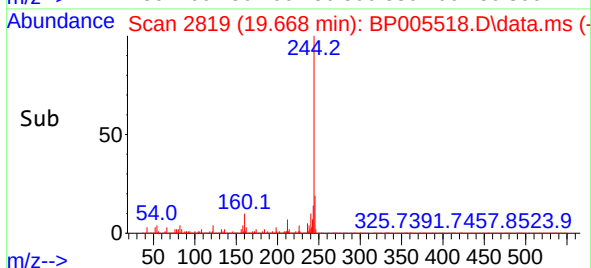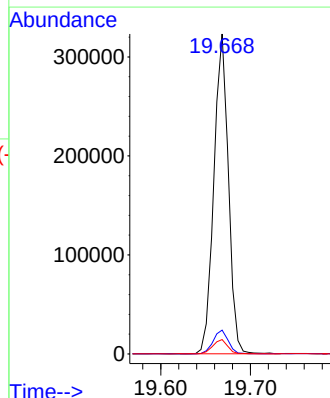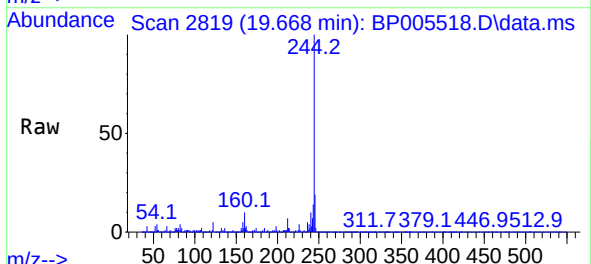

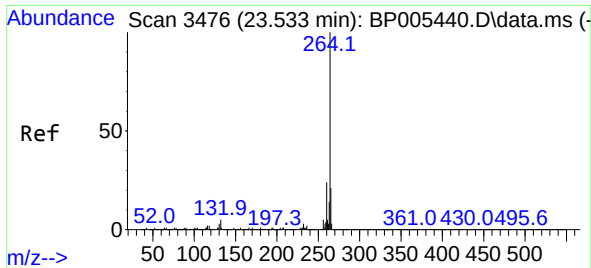

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.503 min Scan# 3471
Delta R.T. -0.000 min
Lab File: BP005518.D
Acq: 12 May 2021 23:04

Instrument :
BNA_P
ClientSampleId :
MW-1

Tgt Ion:264 Resp: 115073

Ion	Ratio	Lower	Upper
264	100		
260	24.3	20.6	30.8
265	21.5	19.0	28.6

