

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051221\
 Data File : BP005511.D
 Acq On : 12 May 2021 19:07
 Operator : CG/JU
 Sample : M2322-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EB-20210505

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.281	366	373	383	rBV	170806	252813	23.08%	7.066%
2	6.887	640	646	658	rBV	72706	128700	11.75%	3.597%
3	7.687	776	782	790	rVB	48287	76120	6.95%	2.127%
4	8.857	973	981	996	rBV	141272	234486	21.40%	6.554%
5	10.481	1250	1257	1267	rBV	40831	73966	6.75%	2.067%
6	12.963	1671	1679	1697	rBV	348592	509782	46.53%	14.248%
7	14.339	1907	1913	1922	rBV	58393	91350	8.34%	2.553%
8	15.839	2162	2168	2185	rBV	361001	527500	48.15%	14.743%
9	17.098	2376	2382	2390	rBV	83734	123303	11.25%	3.446%
10	19.669	2813	2819	2829	rBV	924220	1095547	100.00%	30.619%
11	20.910	3027	3030	3034	rBV5	13836	18198	1.66%	0.509%
12	21.198	3074	3079	3085	rBV	149763	192546	17.58%	5.381%
13	23.504	3466	3471	3485	rVB	120114	253676	23.16%	7.090%




Sum of corrected areas: 3577987

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051221\
Data File : BP005511.D
Acq On : 12 May 2021 19:07
Operator : CG/JU
Sample : M2322-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB-20210505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

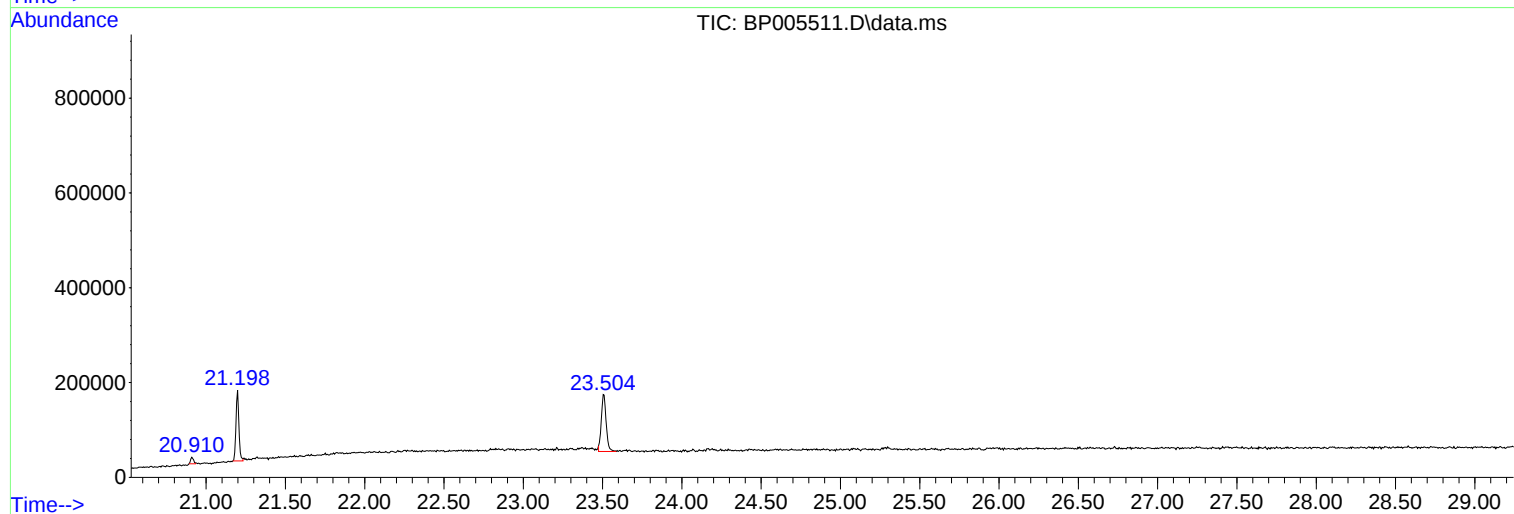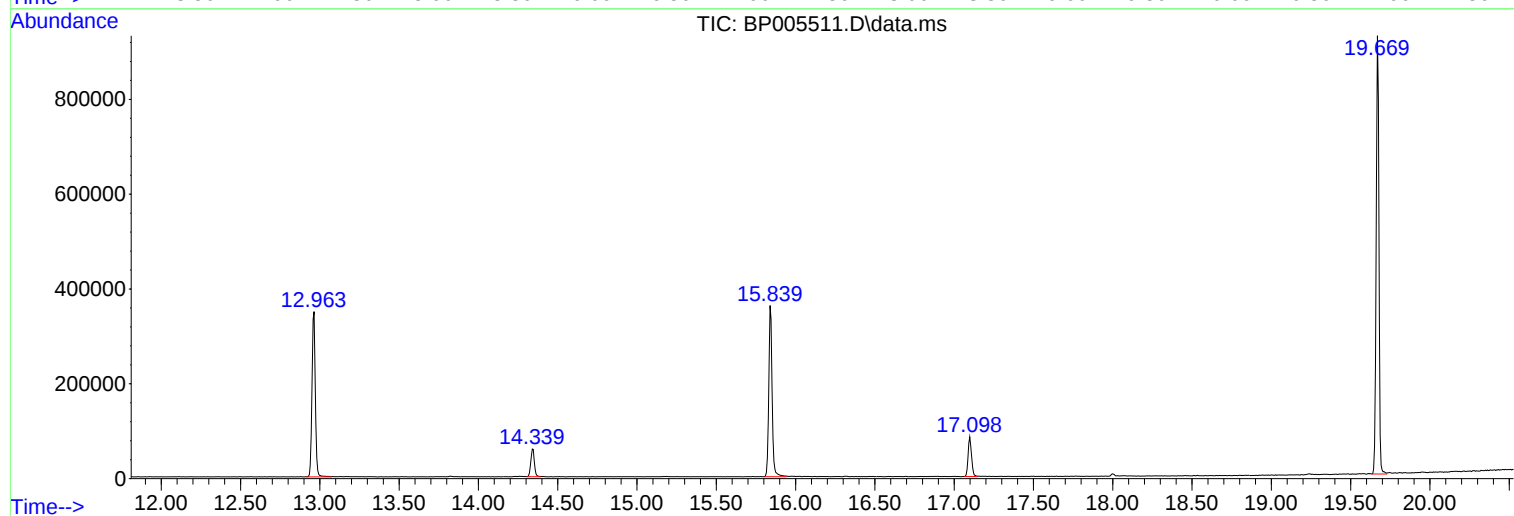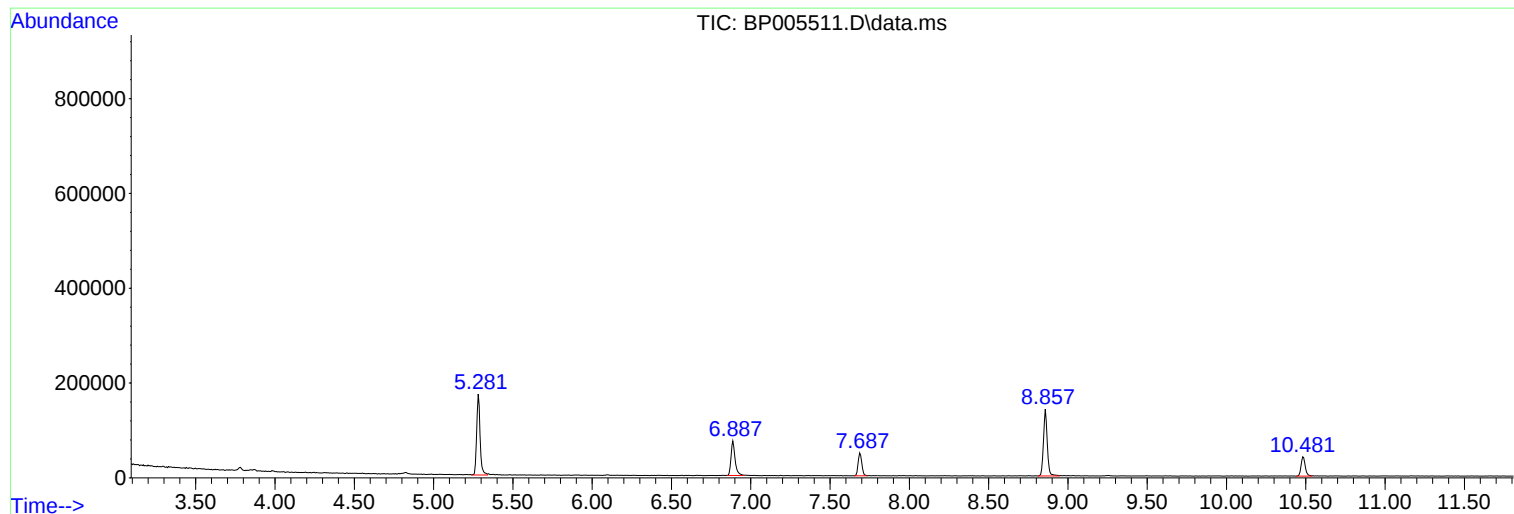

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051221\
Data File : BP005511.D
Acq On : 12 May 2021 19:07
Operator : CG/JU
Sample : M2322-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB-20210505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051221\
Data File : BP005511.D
Acq On : 12 May 2021 19:07
Operator : CG/JU
Sample : M2322-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB-20210505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
