

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051221\
 Data File : BP005520.D
 Acq On : 13 May 2021 00:11
 Operator : CG/JU
 Sample : M2356-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OR-03-051121

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.281	368	373	386	rVB	61744	95951	24.31%	3.813%
2	6.887	641	646	661	rBV	41176	77184	19.56%	3.067%
3	7.687	776	782	799	rBV	93716	148337	37.59%	5.895%
4	8.858	975	981	992	rBV	25402	47374	12.00%	1.883%
5	10.481	1250	1257	1265	rBV	89941	150597	38.16%	5.985%
6	12.957	1673	1678	1686	rBV	73229	107969	27.36%	4.291%
7	13.746	1807	1812	1816	rVB8	2791	4437	1.12%	0.176%
8	13.816	1817	1824	1828	rBV7	5770	9115	2.31%	0.362%
9	14.246	1890	1897	1900	rBV8	2935	5594	1.42%	0.222%
10	14.340	1907	1913	1920	rVV	133995	196518	49.80%	7.809%
11	14.398	1920	1923	1930	rVB6	4858	7336	1.86%	0.292%
12	14.745	1977	1982	1985	rBV7	3599	5114	1.30%	0.203%
13	15.128	2040	2047	2051	rBV10	1835	4640	1.18%	0.184%
14	15.398	2087	2093	2096	rBV4	4149	6576	1.67%	0.261%
15	15.604	2123	2128	2132	rBV8	3714	5012	1.27%	0.199%
16	15.693	2139	2143	2150	rVB9	2194	4003	1.01%	0.159%
17	15.840	2160	2168	2175	rBV	68892	104605	26.51%	4.157%
18	16.081	2203	2209	2213	rVB6	7690	13184	3.34%	0.524%
19	16.757	2320	2324	2329	rBV8	3041	4450	1.13%	0.177%
20	16.822	2331	2335	2338	rBV6	2157	4396	1.11%	0.175%
21	16.904	2345	2349	2360	rVB6	7181	17945	4.55%	0.713%
22	17.092	2376	2381	2385	rBV	175584	246868	62.56%	9.810%
23	17.139	2385	2389	2394	rVB	37062	53099	13.46%	2.110%
24	17.228	2401	2404	2410	rVB	14657	18354	4.65%	0.729%
25	17.969	2527	2530	2531	rBV3	5690	5541	1.40%	0.220%
26	18.092	2549	2551	2556	rBV6	4322	6097	1.55%	0.242%
27	18.157	2557	2562	2565	rBV2	13425	19580	4.96%	0.778%
28	18.451	2610	2612	2616	rVB5	5908	6480	1.64%	0.258%
29	18.863	2677	2682	2683	rBV4	7104	9941	2.52%	0.395%
30	19.116	2720	2725	2730	rBV	86682	110130	27.91%	4.376%
31	19.469	2776	2785	2788	rBV2	69841	127681	32.36%	5.074%
32	19.663	2814	2818	2822	rBV	158908	183060	46.39%	7.275%
33	21.192	3072	3078	3082	rBV2	282716	394623	100.00%	15.682%
34	23.504	3466	3471	3477	rVB	182506	314608	79.72%	12.502%

Sum of corrected areas: 2516399

Instrument :

BNA_P

ClientSampleId :




OR-03-051121

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051221\
Data File : BP005520.D
Acq On : 13 May 2021 00:11
Operator : CG/JU
Sample : M2356-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-03-051121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

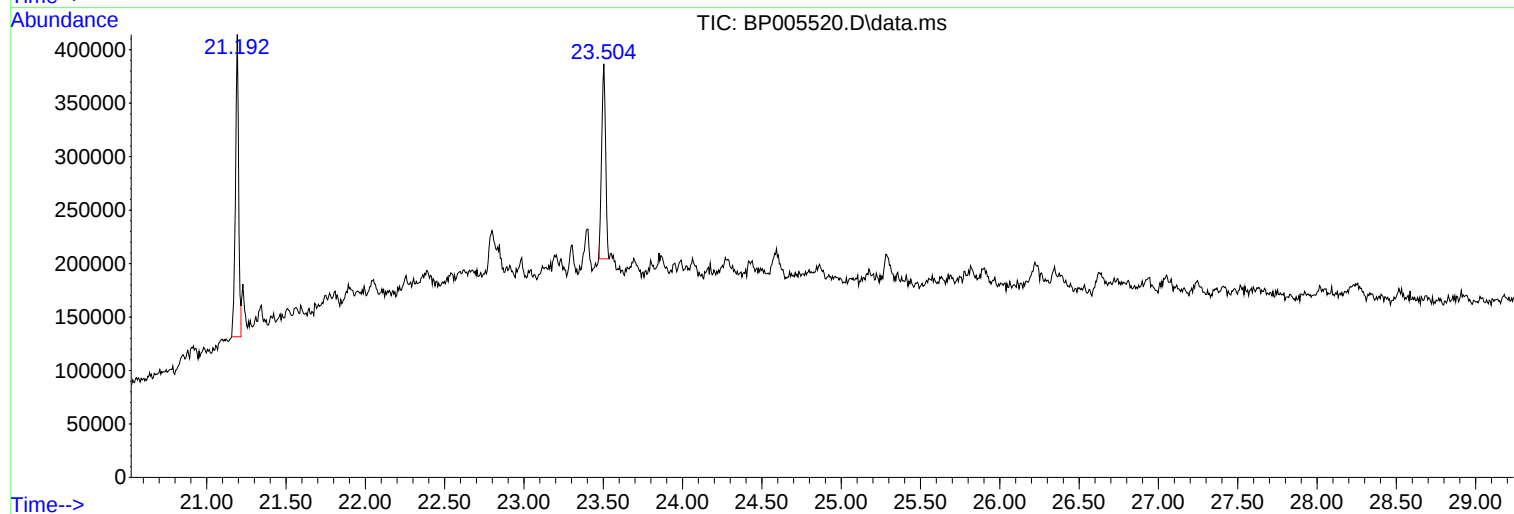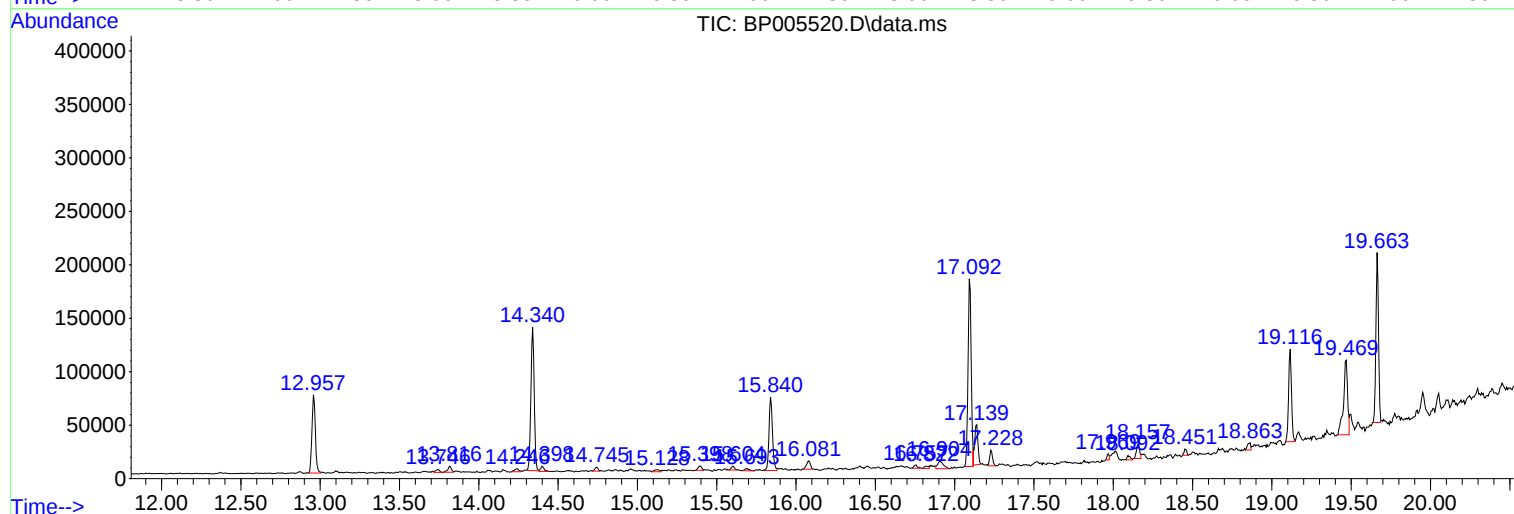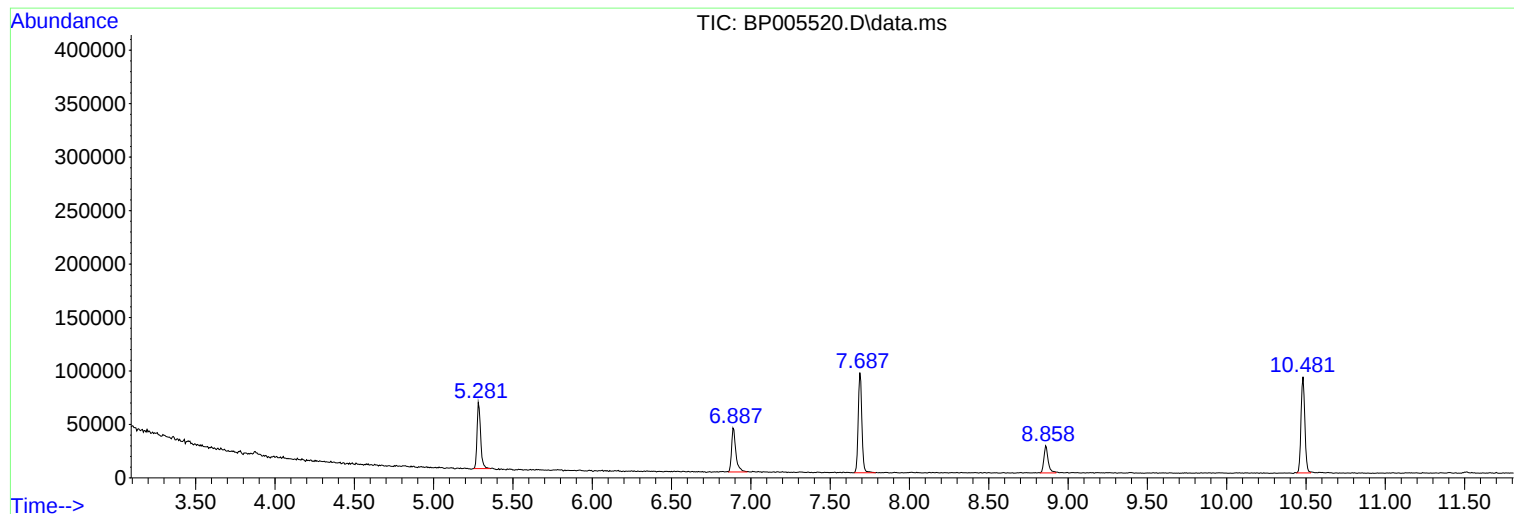

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051221\
Data File : BP005520.D
Acq On : 13 May 2021 00:11
Operator : CG/JU
Sample : M2356-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-03-051121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051221\
Data File : BP005520.D
Acq On : 13 May 2021 00:11
Operator : CG/JU
Sample : M2356-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-03-051121

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc