
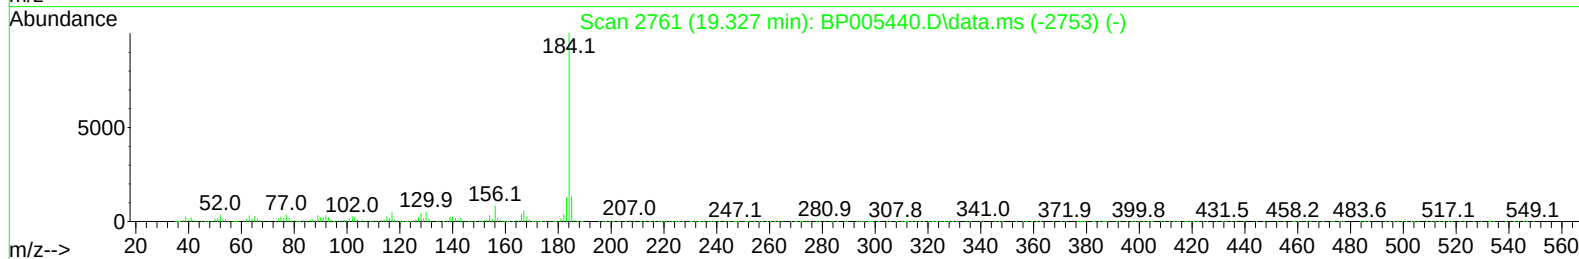
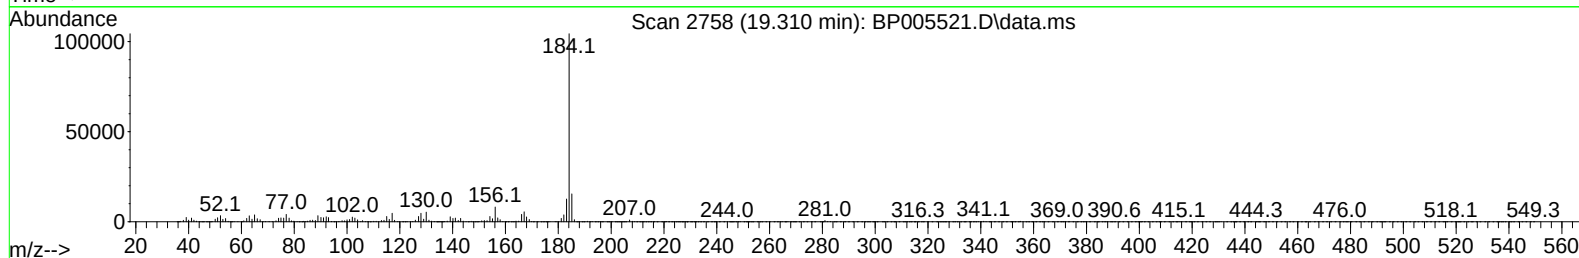


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051321\
 Data File : BP005521.D
 Acq On : 13 May 2021 15:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 16:15:02 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 11 11:20:59 2021
 Response via : Initial Calibration

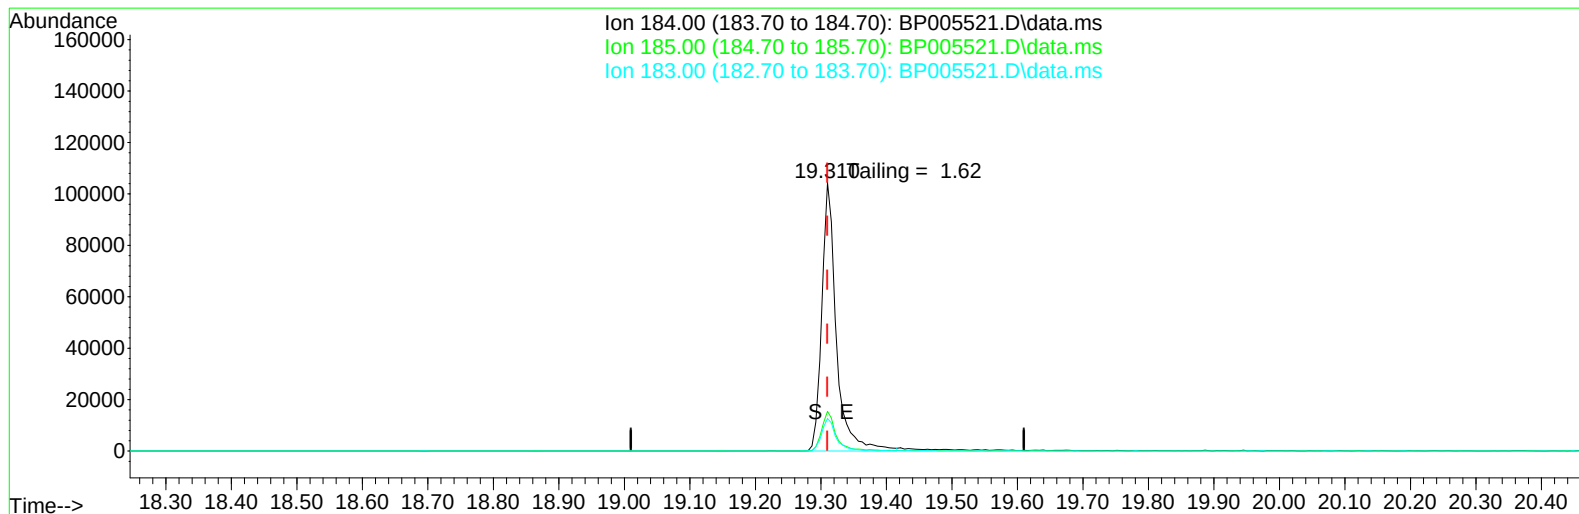

TIC: BP005521.D\data.ms

(77) Benzidine




19.310min (0.000) 109529.60 ng

response 162757

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.81
183.00	12.30	12.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051321\
Data File : BP005521.D
Acq On : 13 May 2021 15:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 16:15:02 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 11 11:20:59 2021
Response via : Initial Calibration

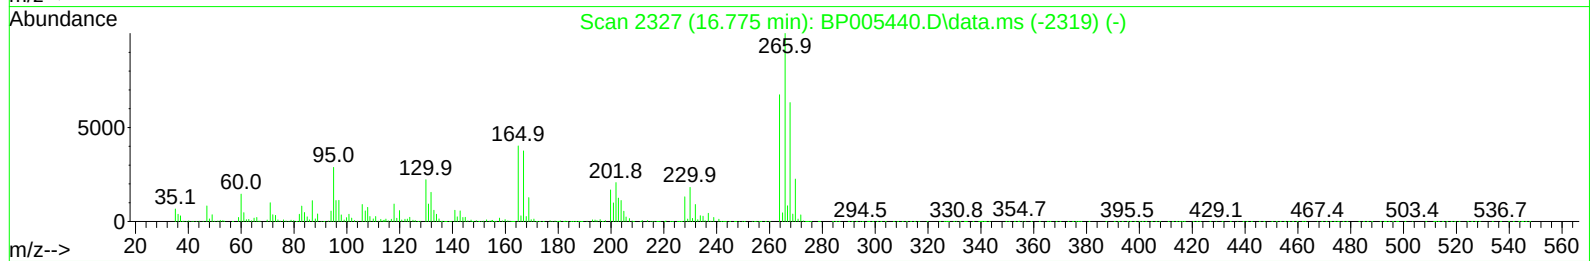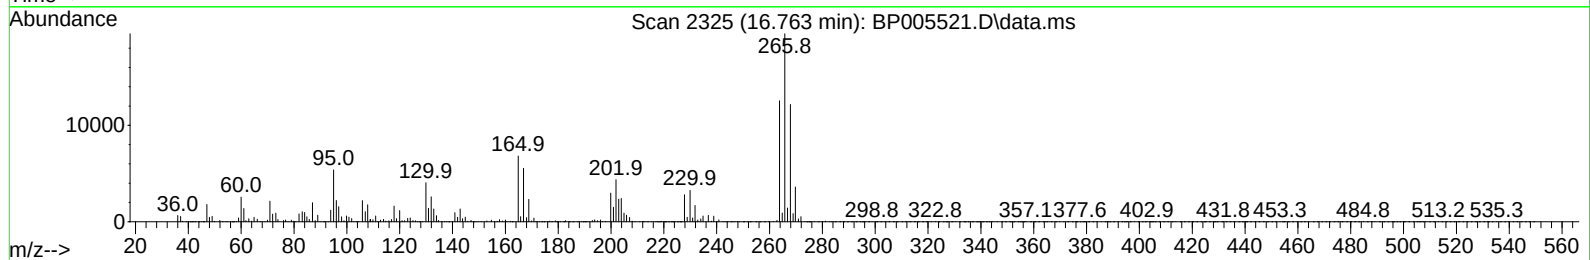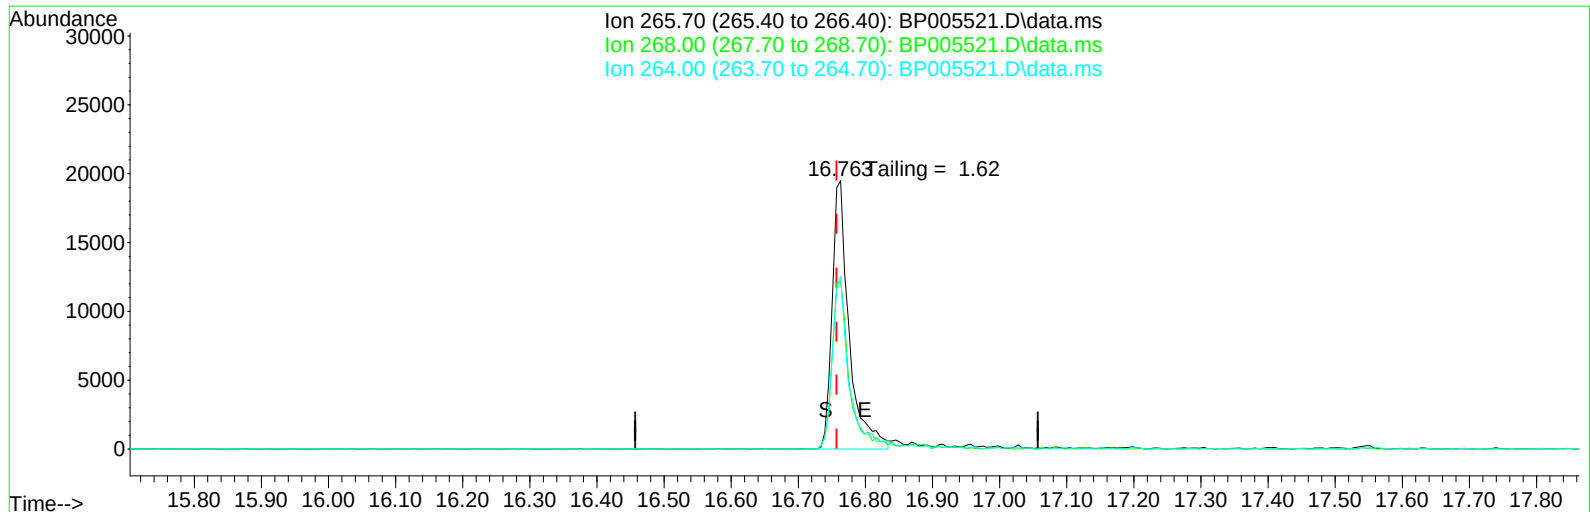

TIC: BP005521.D\data.ms

(70) Pentachlorophenol (C)

16.763min (+ 0.006) 670992.25 ng

response 35239

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	62.41
264.00	67.10	64.38
0.00	0.00	0.00