


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051321\
 Data File : BP005521.D
 Acq On : 13 May 2021 15:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 11 11:20:59 2021

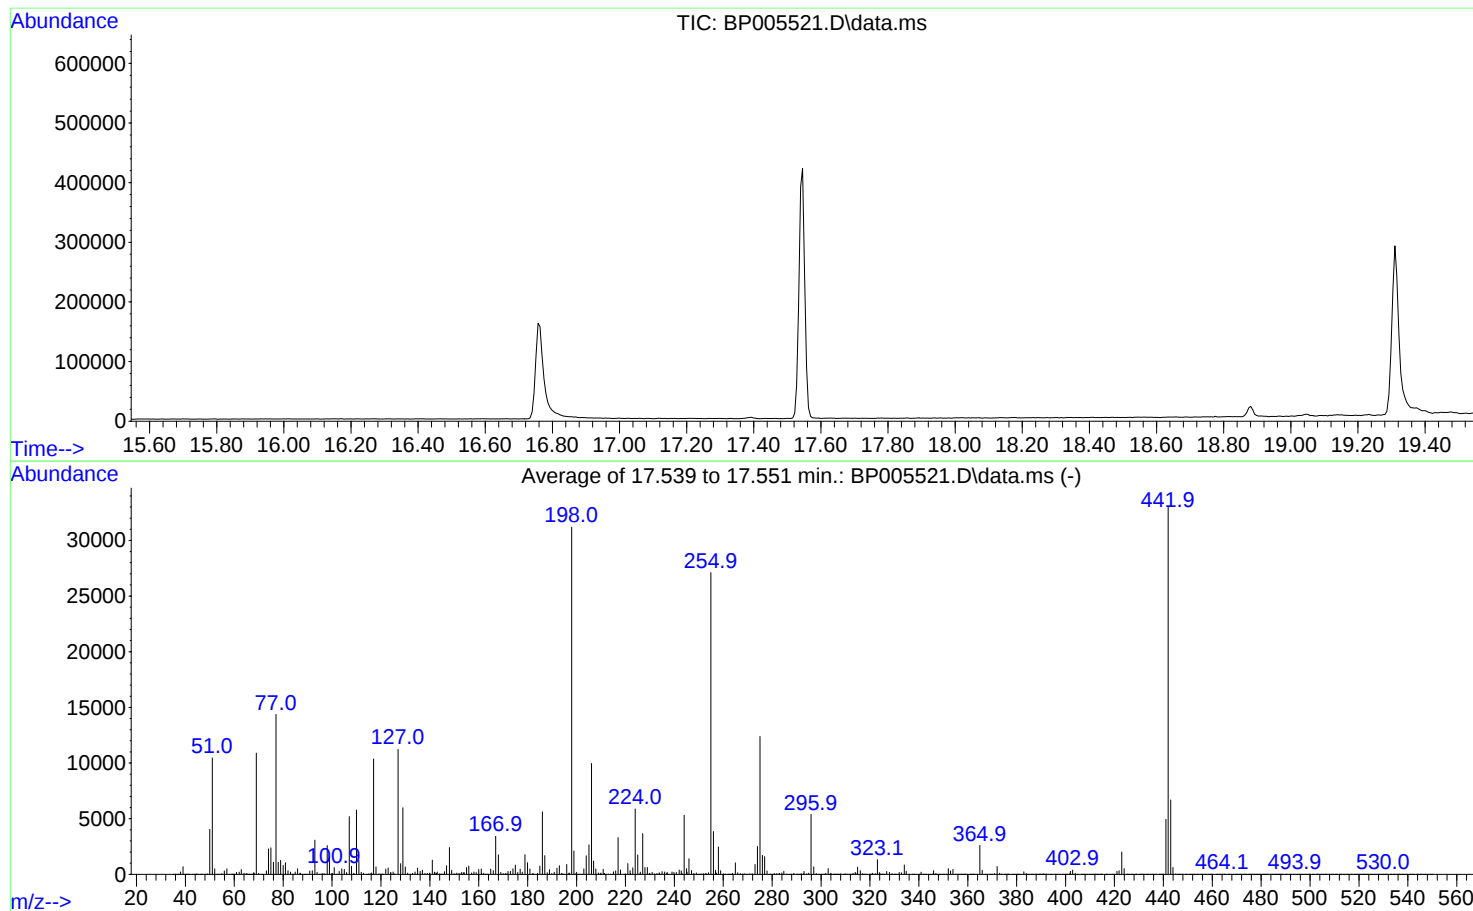




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	10469	PASS
68	69	0.00	2	1.3	140	PASS
69	198	0.00	100	35.0	10900	PASS
70	69	0.00	2	0.8	82	PASS
127	198	10	80	36.0	11234	PASS
197	198	0.00	2	0.4	110	PASS
198	198	100	100	100.0	31187	PASS
199	198	5	9	6.7	2100	PASS
275	198	10	60	39.7	12393	PASS
365	198	1	100	8.3	2596	PASS
441	198	0.01	100	15.9	4951	PASS
442	442	100	100	100.0	33048	PASS
443	442	15	24	20.2	6680	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051321\
 Data File : BP005521.D
 Acq On : 13 May 2021 15:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 13 16:15:02 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 11 11:20:59 2021
 Response via : Initial Calibration

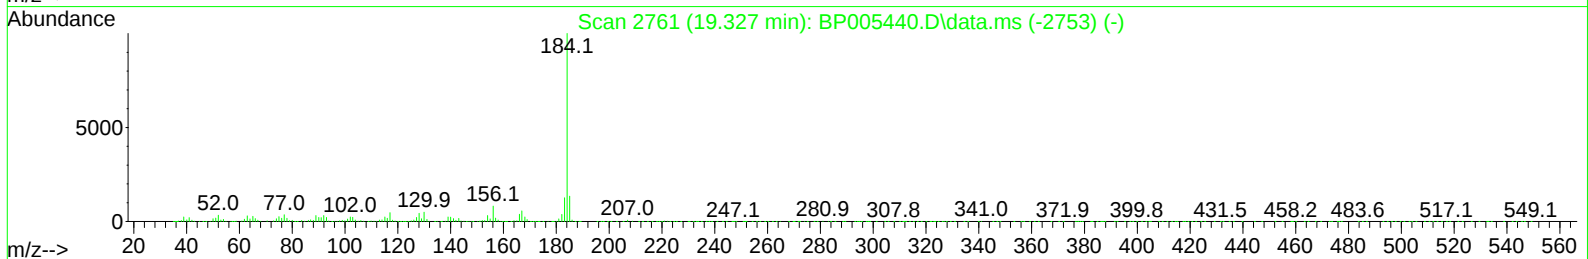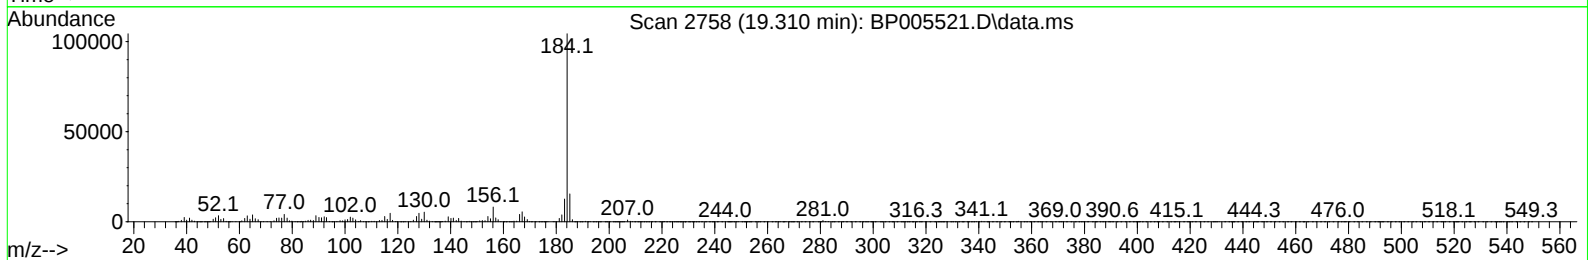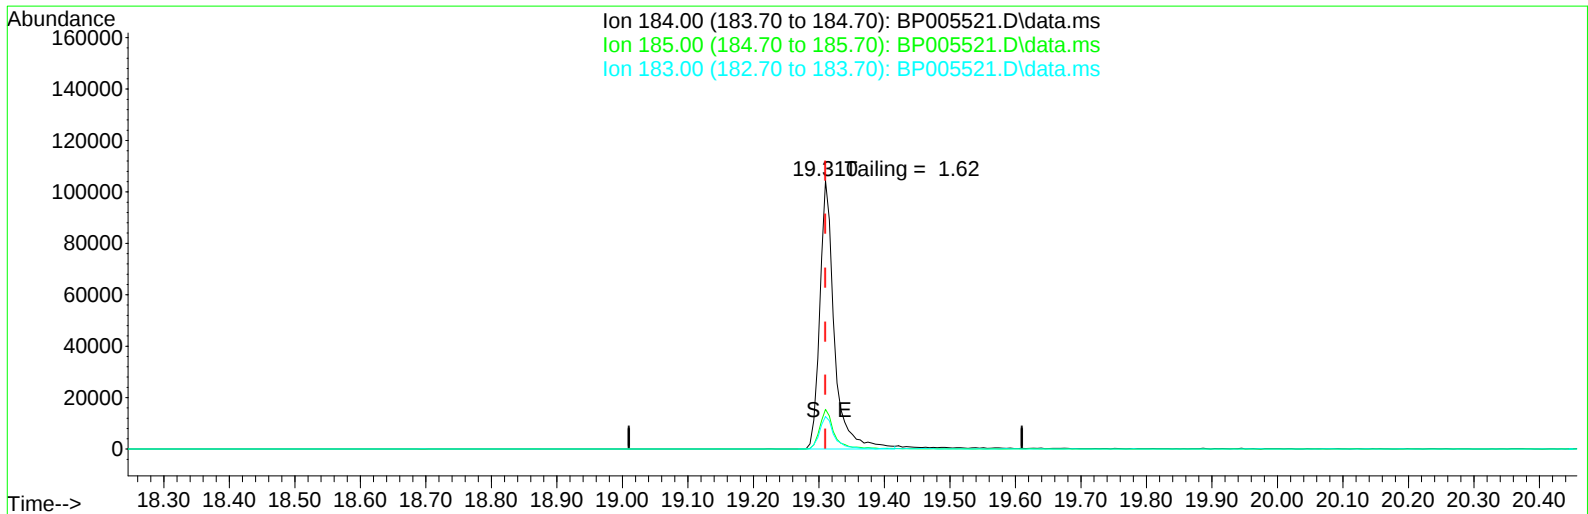

TIC: BP005521.D\data.ms

(77) Benzidine

19.310min (0.000) 109529.60 ng




response 162757

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.81
183.00	12.30	12.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051321\
 Data File : BP005521.D
 Acq On : 13 May 2021 15:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 13 16:15:02 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 11 11:20:59 2021
 Response via : Initial Calibration

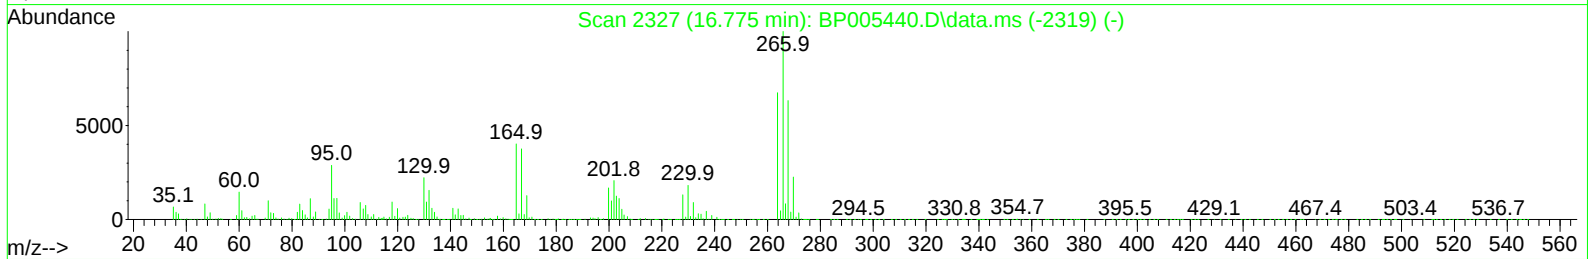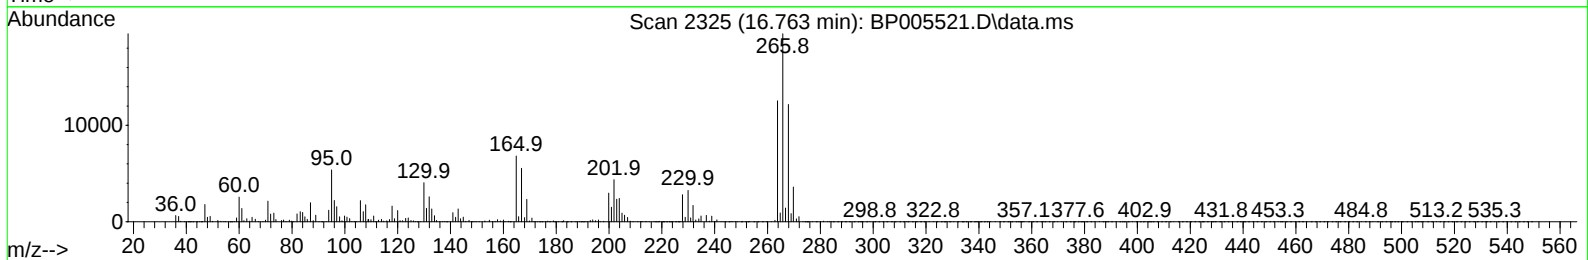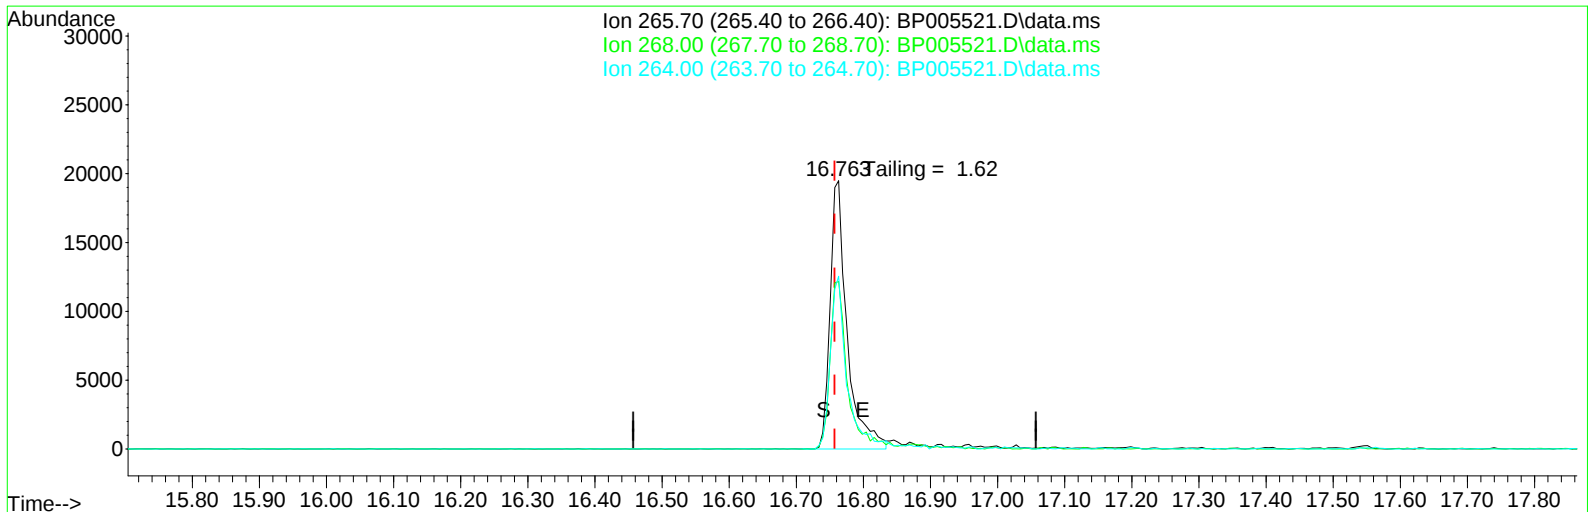

TIC: BP005521.D\data.ms

(70) Pentachlorophenol (C)

16.763min (+ 0.006) 670992.25 ng

response 35239

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	62.41
264.00	67.10	64.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/13/2021	BNA_P	<u>BP005521.D</u>
Compound Name	Response	Retention Time
DDT	118693	20.5
DDD	3925	20.07
DDE	515	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4440	123133	3.61

Instrument :
BNA_P
ClientSampleId :
DFTPP