
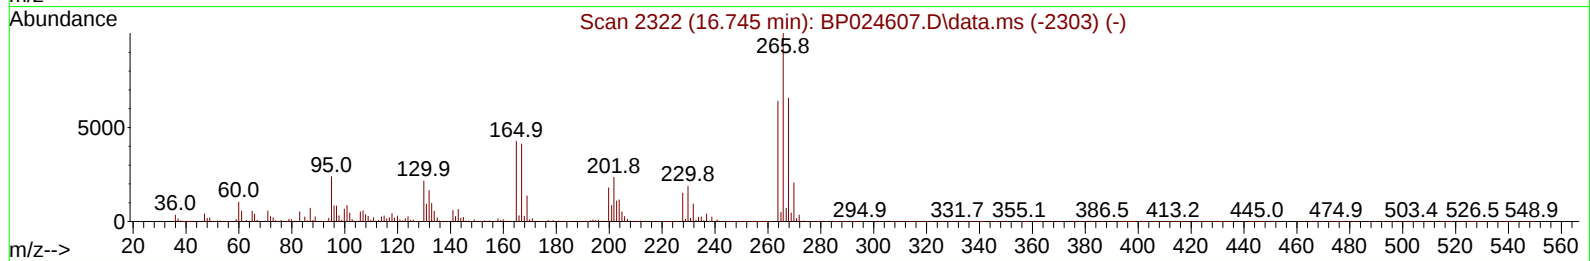
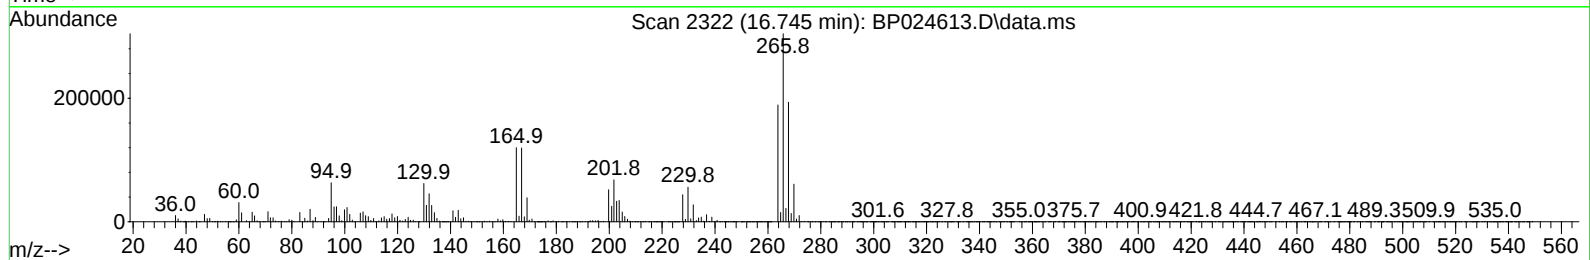


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051325\
Data File : BP024613.D
Acq On : 13 May 2025 10:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 12:28:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 12:28:24 2025
Response via : Initial Calibration

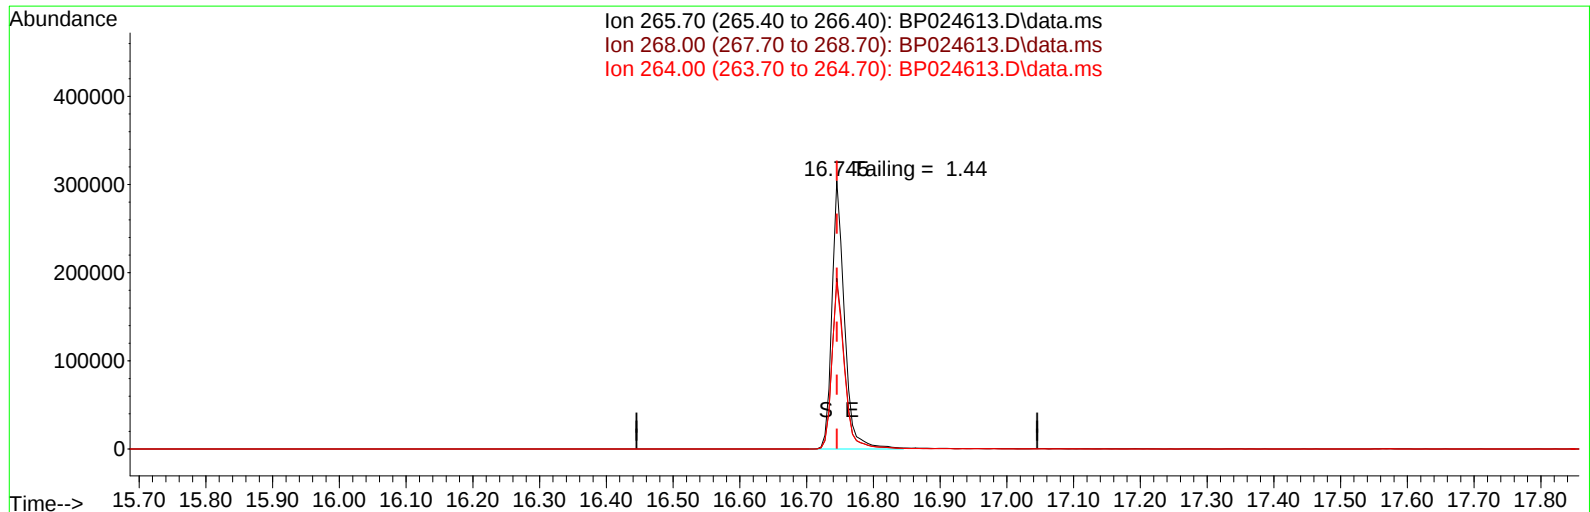

TIC: BP024613.D\data.ms

(70) Pentachlorophenol (C)




16.745min (-0.000) 42670.46 ng

response 398426

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	63.59
264.00	64.00	62.12
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051325\  
Data File : BP024613.D  
Acq On    : 13 May 2025  10:00  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 13 12:28:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 12:28:24 2025
Response via : Initial Calibration

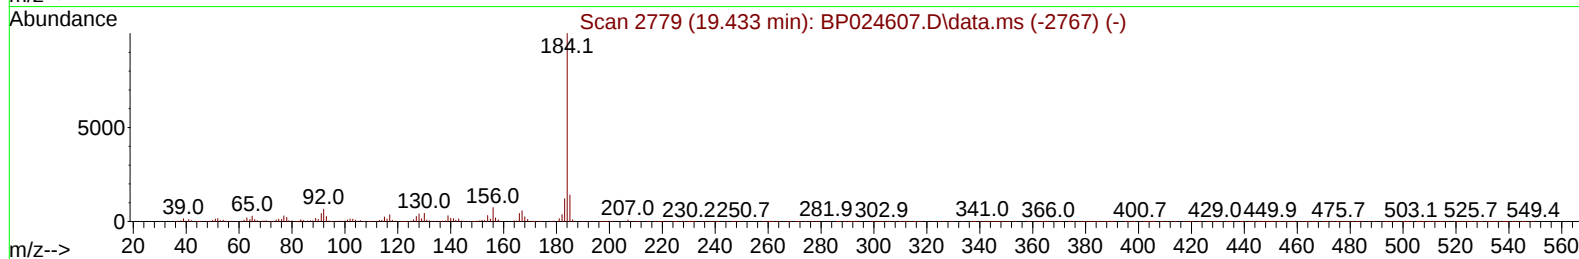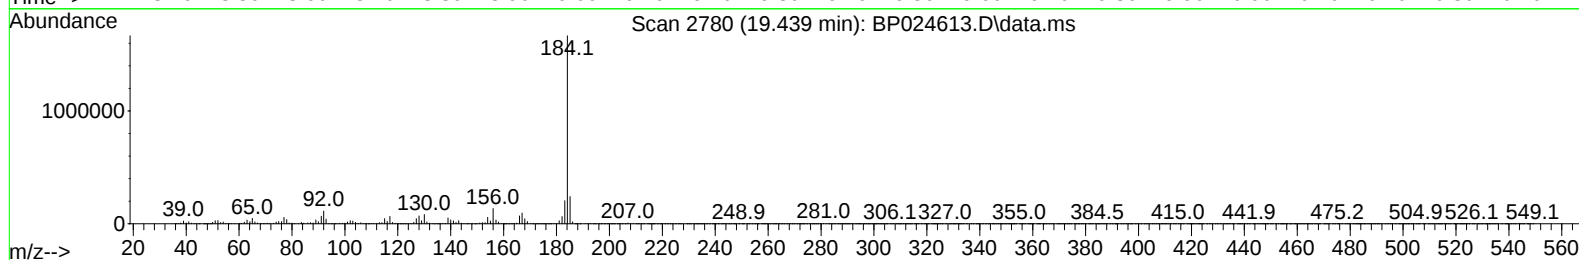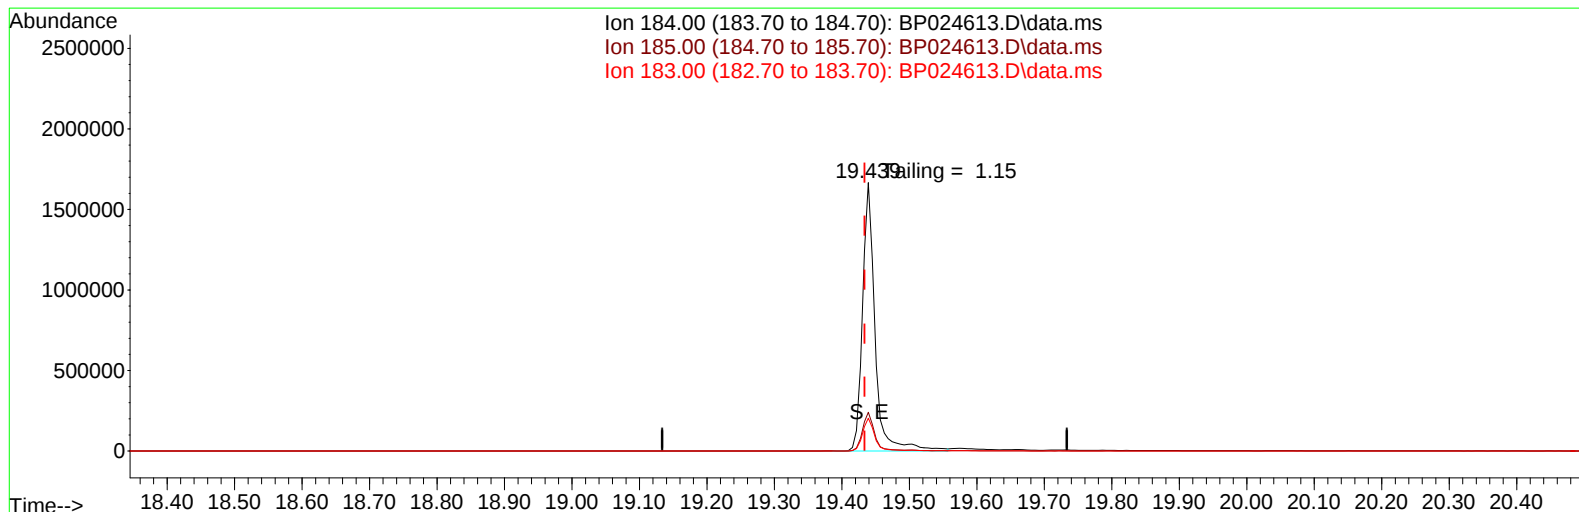

TIC: BP024613.D\data.ms

(77) Benzidine

19.439min (+ 0.006) 5637.89 ng

response 2074486

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.46
183.00	12.10	12.23
0.00	0.00	0.00