
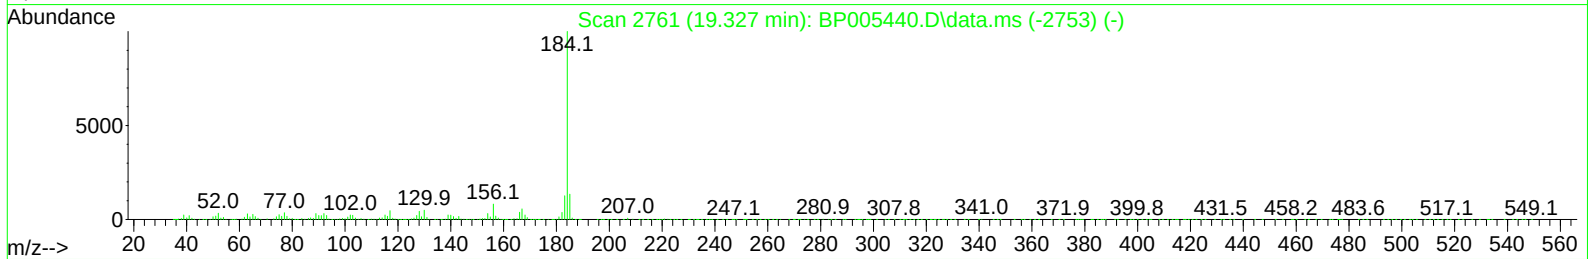
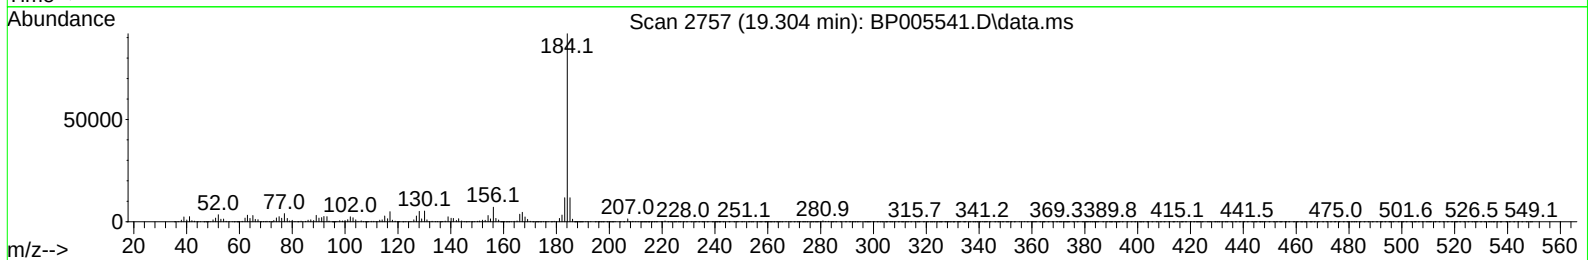


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051421\
 Data File : BP005541.D
 Acq On : 14 May 2021 10:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 11:55:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 11 11:20:59 2021
 Response via : Initial Calibration

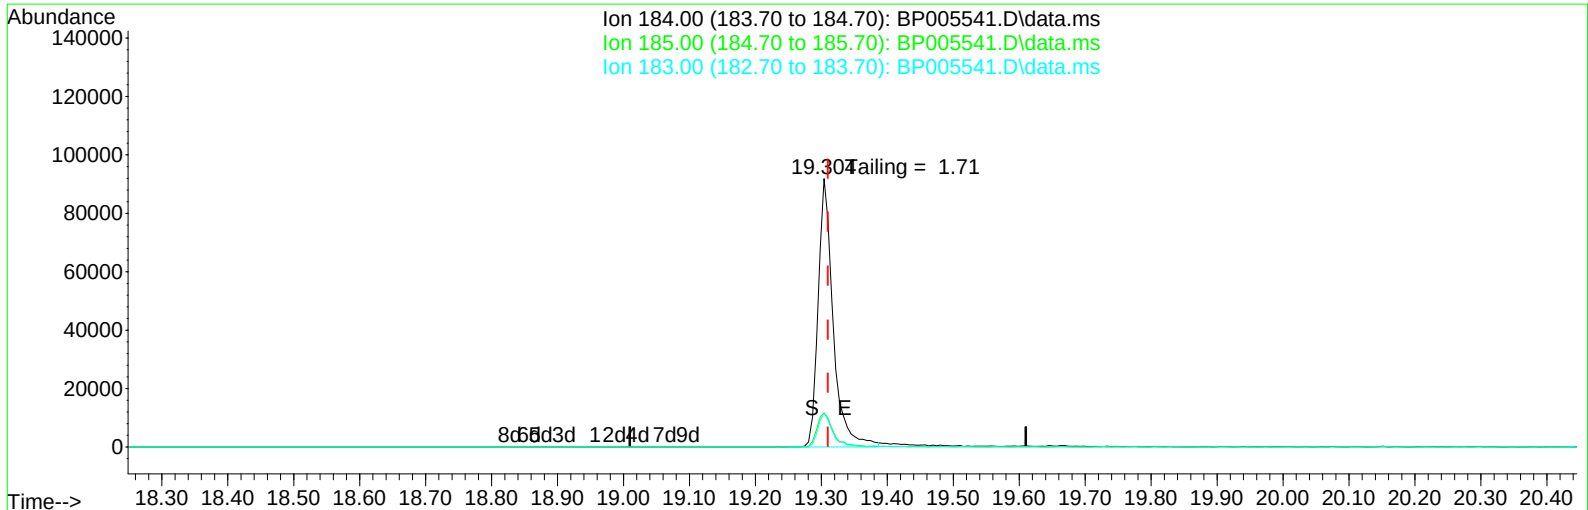

TIC: BP005541.D\data.ms

(77) Benzidine




19.304min (-0.006) 235784.52 ng m

response 149636

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	12.76
183.00	12.30	12.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051421\
 Data File : BP005541.D
 Acq On : 14 May 2021 10:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 11:55:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 11 11:20:59 2021
 Response via : Initial Calibration

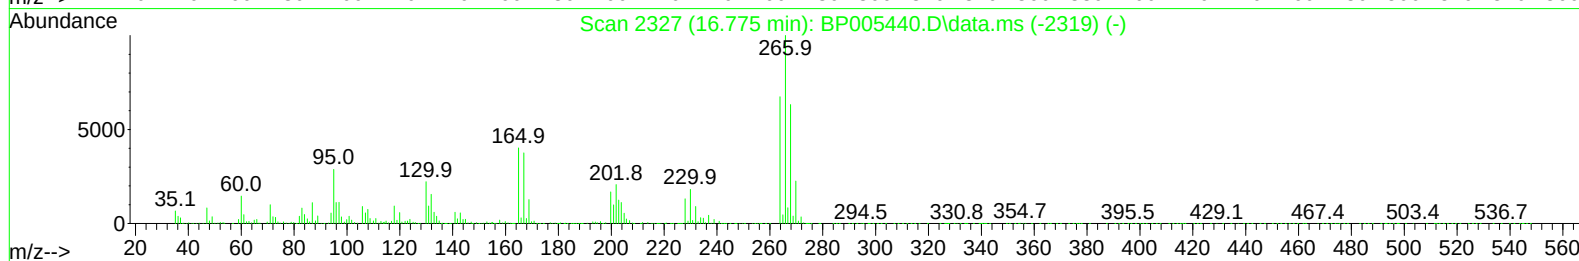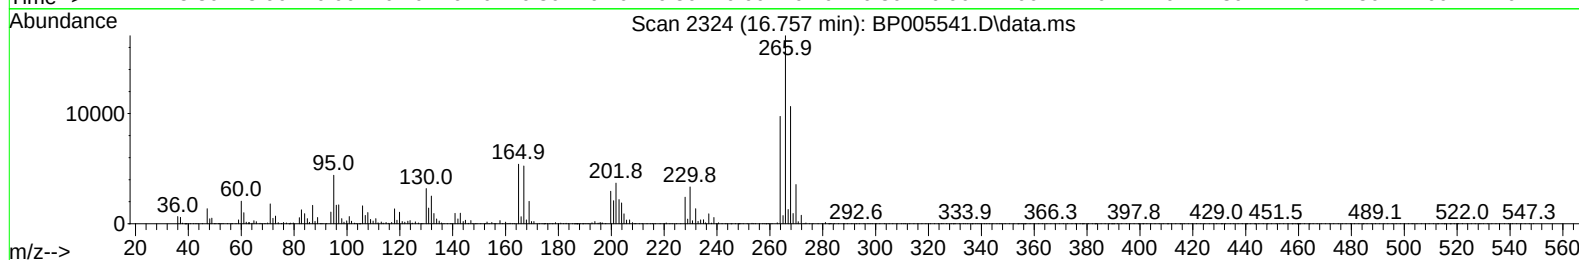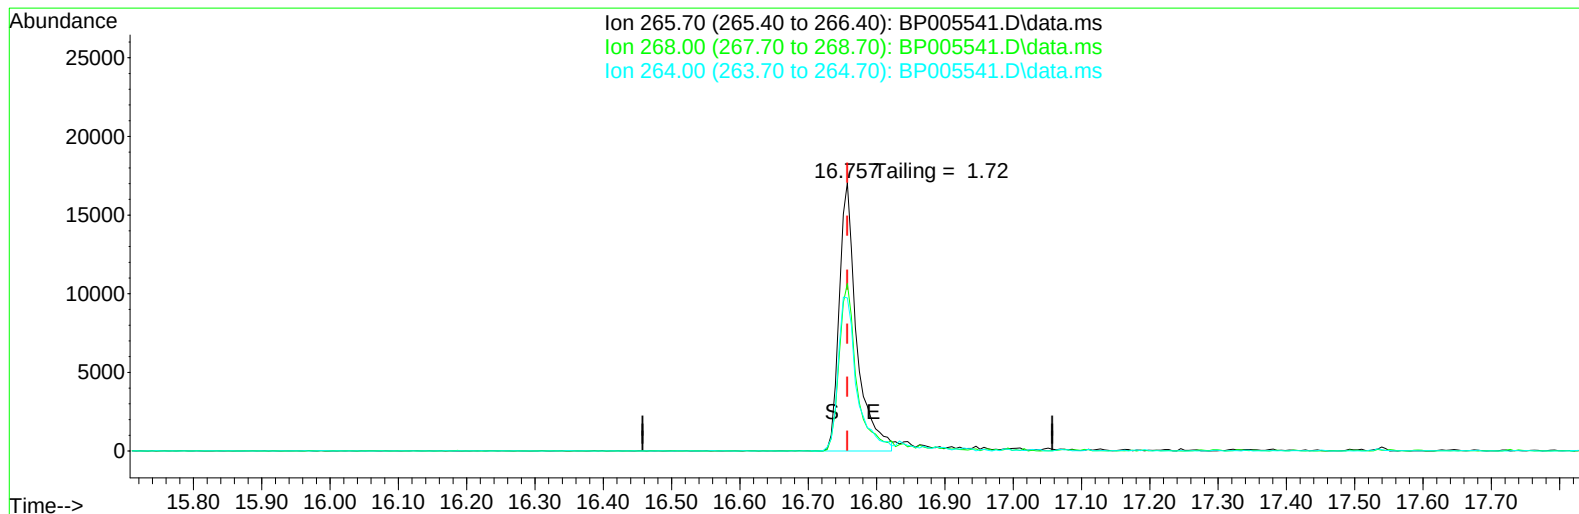

TIC: BP005541.D\data.ms

(70) Pentachlorophenol (C)

16.757min (-0.000) 324472.34 ng m

response 30673

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	62.36
264.00	67.10	57.09
0.00	0.00	0.00