


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051421\
 Data File : BP005541.D
 Acq On : 14 May 2021 10:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 17 15:35:47 2021

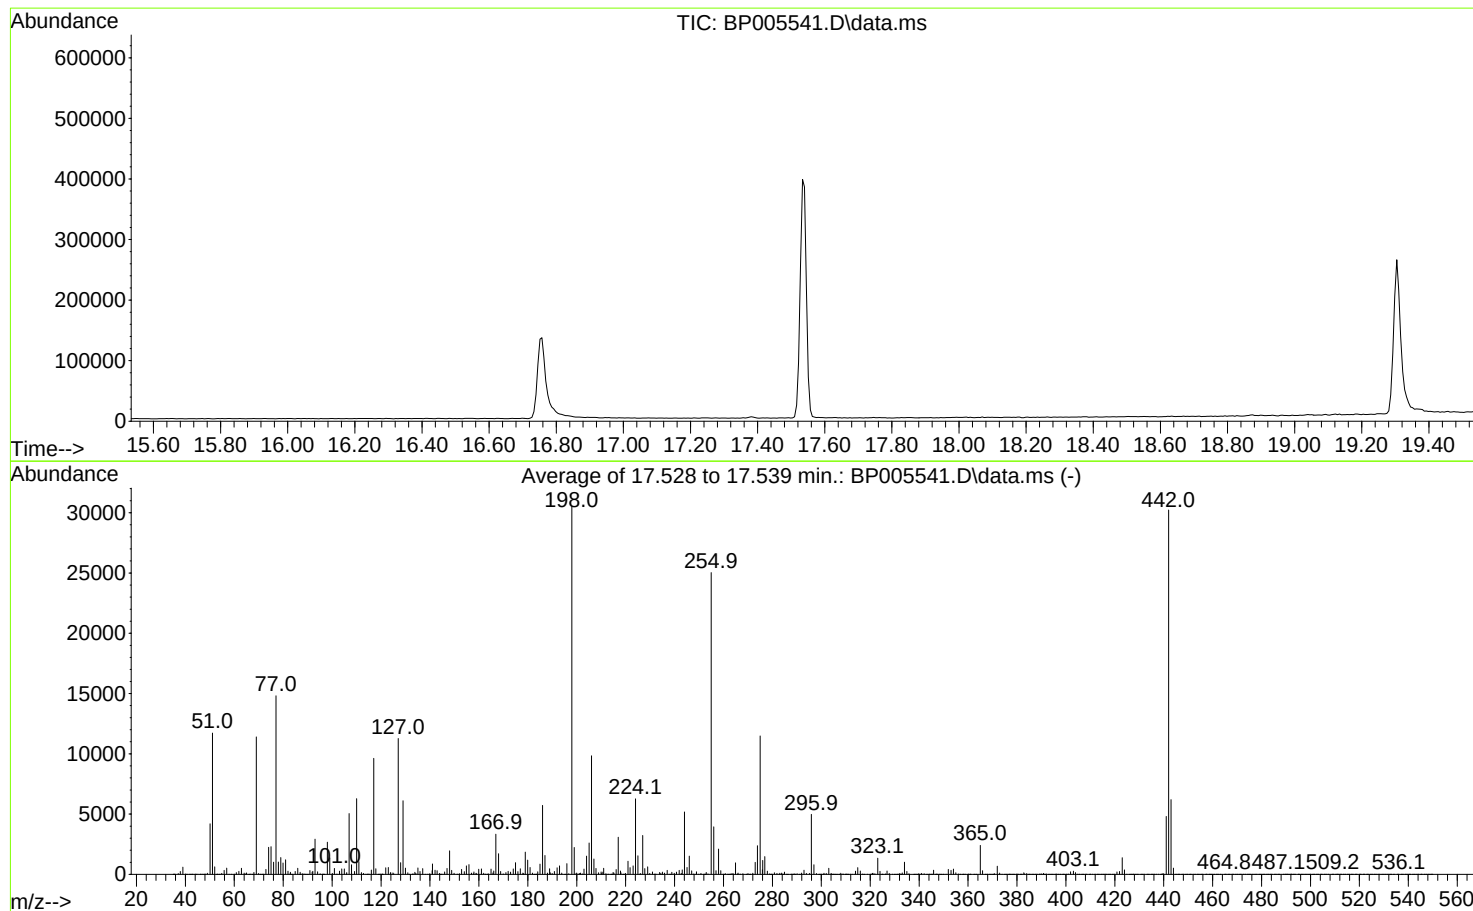

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	11718	PASS
68	69	0.00	2	1.4	162	PASS
69	198	0.00	100	37.4	11403	PASS
70	69	0.00	2	0.6	67	PASS
127	198	10	80	36.9	11269	PASS
197	198	0.00	2	0.2	58	PASS
198	198	100	100	100.0	30517	PASS
199	198	5	9	7.3	2230	PASS
275	198	10	60	37.6	11479	PASS
365	198	1	100	7.9	2404	PASS
441	198	0.01	100	15.8	4809	PASS
442	442	100	100	100.0	30229	PASS
443	442	15	24	20.5	6204	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/14/2021	BNA_P	<u>BP005541.D</u>
Compound Name	Response	Retention Time
DDT	109773	20.49
DDD	4109	20.06
DDE	601	19.57
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4710	114483	4.11

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051421\
 Data File : BP005541.D
 Acq On : 14 May 2021 10:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 14 11:55:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 11 11:20:59 2021
 Response via : Initial Calibration

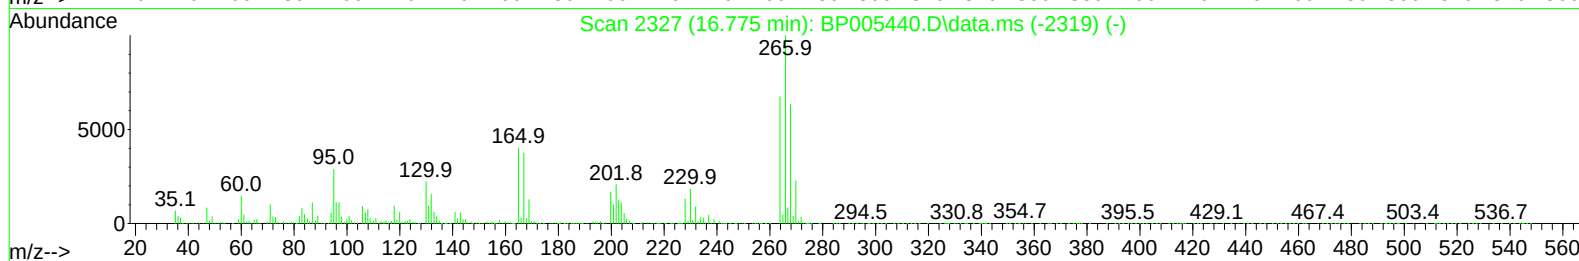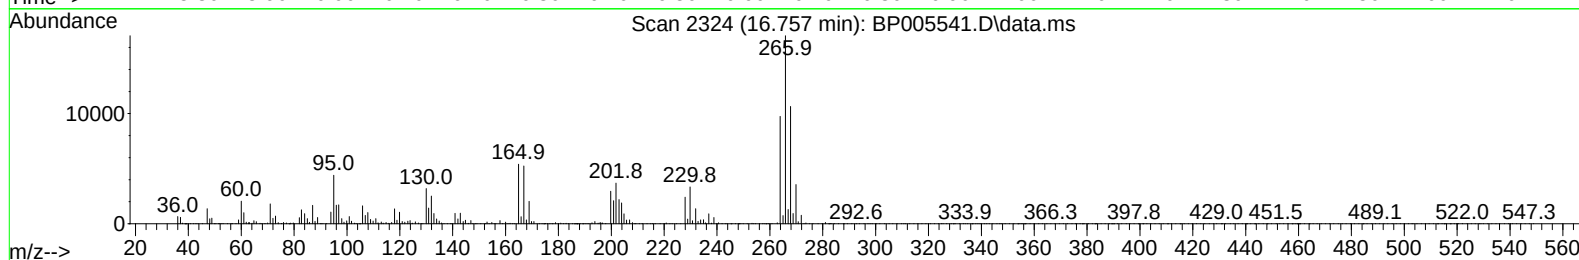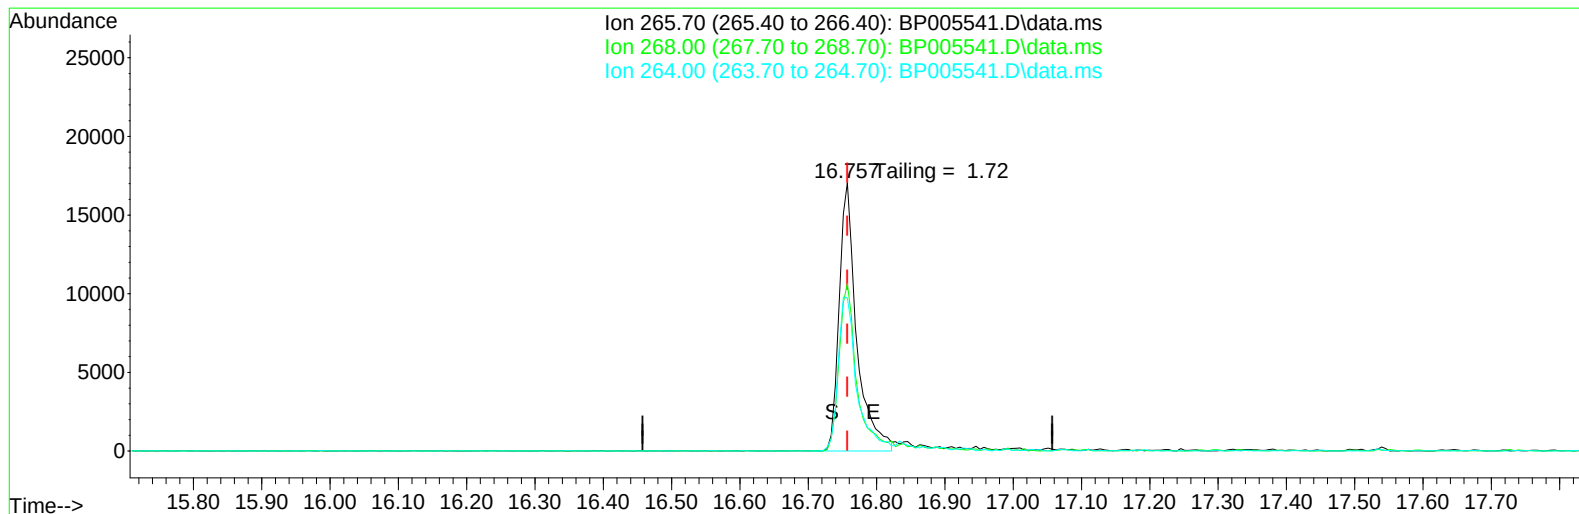

TIC: BP005541.D\data.ms

(70) Pentachlorophenol (C)

16.757min (-0.000) 324472.34 ng m




response 30673

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	62.36
264.00	67.10	57.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051421\
 Data File : BP005541.D
 Acq On : 14 May 2021 10:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 14 11:55:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 11 11:20:59 2021
 Response via : Initial Calibration

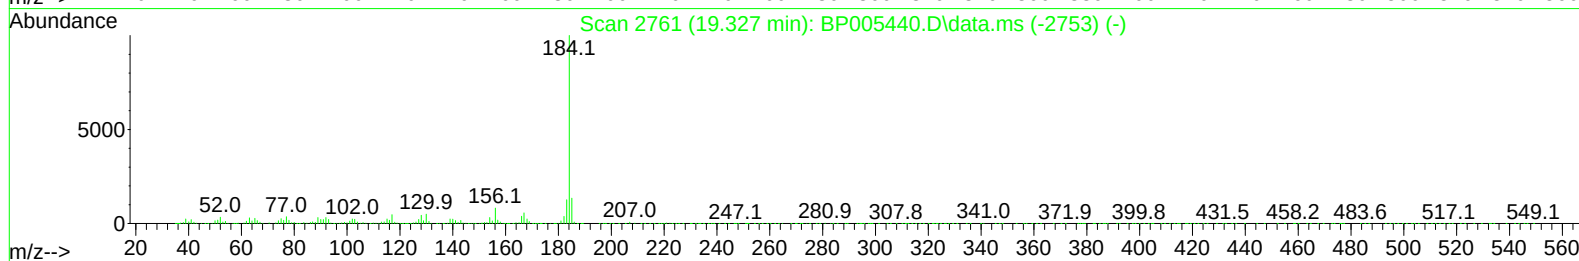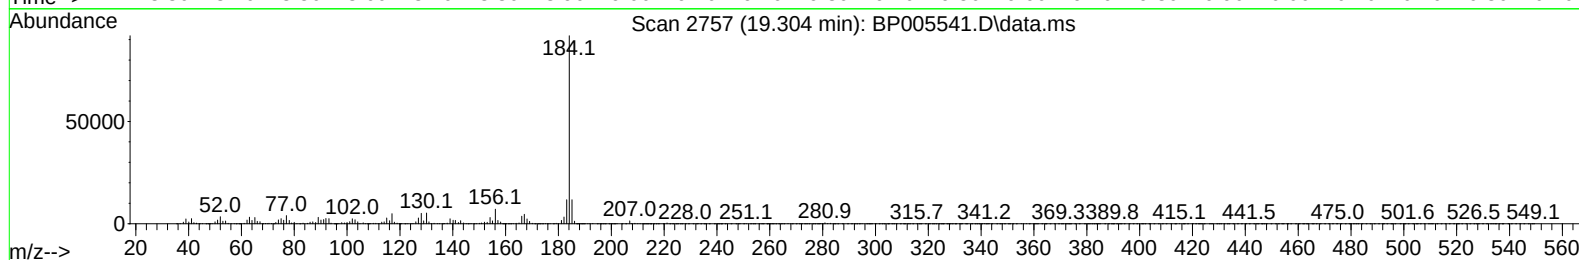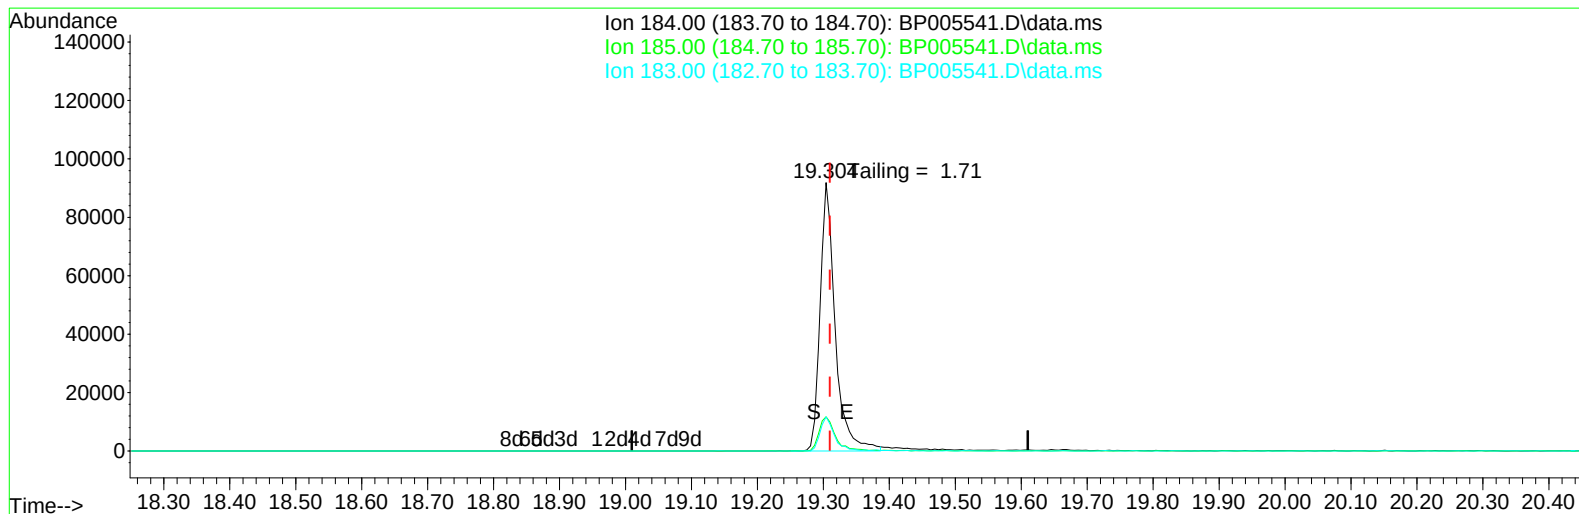

TIC: BP005541.D\data.ms

(77) Benzidine

19.304min (-0.006) 235784.52 ng m

response 149636

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	12.76
183.00	12.30	12.73
0.00	0.00	0.00