




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020384.D
Acq On : 15 May 2024 03:08
Operator : MA/JU
Sample : P2372-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43W4

Manual IntegrationsAPPROVED

Quant Time: May 15 03:47:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 14 23:58:44 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
Supervised By :mohammad ahmed 05/17/2024

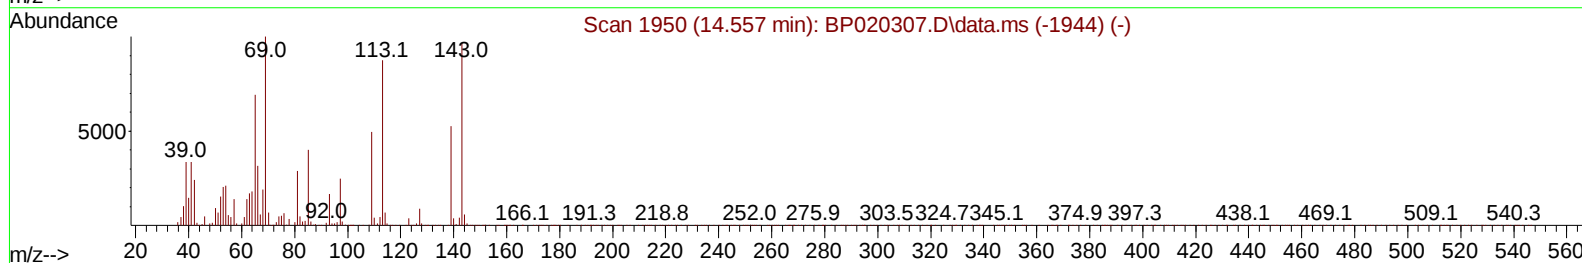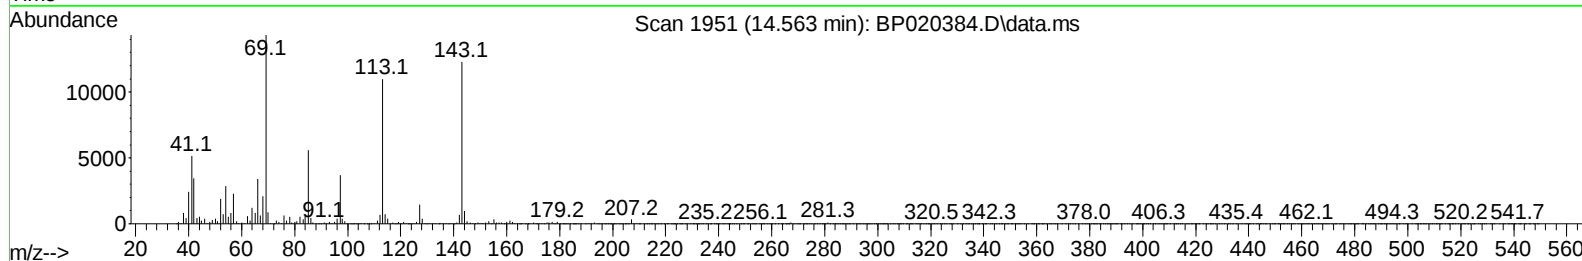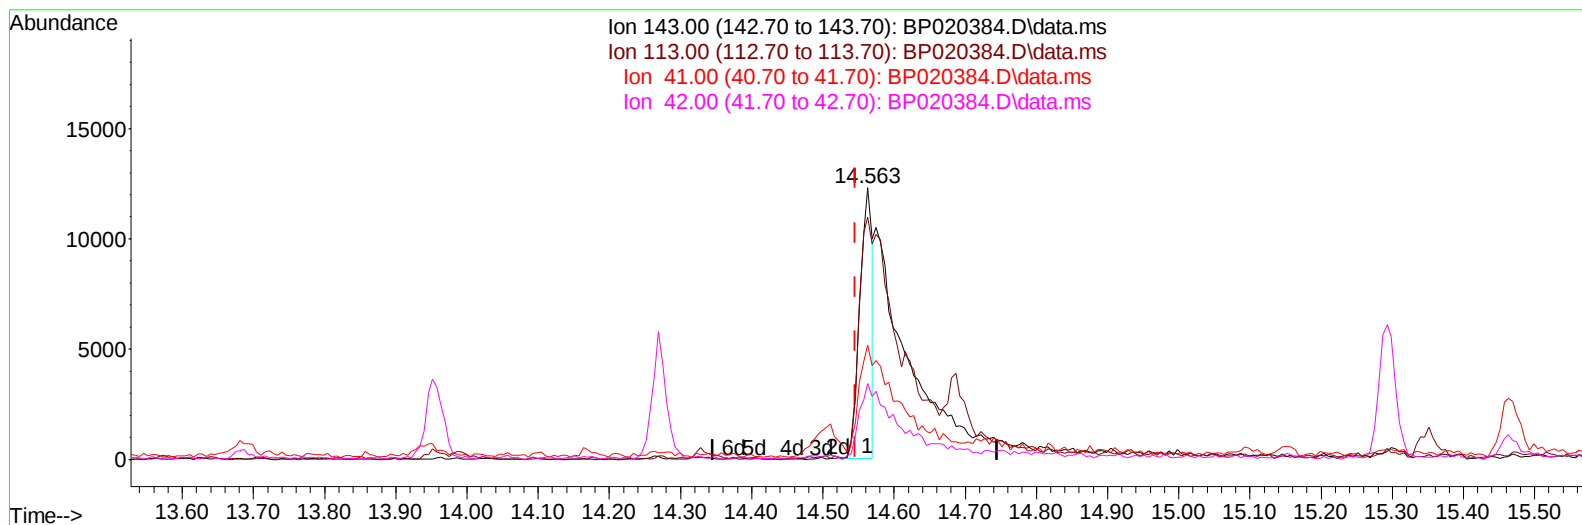

TIC: BP020384.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.563min (+ 0.018) 5.79 ng/u1

response 15198

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	89.35
41.00	50.30	42.03
42.00	32.50	28.03




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020384.D
 Acq On : 15 May 2024 03:08
 Operator : MA/JU
 Sample : P2372-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W4

Manual IntegrationsAPPROVED

Quant Time: May 15 03:47:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

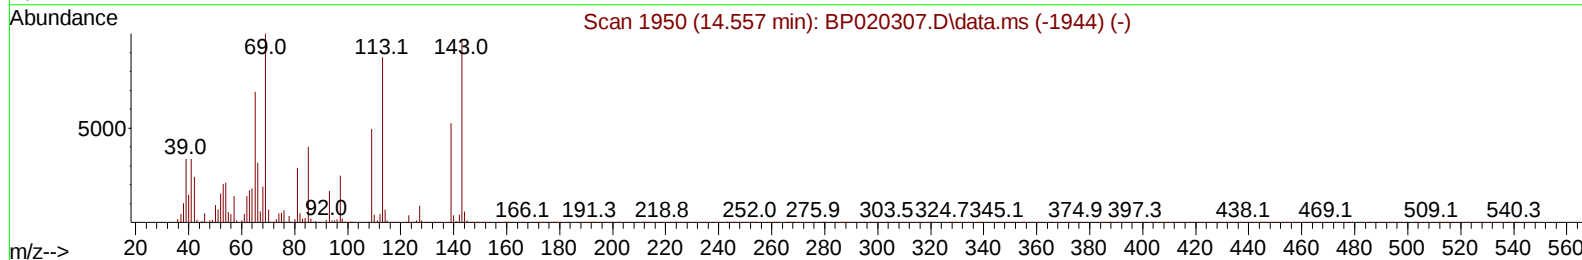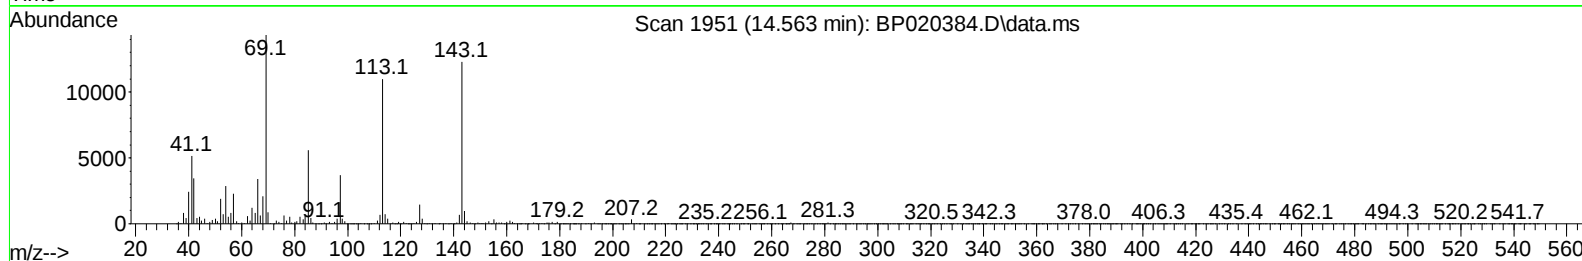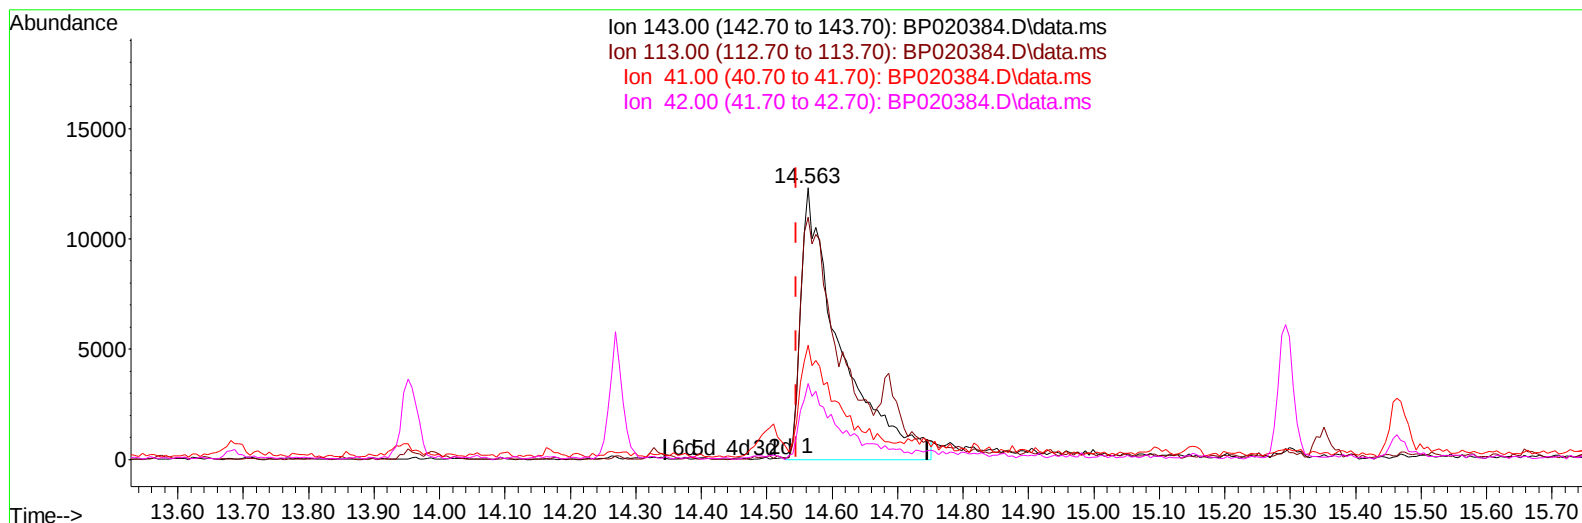

TIC: BP020384.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.563min (+ 0.018) 19.65 ng/ul m

response 51546

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	89.35
41.00	50.30	42.03
42.00	32.50	28.03

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020384.D
 Acq On : 15 May 2024 03:08
 Operator : MA/JU
 Sample : P2372-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

Quant Time: May 15 03:49:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.593	152		81125	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136		337347	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.269	164		233733	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.116	188		530773	20.000	ng/ul	0.00
79) Chrysene-d12	21.604	240		544206	20.000	ng/ul	0.00
88) Perylene-d12	24.945	264		628427	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.193	96		7459	3.883	ng/uL	0.00
4) Pyridine-d5	3.605	84		42087	7.541	ng/ul	0.00
7) Phenol-d5	6.787	99		143548	20.604	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.952	67		88494	20.910	ng/ul	0.00
11) 2-Chlorophenol-d4	7.134	132		117047	23.501	ng/ul	0.00
15) 4-Methylphenol-d8	8.311	113		108926	19.339	ng/ul	0.00
21) Nitrobenzene-d5	8.758	128		59937	23.727	ng/ul	0.00
24) 2-Nitrophenol-d4	9.469	143		68819	23.789	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.010	165		125965	23.862	ng/ul	0.00
31) 4-Chloroaniline-d4	10.540	131		102932	13.932	ng/ul	0.01
46) Dimethylphthalate-d6	13.687	166		439539	25.751	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160		472106	25.039	ng/ul	0.00
54) 4-Nitrophenol-d4	14.563	143		51546m	19.649	ng/ul	0.02
60) Fluorene-d10	15.293	176		372161	26.141	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.463	200		65036	19.309	ng/ul	0.00
73) Anthracene-d10	17.222	188		619501	26.980	ng/ul	0.00
81) Pyrene-d10	19.616	212		795055	24.993	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.721	264		815545	26.840	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020384.D
Acq On : 15 May 2024 03:08
Operator : MA/JU
Sample : P2372-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43W4

Manual IntegrationsAPPROVED

Quant Time: May 15 03:49:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 14 23:58:44 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
Supervised By :mohammad ahmed 05/17/2024

