




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020385.D
Acq On : 15 May 2024 03:52
Operator : MA/JU
Sample : P2372-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43W5

Manual IntegrationsAPPROVED

Quant Time: May 15 04:30:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 14 23:58:44 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
Supervised By :mohammad ahmed 05/17/2024

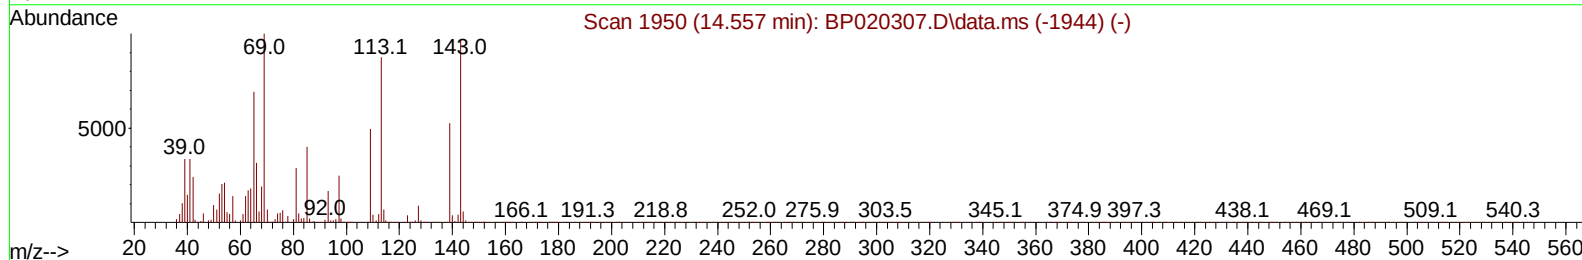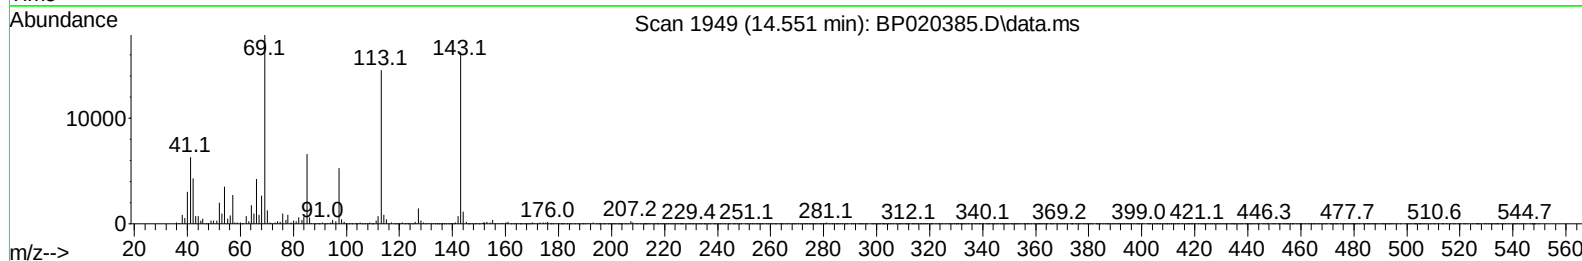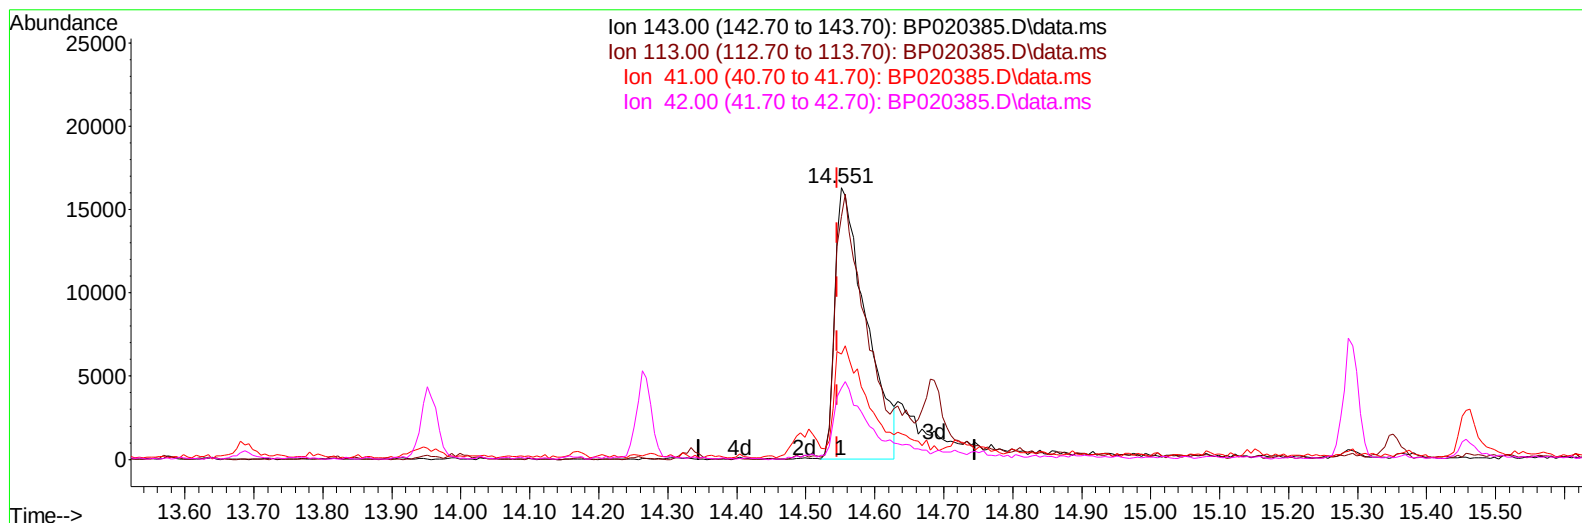

TIC: BP020385.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.551min (+ 0.006) 18.17 ng/ul

response 50915

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	89.59
41.00	50.30	38.89#
42.00	32.50	26.35




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020385.D
Acq On : 15 May 2024 03:52
Operator : MA/JU
Sample : P2372-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43W5

Manual IntegrationsAPPROVED

Quant Time: May 15 04:30:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 14 23:58:44 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
Supervised By :mohammad ahmed 05/17/2024

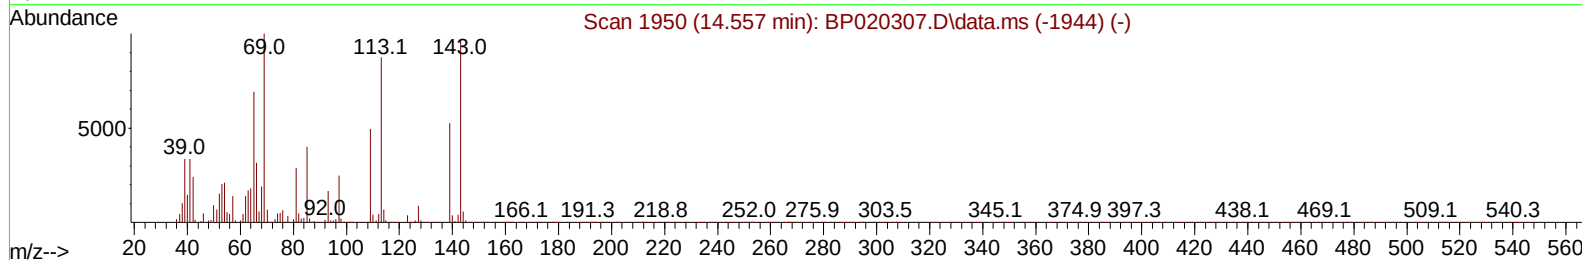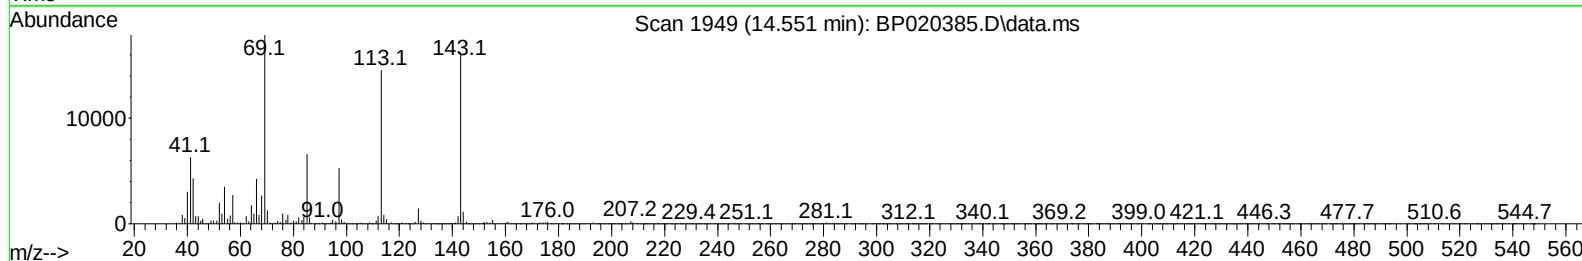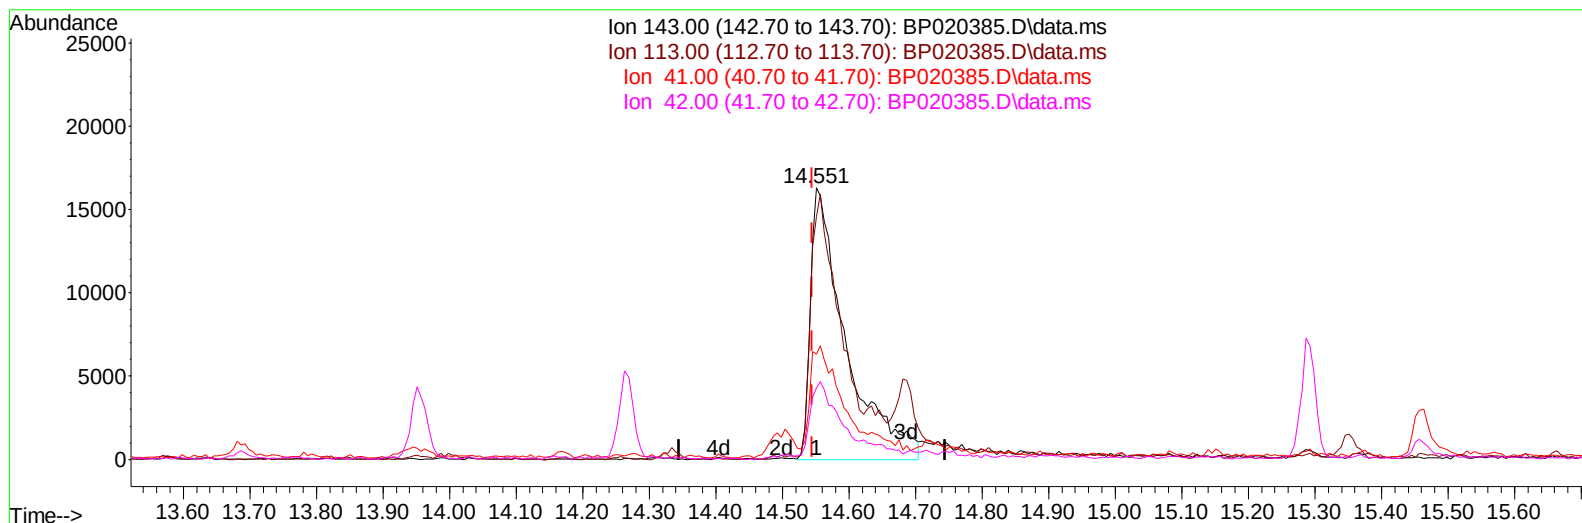

TIC: BP020385.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.551min (+ 0.006) 21.55 ng/ul m

response 60398

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	89.59
41.00	50.30	38.89#
42.00	32.50	26.35

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020385.D
 Acq On : 15 May 2024 03:52
 Operator : MA/JU
 Sample : P2372-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

Quant Time: May 15 04:31:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	78036	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136	338575	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.269	164	249668	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.110	188	569260	20.000	ng/ul	0.00
79) Chrysene-d12	21.598	240	534353	20.000	ng/ul	0.00
88) Perylene-d12	24.945	264	615566	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	7895	4.273	ng/uL	0.00
4) Pyridine-d5	3.605	84	53942	10.047	ng/ul	0.00
7) Phenol-d5	6.787	99	155863	23.257	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.946	67	90090	22.130	ng/ul	0.00
11) 2-Chlorophenol-d4	7.134	132	122427	25.554	ng/ul	0.00
15) 4-Methylphenol-d8	8.310	113	115409	21.301	ng/ul	0.00
21) Nitrobenzene-d5	8.752	128	62279	24.564	ng/ul	0.00
24) 2-Nitrophenol-d4	9.469	143	77604	26.729	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.010	165	134345	25.357	ng/ul	0.00
31) 4-Chloroaniline-d4	10.540	131	110929	14.960	ng/ul	0.01
46) Dimethylphthalate-d6	13.687	166	499211	27.381	ng/ul	0.00
49) Acenaphthylene-d8	13.951	160	543940	27.007	ng/ul	0.00
54) 4-Nitrophenol-d4	14.551	143	60398m	21.554	ng/ul	0.00
60) Fluorene-d10	15.292	176	429895	28.269	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	76255	21.109	ng/ul	0.00
73) Anthracene-d10	17.216	188	681764	27.684	ng/ul	0.00
81) Pyrene-d10	19.616	212	823863	26.376	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.727	264	816299	27.426	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020385.D
Acq On : 15 May 2024 03:52
Operator : MA/JU
Sample : P2372-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43W5

Manual IntegrationsAPPROVED

Quant Time: May 15 04:31:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 14 23:58:44 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
Supervised By :mohammad ahmed 05/17/2024

