




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020390.D
Acq On : 15 May 2024 07:28
Operator : MA/JU
Sample : P2372-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43W7

Manual IntegrationsAPPROVED

Quant Time: May 15 08:00:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 14 23:58:44 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
Supervised By :mohammad ahmed 05/17/2024

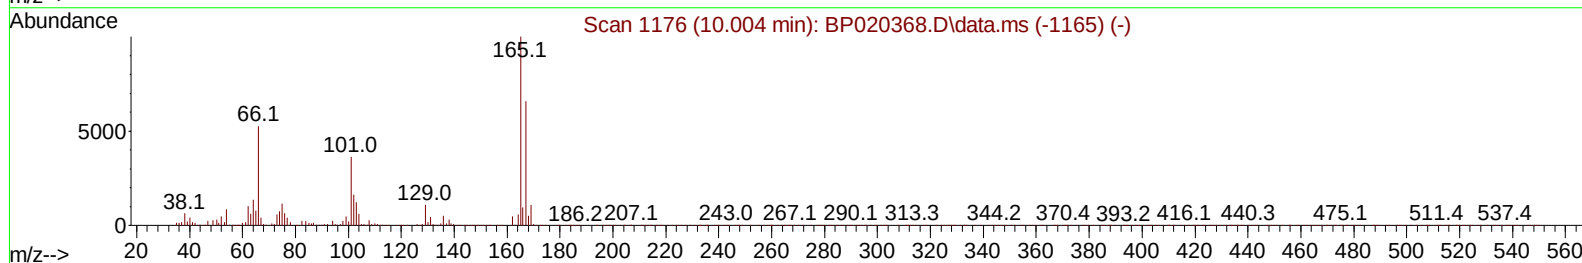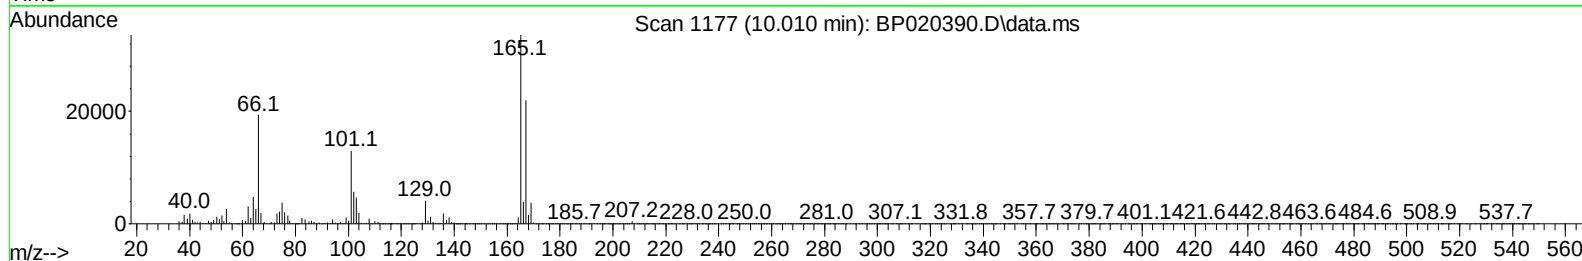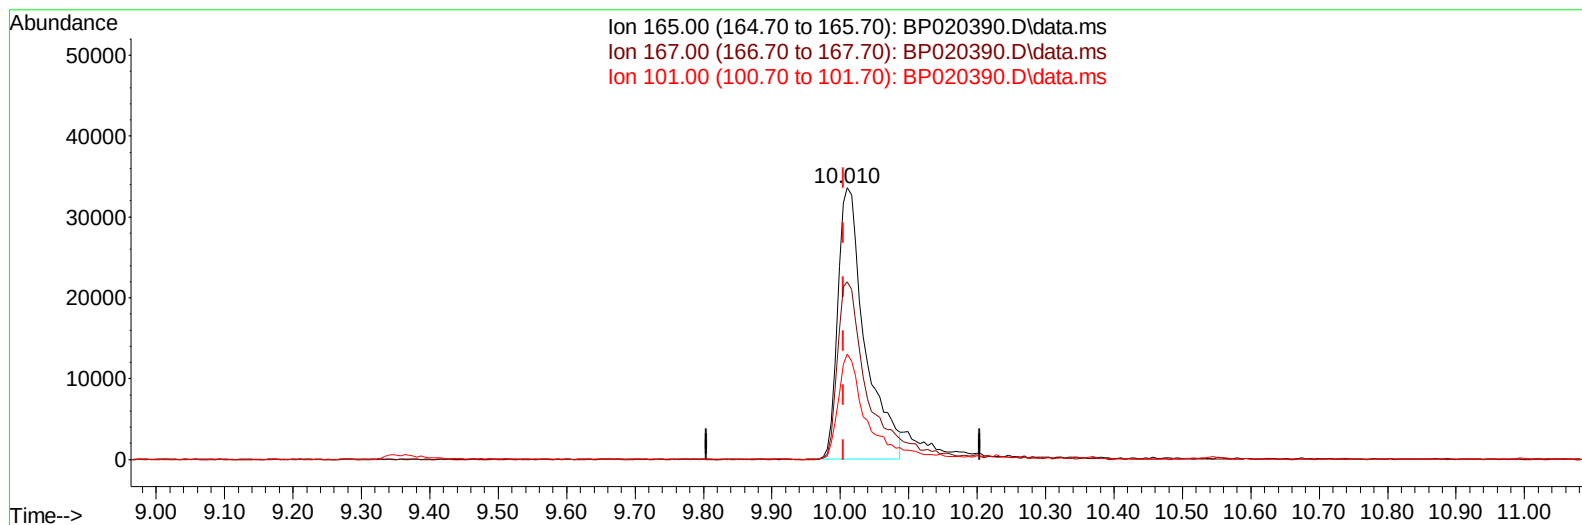

TIC: BP020390.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.010min (+ 0.006) 22.44 ng/ul

response 92712

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	63.00	65.40
101.00	40.90	38.71
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020390.D
 Acq On : 15 May 2024 07:28
 Operator : MA/JU
 Sample : P2372-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W7

Manual IntegrationsAPPROVED

Quant Time: May 15 08:00:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

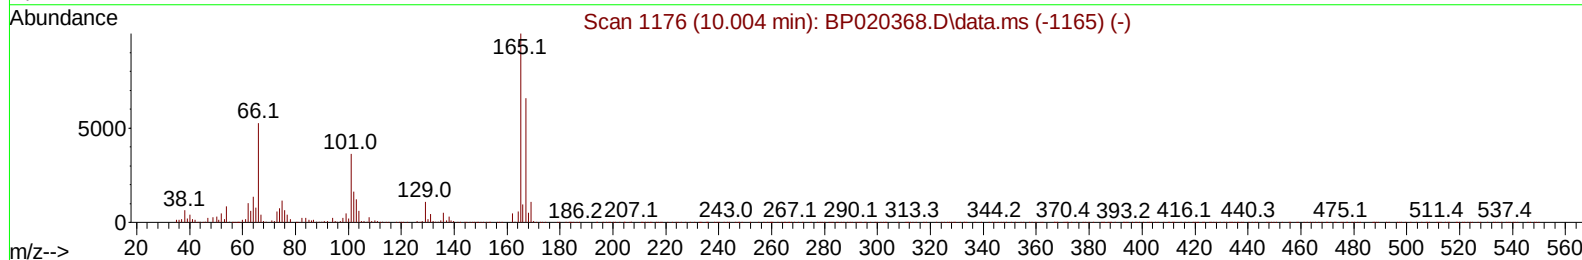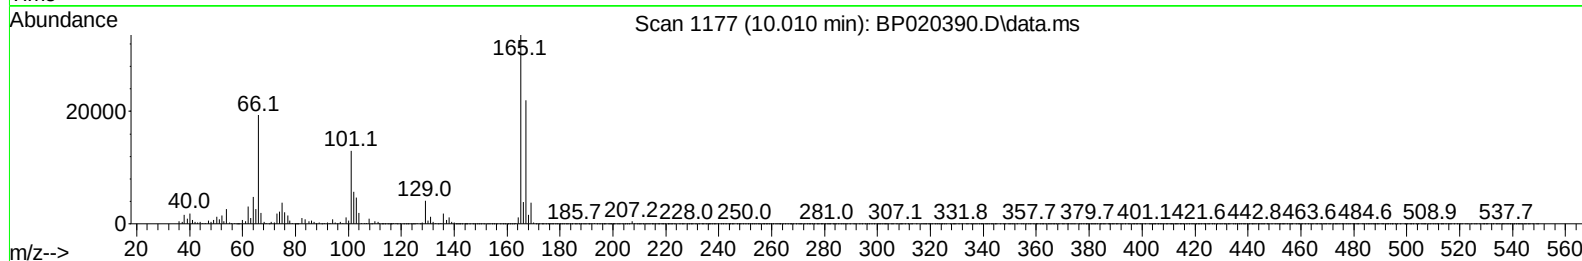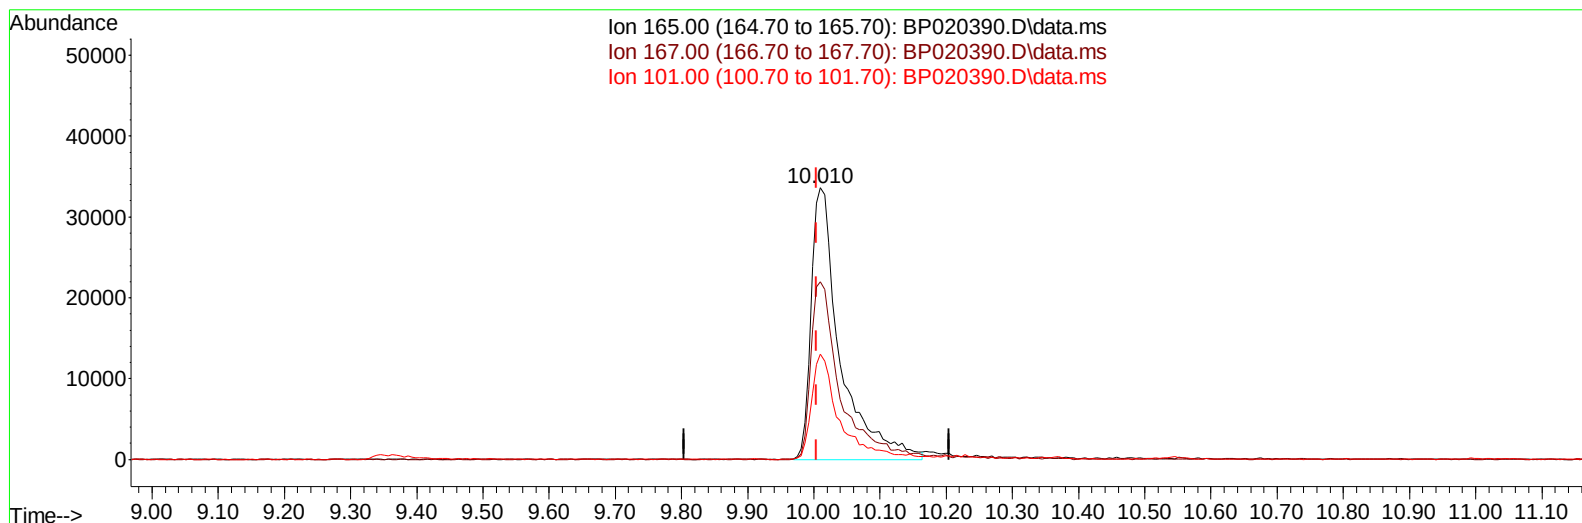

TIC: BP020390.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.010min (+ 0.006) 24.57 ng/ul m

response 101524

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	63.00	65.40
101.00	40.90	38.71
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020390.D
 Acq On : 15 May 2024 07:28
 Operator : MA/JU
 Sample : P2372-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W7

Manual IntegrationsAPPROVED

Quant Time: May 15 08:00:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

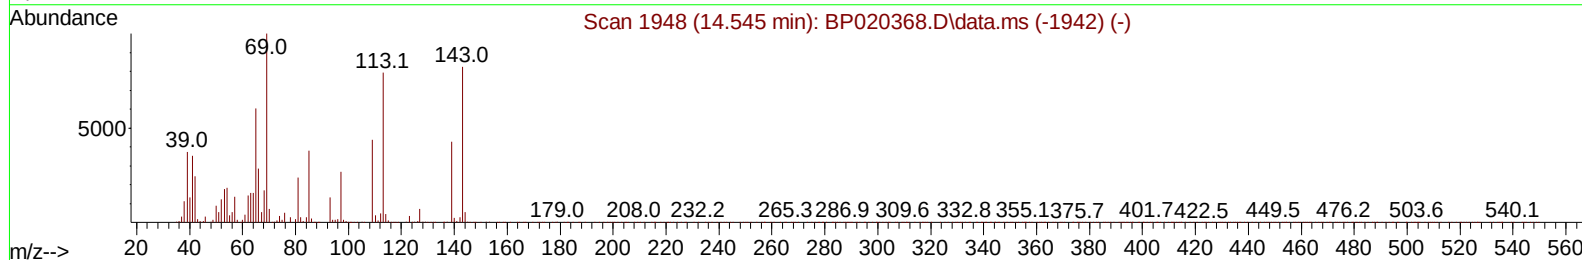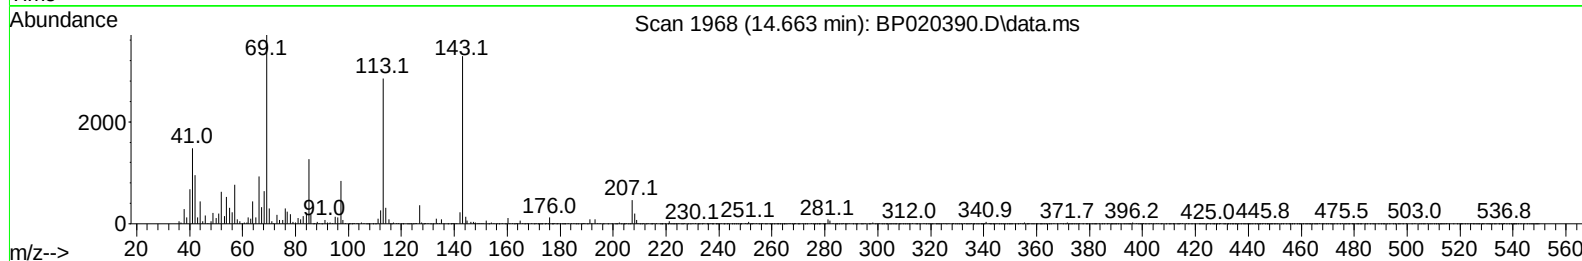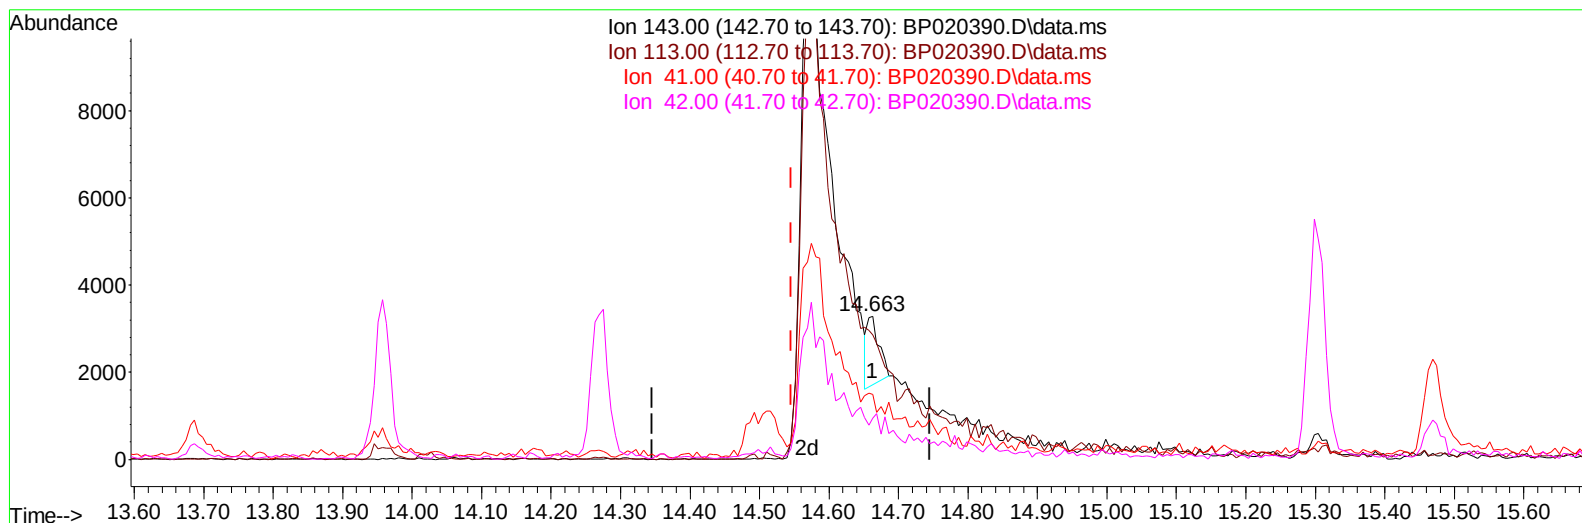

TIC: BP020390.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.663min (+ 0.118) 0.88 ng/ul

response 1913

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	86.76
41.00	50.30	45.19
42.00	32.50	28.97




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020390.D
 Acq On : 15 May 2024 07:28
 Operator : MA/JU
 Sample : P2372-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W7

Manual IntegrationsAPPROVED

Quant Time: May 15 08:00:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

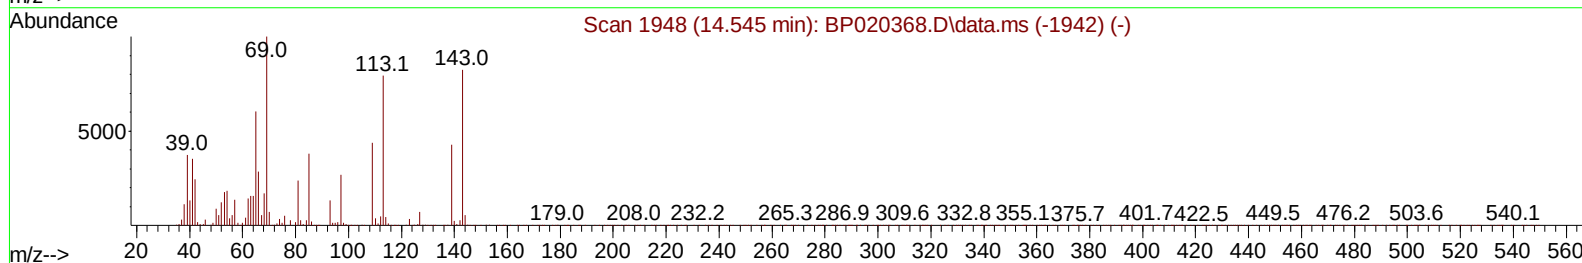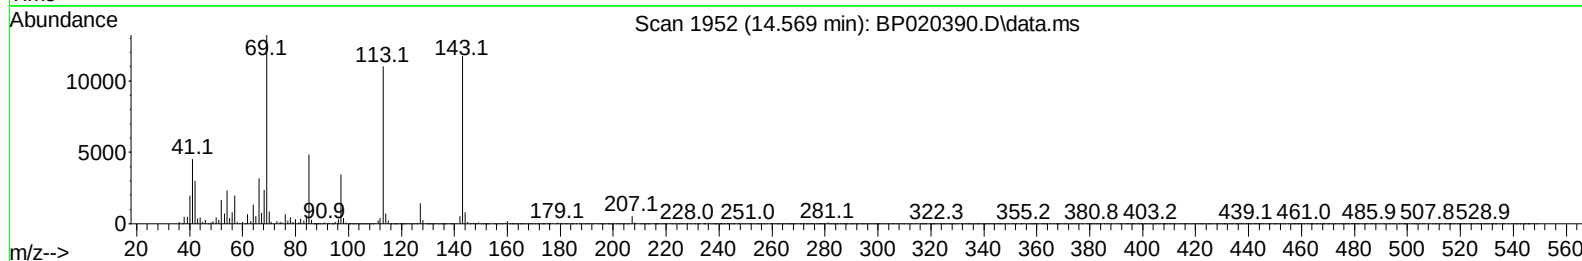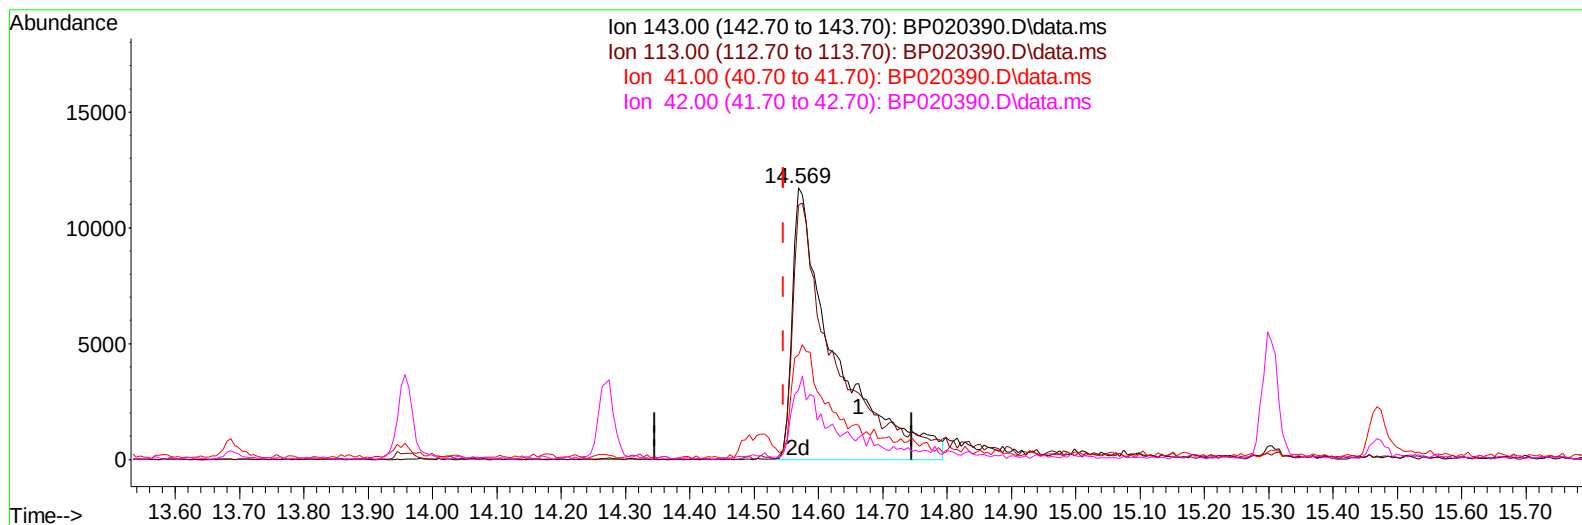

TIC: BP020390.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.569min (+ 0.024) 24.82 ng/ul m

response 53848

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	93.76
41.00	50.30	38.67#
42.00	32.50	25.70#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020390.D
 Acq On : 15 May 2024 07:28
 Operator : MA/JU
 Sample : P2372-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

Quant Time: May 15 08:02:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	65749	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136	264042	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.275	164	193304	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.116	188	452489	20.000	ng/ul	0.00
79) Chrysene-d12	21.604	240	501118	20.000	ng/ul	0.00
88) Perylene-d12	24.957	264	558384	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	7961	5.114	ng/uL	0.00
4) Pyridine-d5	3.599	84	86995	19.232	ng/ul	0.00
7) Phenol-d5	6.787	99	121312	21.485	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.946	67	78863	22.992	ng/ul	0.00
11) 2-Chlorophenol-d4	7.134	132	103009	25.519	ng/ul	0.00
15) 4-Methylphenol-d8	8.304	113	95337	20.884	ng/ul	0.00
21) Nitrobenzene-d5	8.752	128	52190	26.396	ng/ul	0.00
24) 2-Nitrophenol-d4	9.463	143	58634	25.896	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.010	165	101524m	24.571	ng/ul	0.00
31) 4-Chloroaniline-d4	10.528	131	133677	23.116	ng/ul	0.00
46) Dimethylphthalate-d6	13.687	166	412589	29.228	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	437180	28.036	ng/ul	0.00
54) 4-Nitrophenol-d4	14.569	143	53848m	24.820	ng/ul	0.02
60) Fluorene-d10	15.304	176	346099	29.395	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.469	200	56041	19.517	ng/ul	0.01
73) Anthracene-d10	17.228	188	605263	30.920	ng/ul	0.01
81) Pyrene-d10	19.616	212	808587	27.604	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.721	264	827263	30.641	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020390.D
Acq On : 15 May 2024 07:28
Operator : MA/JU
Sample : P2372-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43W7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/15/2024
Supervised By :mohammad ahmed 05/17/2024

Quant Time: May 15 08:02:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 14 23:58:44 2024
Response via : Initial Calibration

