




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020396.D
 Acq On : 15 May 2024 11:52
 Operator : MA/JU
 Sample : P2372-10
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W0

Manual IntegrationsAPPROVED

Quant Time: May 15 12:22:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

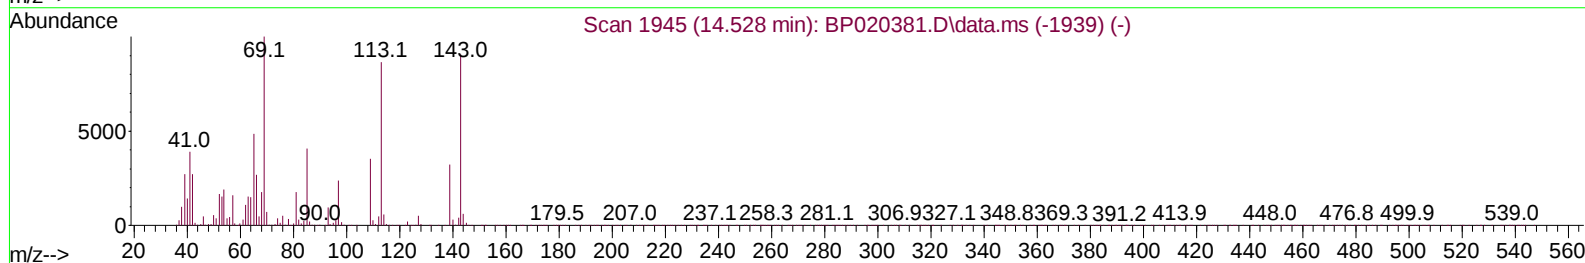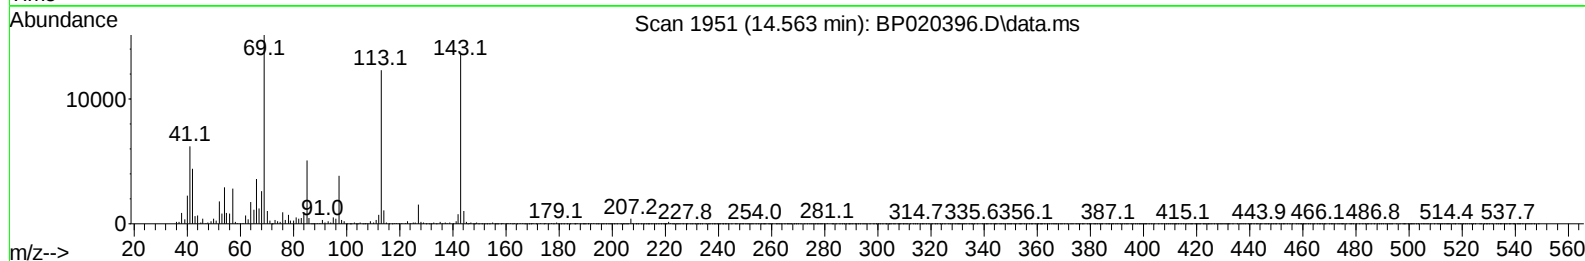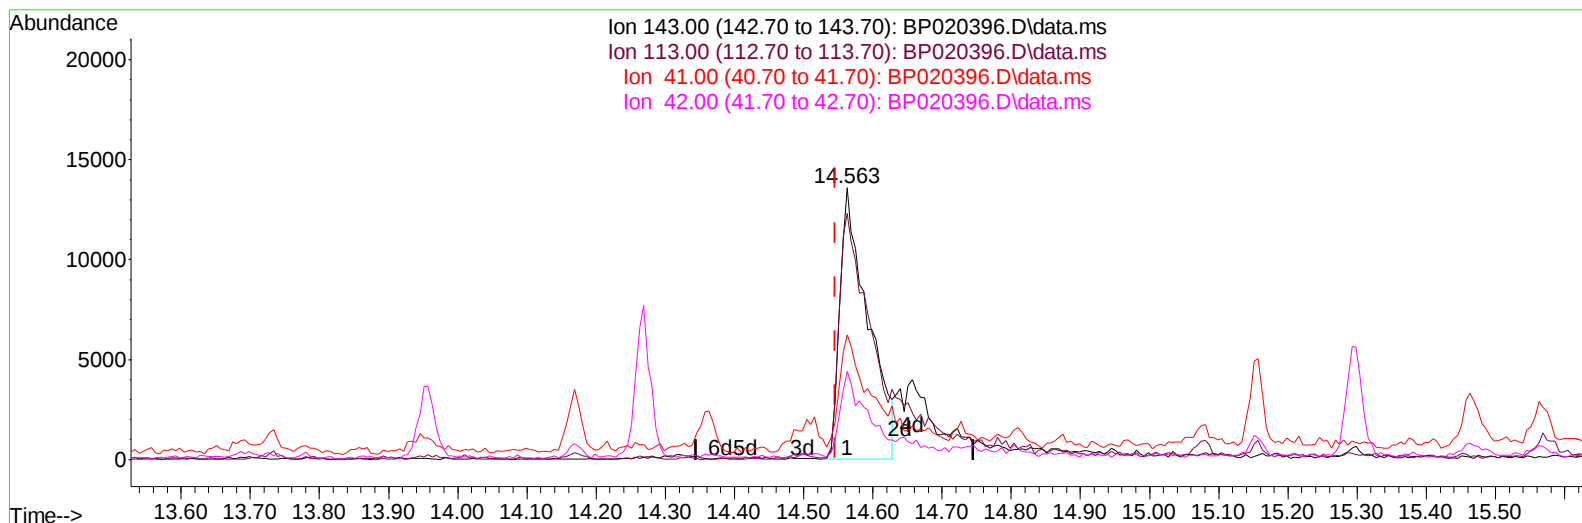

TIC: BP020396.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.563min (+ 0.018) 10.35 ng/u1

response 38129

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	90.64
41.00	50.30	45.79
42.00	32.50	32.48




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020396.D
 Acq On : 15 May 2024 11:52
 Operator : MA/JU
 Sample : P2372-10
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W0

Manual IntegrationsAPPROVED

Quant Time: May 15 12:22:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

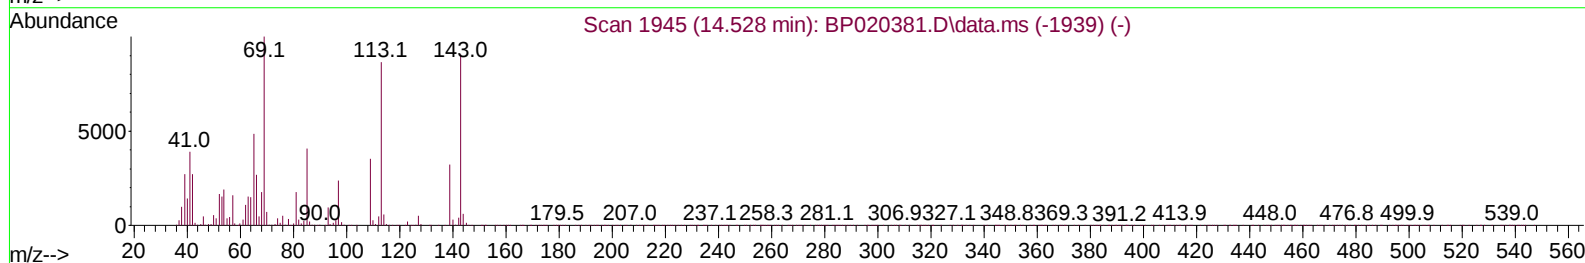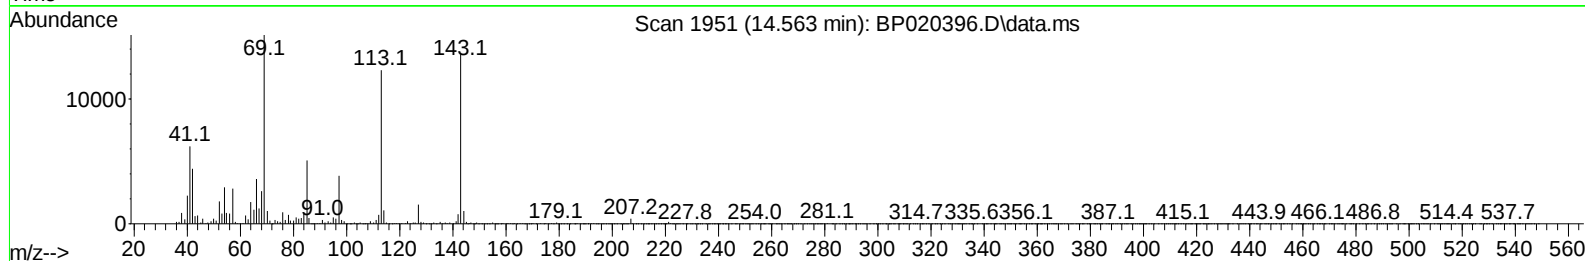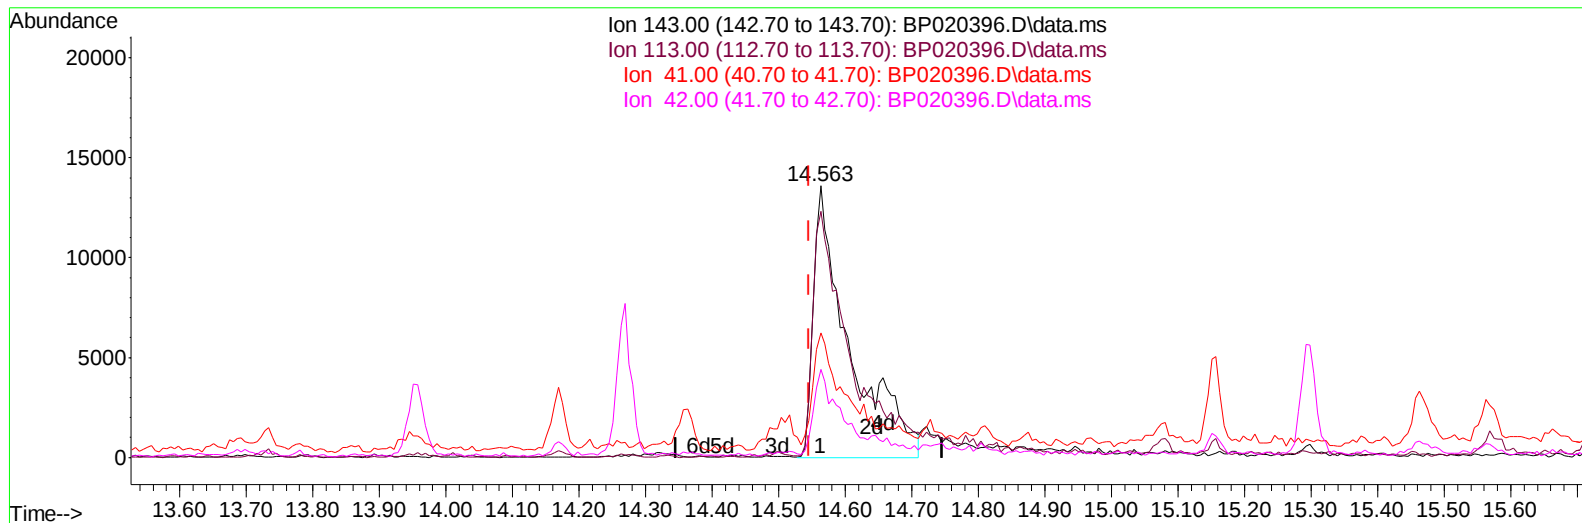

TIC: BP020396.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.563min (+ 0.018) 13.75 ng/ul m

response 50680

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	90.64
41.00	50.30	45.79
42.00	32.50	32.48

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020396.D
 Acq On : 15 May 2024 11:52
 Operator : MA/JU
 Sample : P2372-10
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

Quant Time: May 15 12:24:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.593	152		100619	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136		441779	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.269	164		328346	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.116	188		740982	20.000	ng/ul	0.00
79) Chrysene-d12	21.610	240		732439	20.000	ng/ul	0.00
88) Perylene-d12	24.956	264		819404	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.193	96		5361	2.250	ng/uL	0.00
4) Pyridine-d5	3.605	84		35881	5.183	ng/ul	0.00
7) Phenol-d5	6.787	99		98501	11.399	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.952	67		65162	12.414	ng/ul	0.00
11) 2-Chlorophenol-d4	7.134	132		84568	13.690	ng/ul	0.00
15) 4-Methylphenol-d8	8.322	113		35886	5.137	ng/ul	0.01
21) Nitrobenzene-d5	8.763	128		44777	13.535	ng/ul	0.00
24) 2-Nitrophenol-d4	9.469	143		49880	13.167	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.022	165		89284	12.915	ng/ul	0.02
31) 4-Chloroaniline-d4	10.546	131		66769	6.901	ng/ul	0.02
46) Dimethylphthalate-d6	13.687	166		382727	15.962	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160		404820	15.283	ng/ul	0.00
54) 4-Nitrophenol-d4	14.563	143		50680m	13.752	ng/ul	0.02
60) Fluorene-d10	15.298	176		335508	16.776	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.463	200		55733	11.853	ng/ul	0.00
73) Anthracene-d10	17.222	188		529164	16.508	ng/ul	0.00
81) Pyrene-d10	19.616	212		702313	16.404	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.727	264		683689	17.257	ng/ul	0.01
Target Compounds							
						Qvalue	
71) Pentachlorophenol	16.775	266		11580	2.061	ng/ul	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020396.D
Acq On : 15 May 2024 11:52
Operator : MA/JU
Sample : P2372-10
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43W0

Manual IntegrationsAPPROVED

Quant Time: May 15 12:24:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 14 23:58:44 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
Supervised By :mohammad ahmed 05/17/2024

