




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020400.D
 Acq On : 15 May 2024 14:47
 Operator : MA/JU
 Sample : P2372-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W7

Manual IntegrationsAPPROVED

Quant Time: May 15 15:14:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

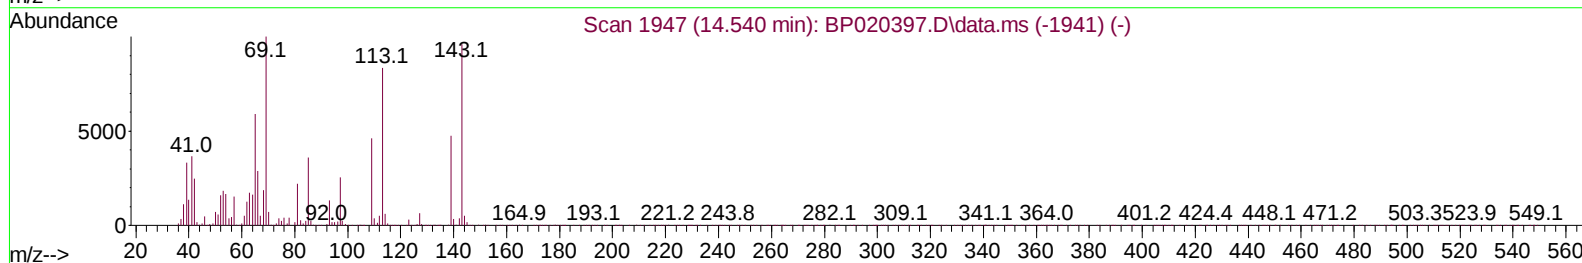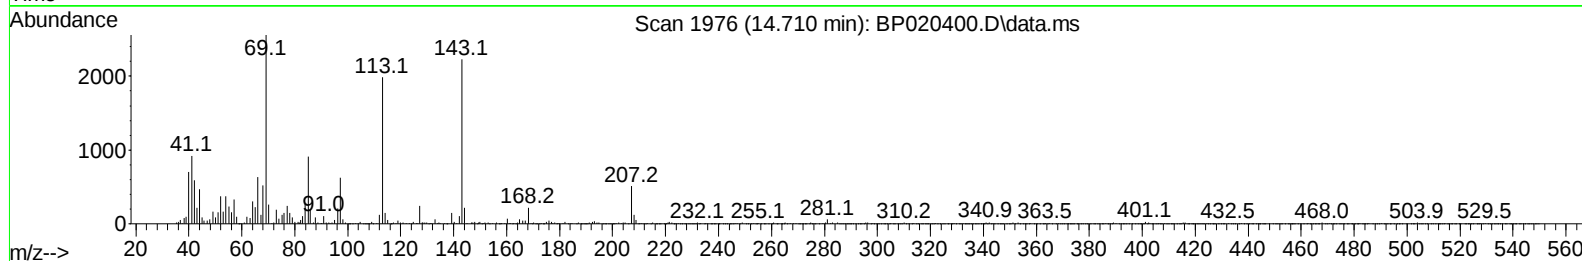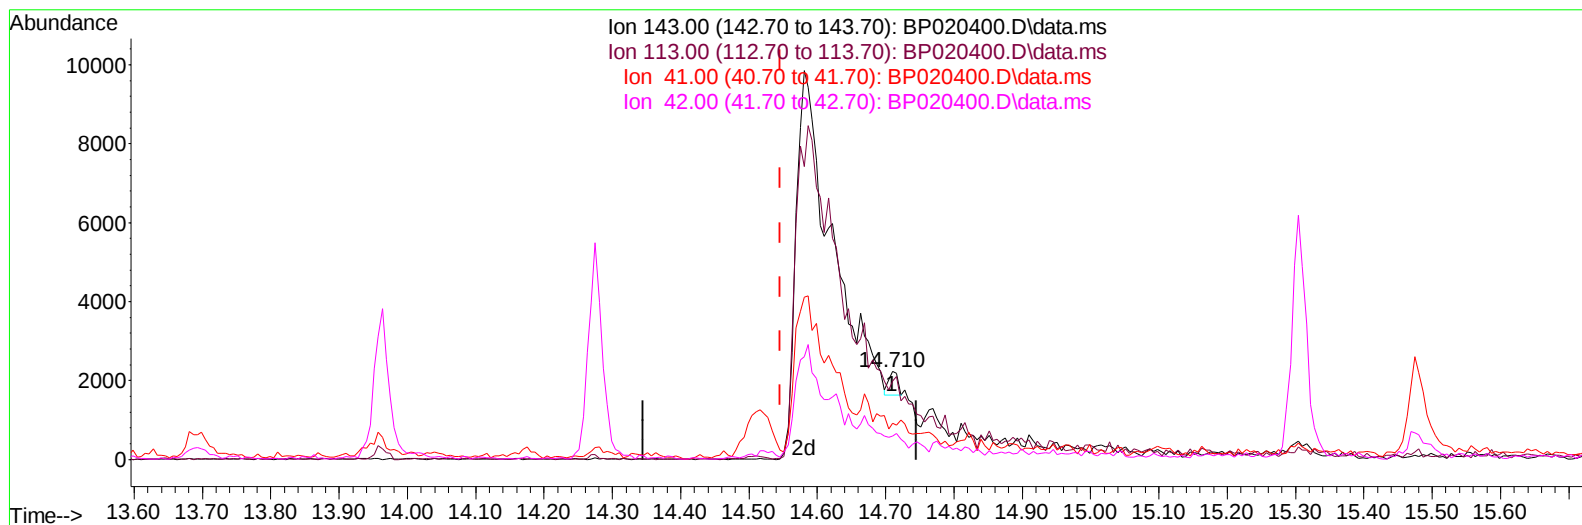

TIC: BP020400.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.710min (+ 0.165) 0.21 ng/ul

response 546

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	89.04
41.00	50.30	41.42
42.00	32.50	26.46




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020400.D
 Acq On : 15 May 2024 14:47
 Operator : MA/JU
 Sample : P2372-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W7

Manual IntegrationsAPPROVED

Quant Time: May 15 15:14:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

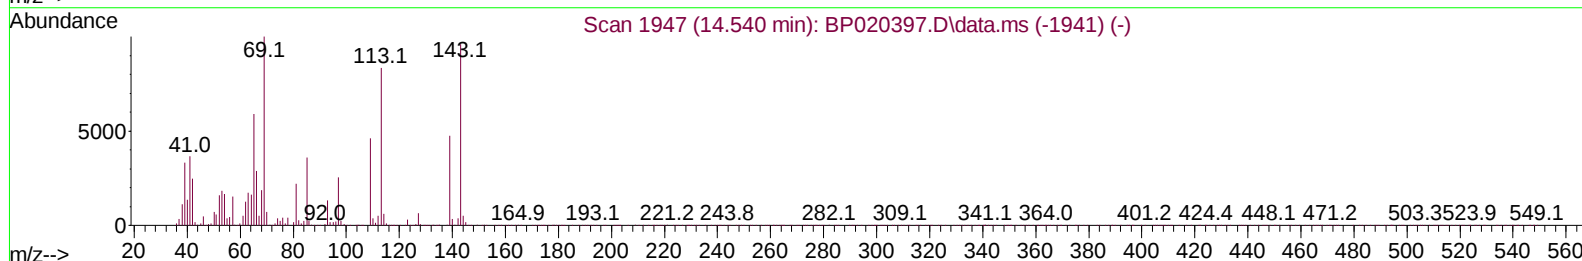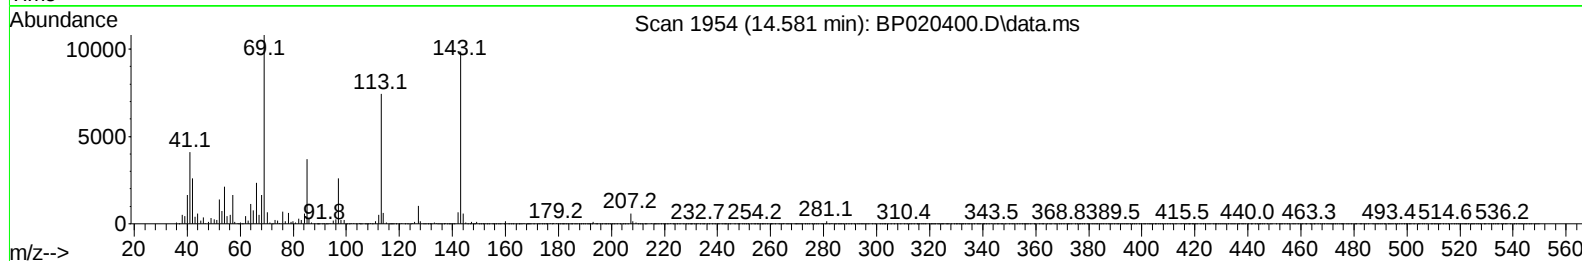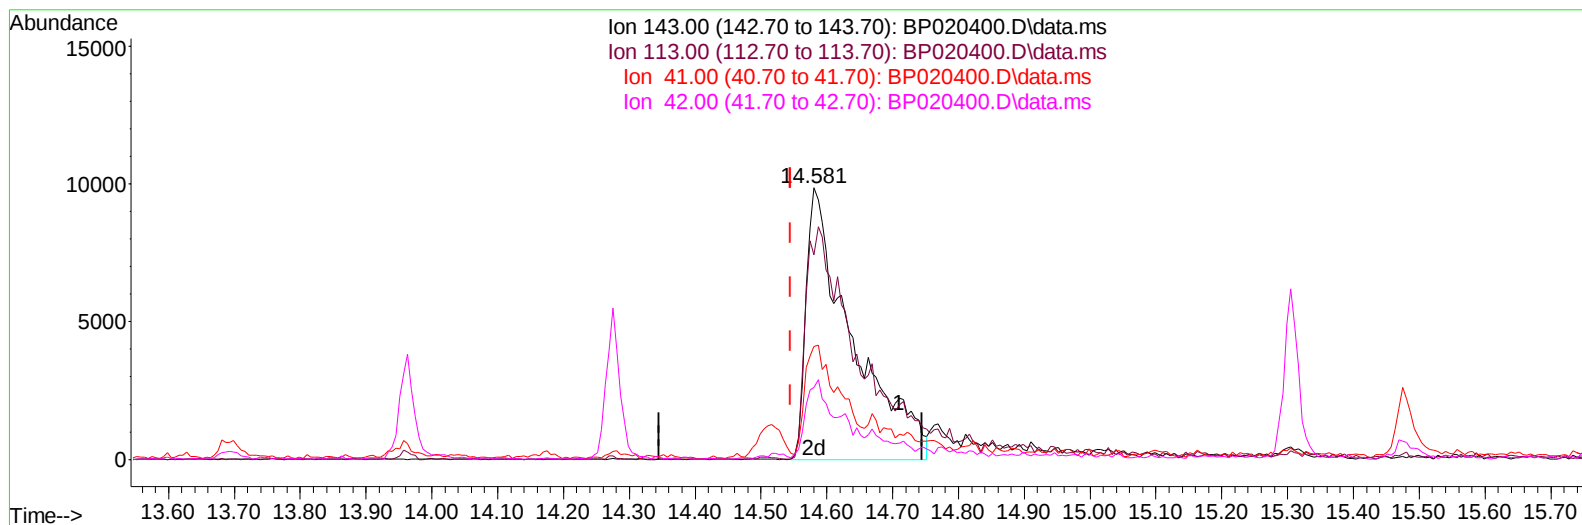

TIC: BP020400.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.581min (+ 0.035) 18.27 ng/ul m

response 47530

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	75.32#
41.00	50.30	41.66
42.00	32.50	26.48

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020400.D
 Acq On : 15 May 2024 14:47
 Operator : MA/JU
 Sample : P2372-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

Quant Time: May 15 15:15:35 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	79183	20.000	ng/ul	0.00
20) Naphthalene-d8	10.352	136	316260	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.275	164	231829	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.128	188	571929	20.000	ng/ul	0.02
79) Chrysene-d12	21.604	240	632376	20.000	ng/ul	0.00
88) Perylene-d12	24.963	264	712822	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	6558	3.498	ng/uL	0.00
4) Pyridine-d5	3.599	84	76457	14.034	ng/ul	0.00
7) Phenol-d5	6.787	99	115662	17.009	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.946	67	72784	17.620	ng/ul	0.00
11) 2-Chlorophenol-d4	7.128	132	97718	20.101	ng/ul	0.00
15) 4-Methylphenol-d8	8.305	113	92968	16.910	ng/ul	0.00
21) Nitrobenzene-d5	8.752	128	47192	19.927	ng/ul	0.00
24) 2-Nitrophenol-d4	9.469	143	51848	19.118	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.005	165	92283	18.647	ng/ul	0.00
31) 4-Chloroaniline-d4	10.534	131	129157	18.647	ng/ul	0.00
46) Dimethylphthalate-d6	13.693	166	398229	23.523	ng/ul	0.00
49) Acenaphthylene-d8	13.963	160	415038	22.193	ng/ul	0.00
54) 4-Nitrophenol-d4	14.581	143	47530m	18.267	ng/ul	0.04
60) Fluorene-d10	15.304	176	335982	23.794	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200	52505	14.467	ng/ul	0.02
73) Anthracene-d10	17.228	188	592502	23.947	ng/ul	0.01
81) Pyrene-d10	19.622	212	796510	21.547	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.727	264	806632	23.404	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020400.D
Acq On : 15 May 2024 14:47
Operator : MA/JU
Sample : P2372-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43W7

Manual IntegrationsAPPROVED

Quant Time: May 15 15:15:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 14 23:58:44 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
Supervised By :mohammad ahmed 05/17/2024

