




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020401.D
 Acq On : 15 May 2024 15:31
 Operator : MA/JU
 Sample : P2372-20
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43X0

Manual IntegrationsAPPROVED

Quant Time: May 15 16:09:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

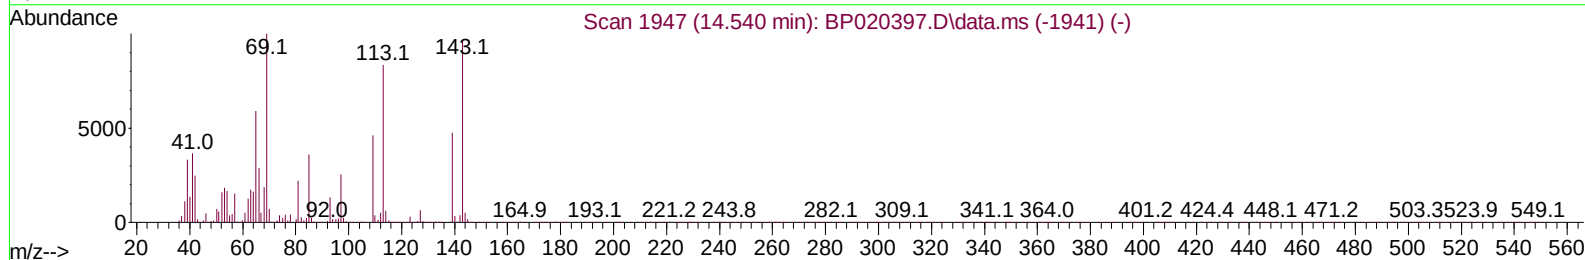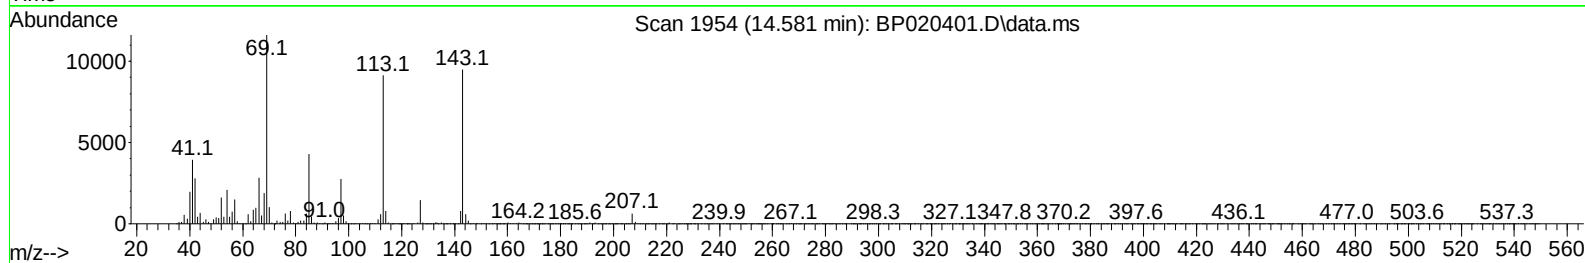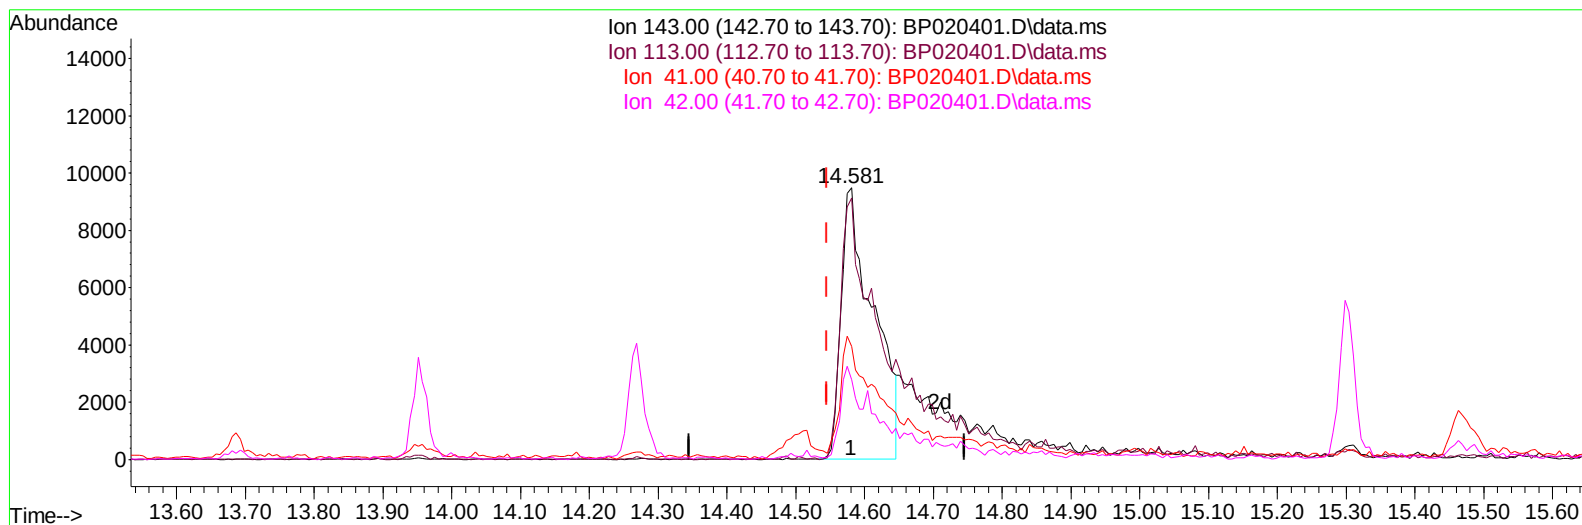

TIC: BP020401.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.581min (+ 0.035) 14.14 ng/ul

response 30692

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	96.21
41.00	50.30	41.68
42.00	32.50	29.48




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020401.D
 Acq On : 15 May 2024 15:31
 Operator : MA/JU
 Sample : P2372-20
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43X0

Manual IntegrationsAPPROVED

Quant Time: May 15 16:09:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

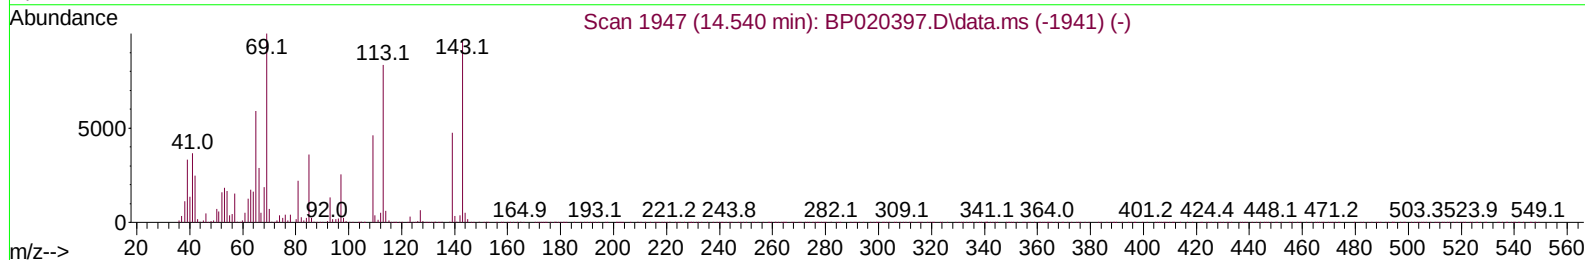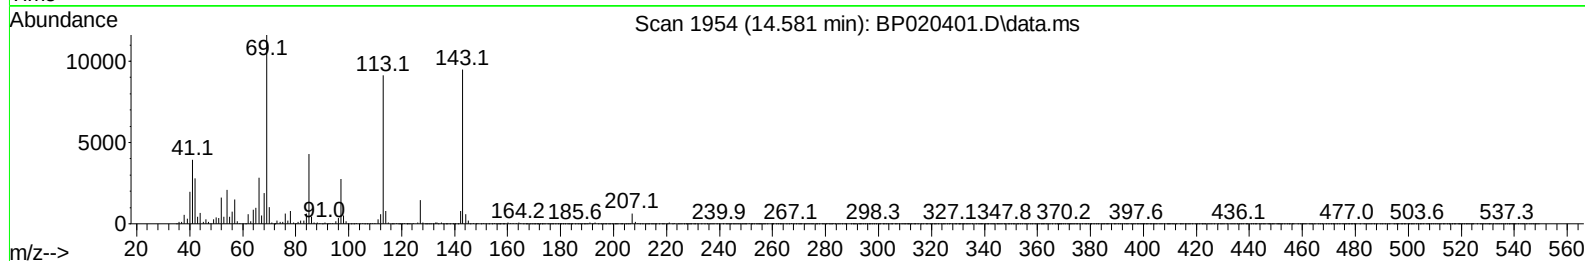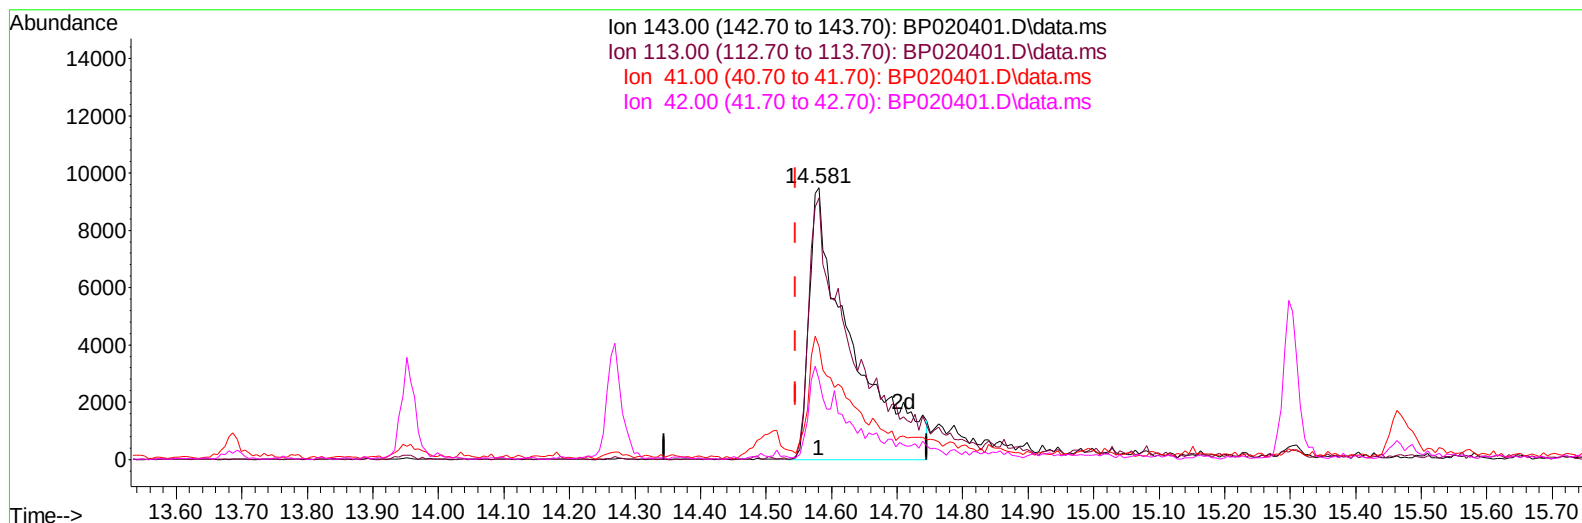

TIC: BP020401.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.581min (+ 0.035) 19.60 ng/ul m

response 42532

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	101.40	96.21
41.00	50.30	41.68
42.00	32.50	29.48

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020401.D
 Acq On : 15 May 2024 15:31
 Operator : MA/JU
 Sample : P2372-20
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43X0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/15/2024
 Supervised By :mohammad ahmed 05/17/2024

Quant Time: May 15 16:13:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 14 23:58:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	68236	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136	273287	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.269	164	193357	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.116	188	435019	20.000	ng/ul	0.00
79) Chrysene-d12	21.610	240	524122	20.000	ng/ul	0.00
88) Perylene-d12	24.974	264	639109	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	6893	4.266	ng/uL	0.00
4) Pyridine-d5	3.599	84	86710	18.470	ng/ul	0.00
7) Phenol-d5	6.787	99	119851	20.452	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.946	67	75606	21.239	ng/ul	0.00
11) 2-Chlorophenol-d4	7.134	132	100483	23.986	ng/ul	0.00
15) 4-Methylphenol-d8	8.310	113	92778	19.583	ng/ul	0.00
21) Nitrobenzene-d5	8.757	128	47782	23.349	ng/ul	0.00
24) 2-Nitrophenol-d4	9.469	143	55124	23.522	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.010	165	90529	21.169	ng/ul	0.00
31) 4-Chloroaniline-d4	10.534	131	125003	20.885	ng/ul	0.00
46) Dimethylphthalate-d6	13.687	166	361979	25.636	ng/ul	0.00
49) Acenaphthylene-d8	13.951	160	384042	24.621	ng/ul	0.00
54) 4-Nitrophenol-d4	14.581	143	42532m	19.599	ng/ul	0.04
60) Fluorene-d10	15.304	176	310869	26.396	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.469	200	47225	17.107	ng/ul	0.01
73) Anthracene-d10	17.228	188	500743	26.608	ng/ul	0.01
81) Pyrene-d10	19.622	212	698952	22.814	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.733	264	818857	26.499	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020401.D
Acq On : 15 May 2024 15:31
Operator : MA/JU
Sample : P2372-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43X0

Manual IntegrationsAPPROVED

Quant Time: May 15 16:13:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 14 23:58:44 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/15/2024
Supervised By :mohammad ahmed 05/17/2024

