

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
 Data File : BP020382.D
 Acq On : 15 May 2024 01:41
 Operator : MA/JU
 Sample : PB160788BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK788

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020382.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	15	18	23	rVB	22227	30076	1.28%	0.129%
2	3.599	84	87	102	rBV	211489	417767	17.84%	1.787%
3	3.887	132	136	140	rVB3	8798	12645	0.54%	0.054%
4	6.787	622	629	650	rBV	254591	555026	23.70%	2.374%
5	6.946	650	656	671	rVV	215969	394436	16.84%	1.687%
6	7.128	681	687	703	rBV	292812	560692	23.94%	2.398%
7	7.593	758	766	781	rBV	281608	536252	22.90%	2.294%
8	8.305	881	887	904	rBV	300954	668544	28.55%	2.859%
9	8.757	955	964	979	rBV	282801	548544	23.42%	2.346%
10	9.469	1073	1085	1104	rBV	219938	492170	21.02%	2.105%
11	10.010	1169	1177	1215	rBV	260036	707108	30.19%	3.024%
12	10.363	1229	1237	1252	rBV	396039	737810	31.50%	3.156%
13	10.540	1259	1267	1301	rBV	214285	676185	28.87%	2.892%
14	12.022	1512	1519	1521	rBV7	3518	7531	0.32%	0.032%
15	12.093	1526	1531	1535	rVB6	1367	2925	0.12%	0.013%
16	12.287	1563	1564	1571	rVB7	2286	3276	0.14%	0.014%
17	12.457	1589	1593	1595	rBV5	2749	3678	0.16%	0.016%
18	12.734	1636	1640	1648	rBV5	1367	3565	0.15%	0.015%
19	13.063	1691	1696	1700	rBV6	2701	4362	0.19%	0.019%
20	13.104	1700	1703	1708	rVV6	2854	5513	0.24%	0.024%
21	13.157	1708	1712	1720	rVB7	3254	6035	0.26%	0.026%
22	13.687	1791	1802	1825	rBV	627785	1120985	47.87%	4.794%
23	13.957	1840	1848	1864	rVV2	741713	1224566	52.29%	5.237%
24	14.269	1894	1901	1910	rVV	665844	1024101	43.73%	4.380%
25	14.334	1910	1912	1921	rVB	8931	14195	0.61%	0.061%
26	14.569	1940	1952	1973	rBV4	88977	436193	18.63%	1.866%
27	14.945	2013	2016	2023	rVB8	4957	9293	0.40%	0.040%
28	15.139	2046	2049	2057	rVB2	6005	9956	0.43%	0.043%
29	15.292	2068	2075	2083	rBV	846988	1533442	65.48%	6.558%
30	15.369	2086	2088	2094	rVB6	12178	15171	0.65%	0.065%
31	15.463	2098	2104	2116	rBV	265866	510320	21.79%	2.183%
32	15.586	2123	2125	2131	rVB5	6816	9659	0.41%	0.041%
33	16.116	2211	2215	2217	rBV5	2634	3514	0.15%	0.015%
34	16.286	2241	2244	2247	rBV5	3850	4781	0.20%	0.020%
35	16.381	2256	2260	2266	rVB7	5910	8835	0.38%	0.038%
36	16.628	2297	2302	2303	rBV4	1711	2375	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020382.D
Acq On : 15 May 2024 01:41
Operator : MA/JU
Sample : PB160788BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK788

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Title : SVOA CALIBRATION

37	16.792	2324	2330	2332	rBV7	2760	4863	0.21%	0.021%
38	16.892	2343	2347	2349	rBV5	2598	3403	0.15%	0.015%
39	17.110	2378	2384	2395	rBV	867955	1345417	57.45%	5.754%
40	17.210	2395	2401	2415	rVV2	930280	1708727	72.96%	7.308%
41	18.104	2548	2553	2556	rBV7	4418	8934	0.38%	0.038%
42	19.163	2729	2733	2738	rVB4	13496	21419	0.91%	0.092%
43	19.245	2743	2747	2750	rBV4	9508	16072	0.69%	0.069%
44	19.622	2805	2811	2823	rBV2	1211856	2113659	90.25%	9.040%
45	20.804	3008	3012	3022	rVB2	46308	84937	3.63%	0.363%
46	21.604	3142	3148	3164	rBV2	865130	1690225	72.17%	7.229%
47	24.727	3669	3679	3695	rVB2	788592	2341915	100.00%	10.016%
48	24.951	3708	3717	3731	rBV	618603	1739960	74.30%	7.442%




Sum of corrected areas: 23381057

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020382.D
Acq On : 15 May 2024 01:41
Operator : MA/JU
Sample : PB160788BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK788

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

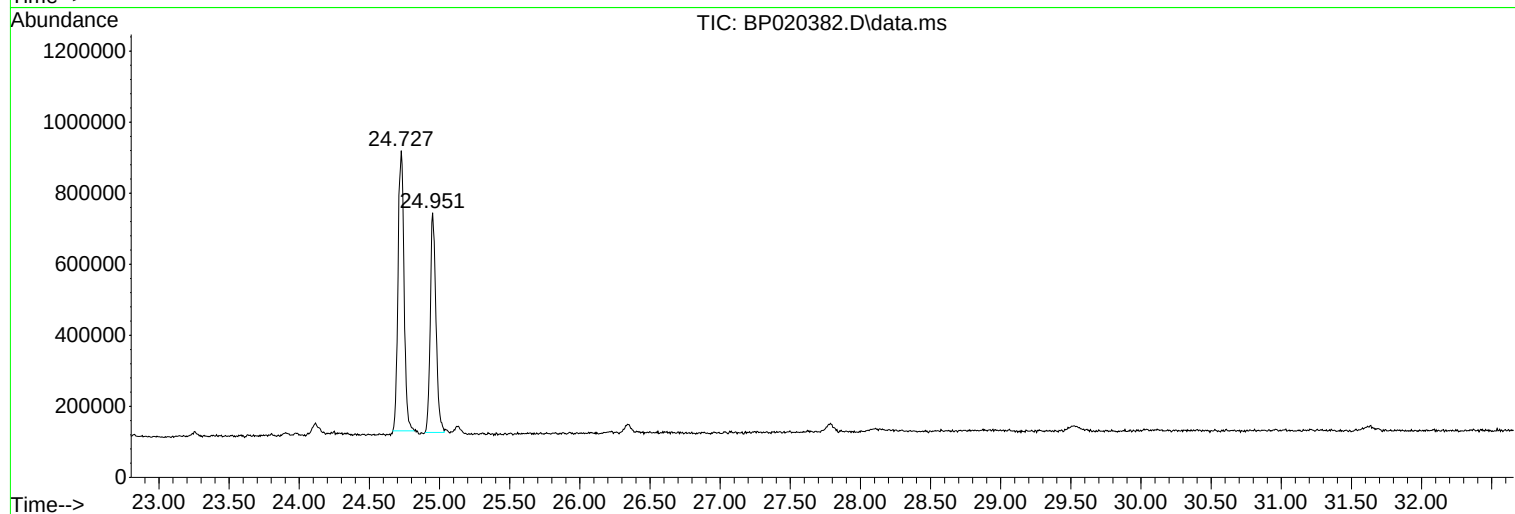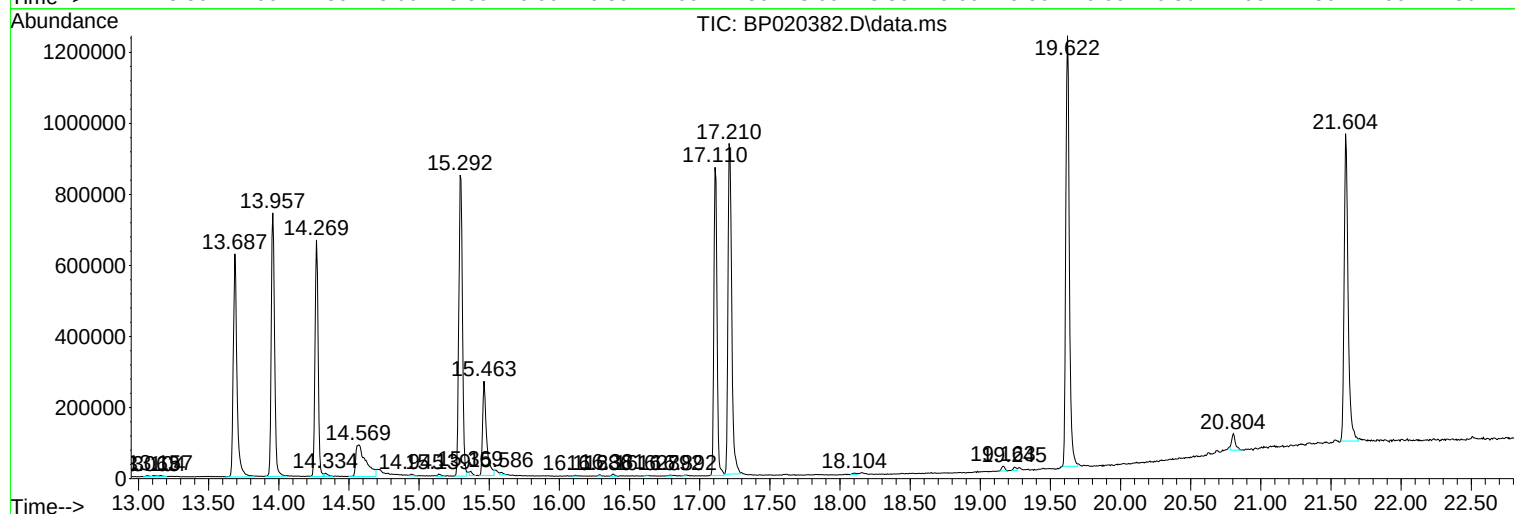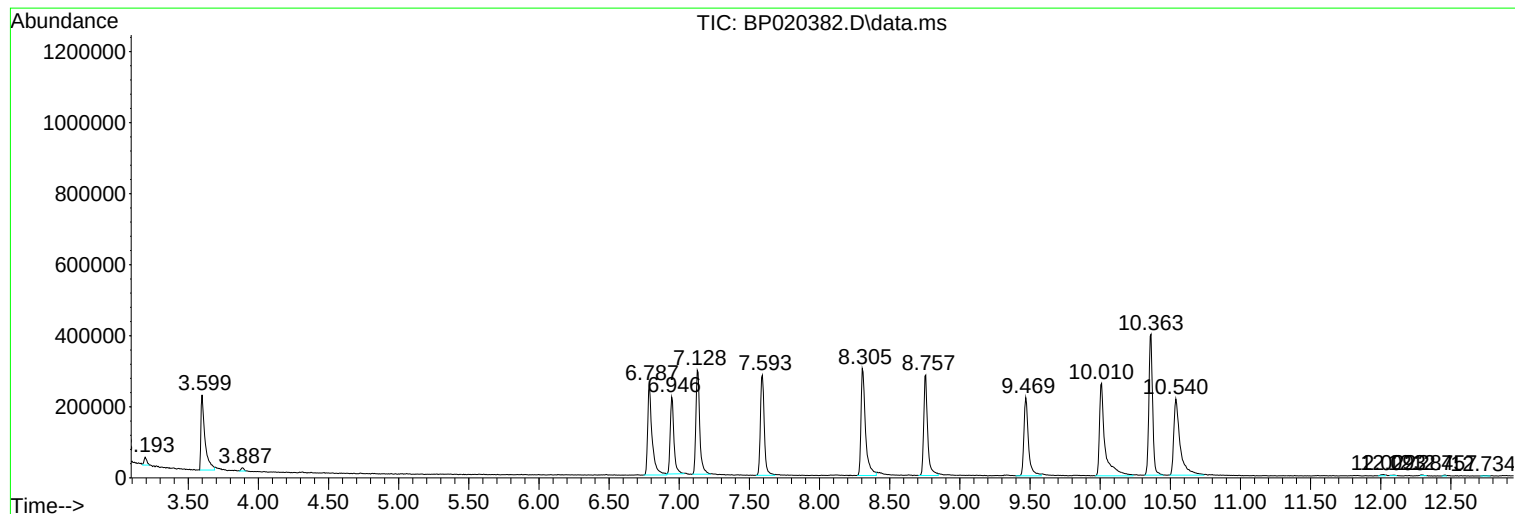

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020382.D
Acq On : 15 May 2024 01:41
Operator : MA/JU
Sample : PB160788BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK788

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051424\
Data File : BP020382.D
Acq On : 15 May 2024 01:41
Operator : MA/JU
Sample : PB160788BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK788

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP050124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------