
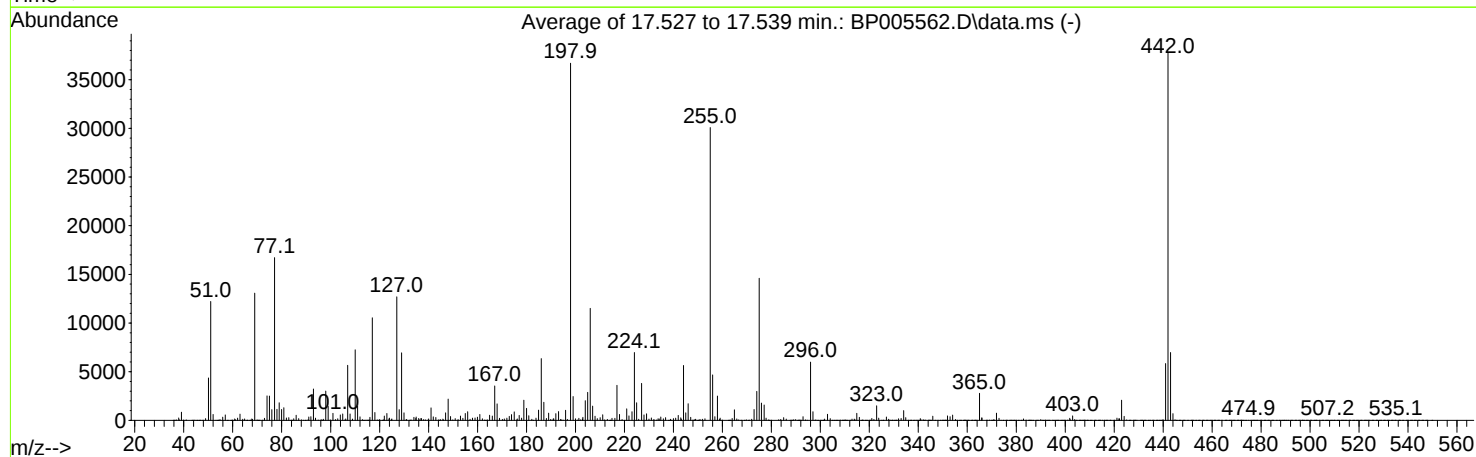


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051521\
 Data File : BP005562.D
 Acq On : 15 May 2021 10:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 17 15:35:47 2021

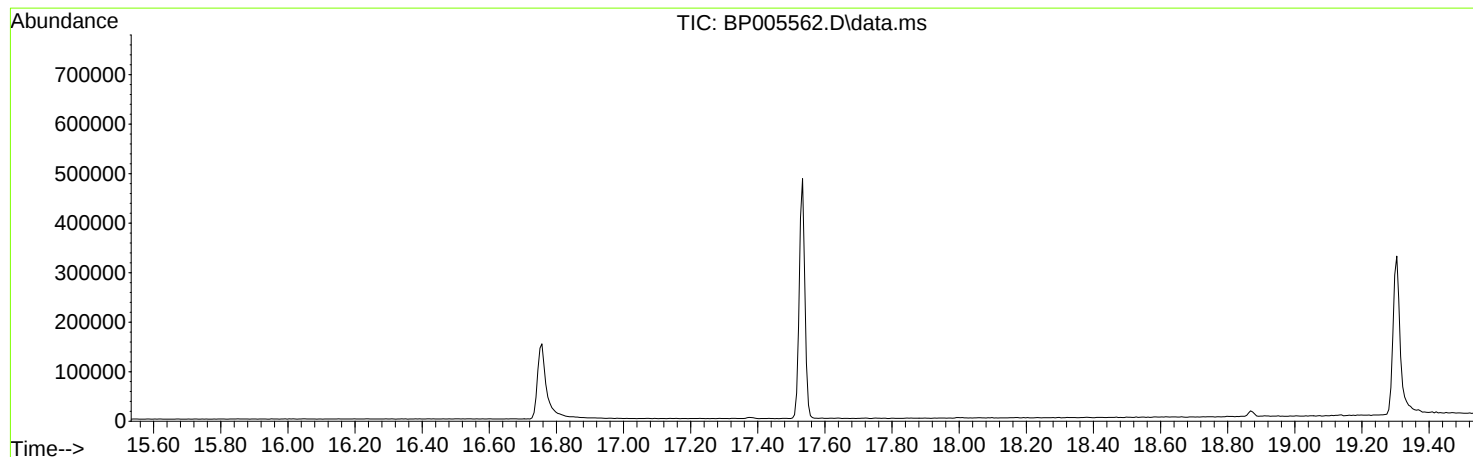

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	12209	PASS
68	69	0.00	2	1.1	142	PASS
69	198	0.00	100	35.6	13073	PASS
70	69	0.00	2	0.3	44	PASS
127	198	10	80	34.6	12697	PASS
197	198	0.00	2	0.3	94	PASS
198	198	100	100	100.0	36692	PASS
199	198	5	9	6.7	2453	PASS
275	198	10	60	39.8	14605	PASS
365	198	1	100	7.6	2773	PASS
441	198	0.01	100	15.9	5839	PASS
442	442	100	100	100.0	37792	PASS
443	442	15	24	18.5	6975	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/15/2021	BNA_P	<u>BP005562.D</u>
Compound Name	Response	Retention Time
DDT	133760	20.492
DDD	2532	20.068
DDE	639	19.562
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3171	136931	2.32

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051521\
 Data File : BP005562.D
 Acq On : 15 May 2021 10:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 16 04:06:48 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 12:01:17 2021
 Response via : Initial Calibration

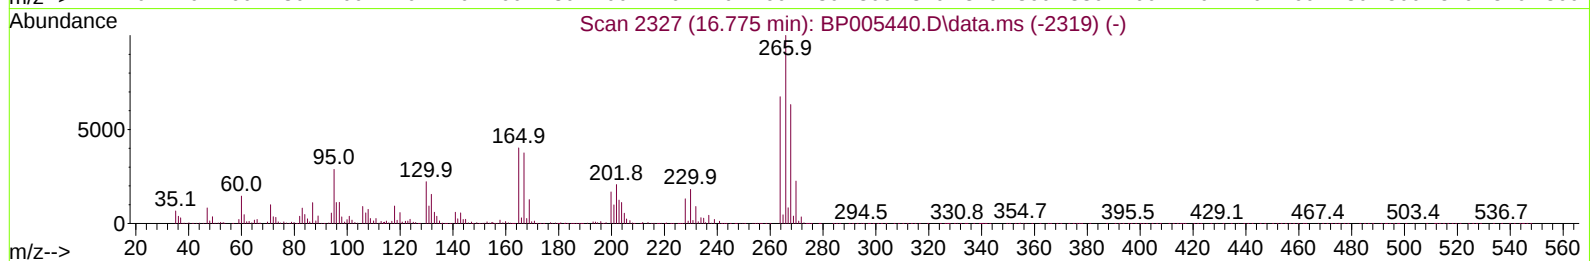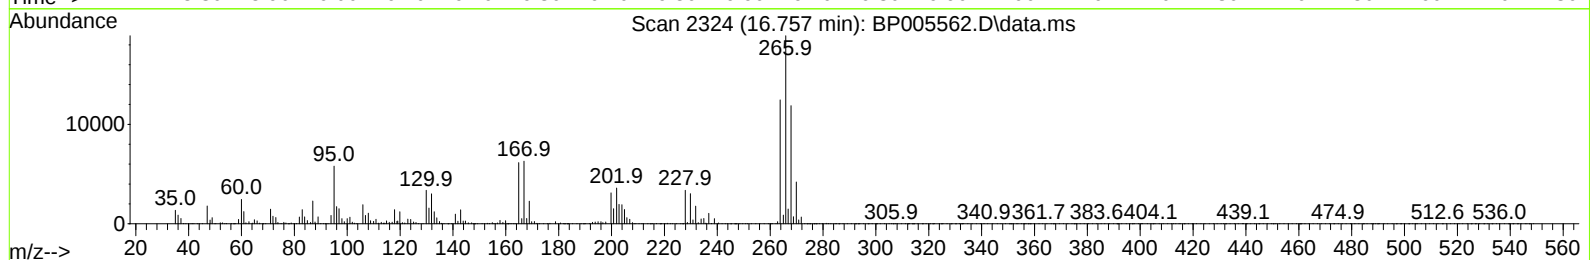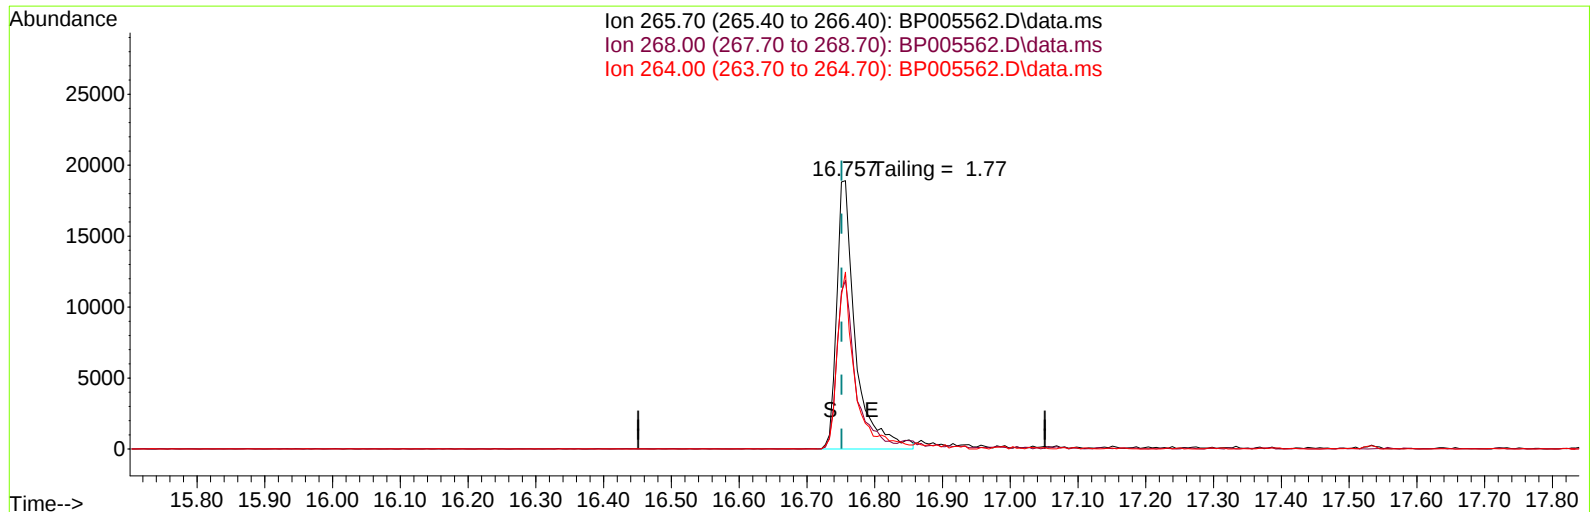

TIC: BP005562.D\data.ms

(70) Pentachlorophenol (C)

16.757min (+ 0.006) 283689.83 ng




response 35757

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	62.80
264.00	67.10	65.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051521\
 Data File : BP005562.D
 Acq On : 15 May 2021 10:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: May 16 04:06:48 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP050521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 12:01:17 2021
 Response via : Initial Calibration

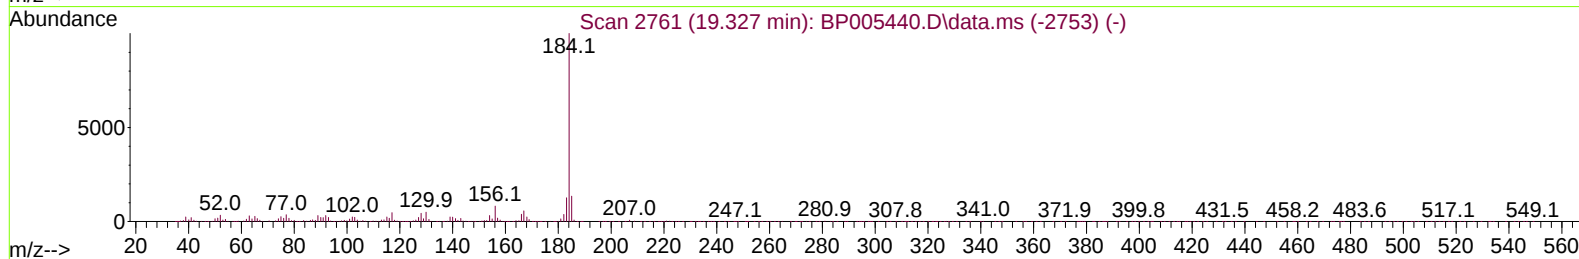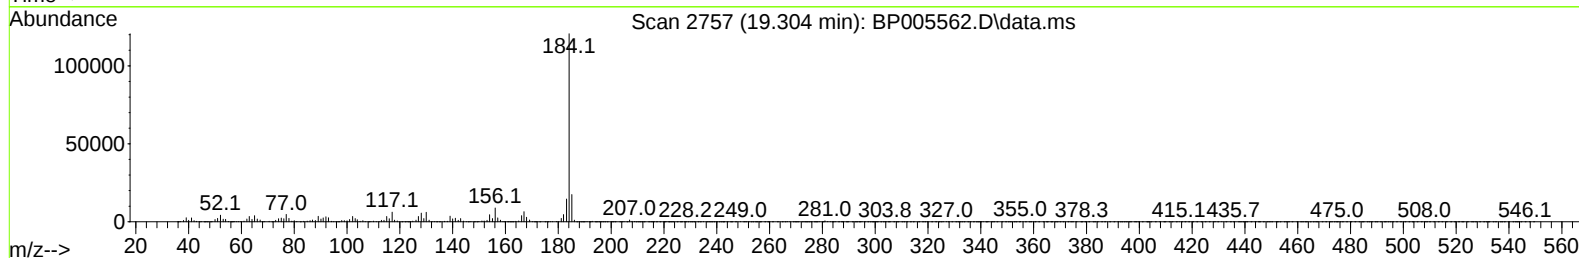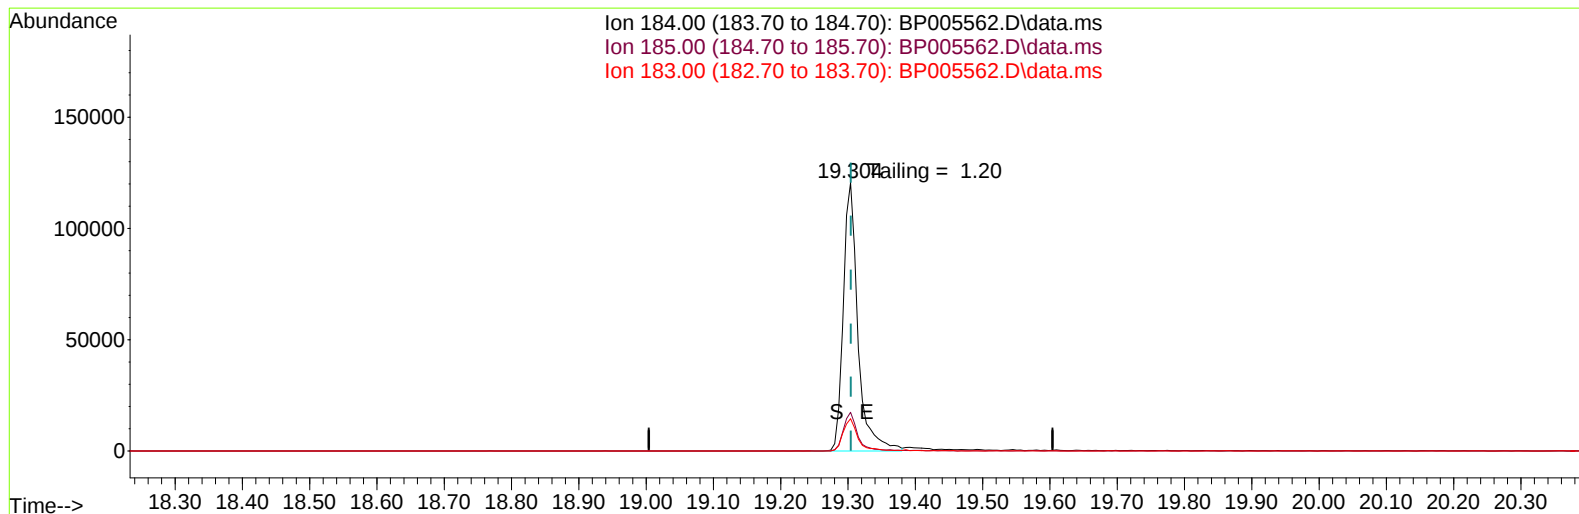

TIC: BP005562.D\data.ms

(77) Benzidine

19.304min (-0.000) 471553.73 ng

response 182477

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.43
183.00	12.30	12.08
0.00	0.00	0.00