

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015081.D
 Acq On : 15 May 2023 19:08
 Operator : CG/JU
 Sample : 02592-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREF4

Quant Time: May 16 01:41:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 16 01:39:21 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.140	152	330272	20.000	ng/ul	0.00
20) Naphthalene-d8	10.969	136	1498072	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.781	164	976369	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.533	188	2143010	20.000	ng/ul	0.00
79) Chrysene-d12	21.610	240	1849591	20.000	ng/ul	0.00
88) Perylene-d12	24.180	264	1887758	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.440	96	18147	2.135	ng/uL	0.00
4) Pyridine-d5	3.881	84	236456	9.814	ng/ul	0.00
7) Phenol-d5	7.287	99	862057	28.112	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.458	67	543161	30.669	ng/ul	0.00
11) 2-Chlorophenol-d4	7.663	132	689691	30.590	ng/ul	0.00
15) 4-Methylphenol-d8	8.846	113	745233	30.499	ng/ul	0.00
21) Nitrobenzene-d5	9.316	128	361255	30.688	ng/ul	0.00
24) 2-Nitrophenol-d4	10.040	143	408935	31.221	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.581	165	698534	29.554	ng/ul	0.00
31) 4-Chloroaniline-d4	11.104	131	1056823	30.220	ng/ul	0.00
46) Dimethylphthalate-d6	14.181	166	2372452	32.156	ng/ul	0.00
49) Acenaphthylene-d8	14.475	160	2737761	32.445	ng/ul	0.00
54) 4-Nitrophenol-d4	14.969	143	402510	28.095	ng/ul	0.00
60) Fluorene-d10	15.769	176	2029748	32.603	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.887	200	354165	26.224	ng/ul	0.00
73) Anthracene-d10	17.633	188	3187868	32.486	ng/ul	0.00
81) Pyrene-d10	19.851	212	3600399	33.563	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.015	264	3119866	33.293	ng/ul	0.00
Target Compounds						
16) Acetophenone	8.969	105	81100	2.127	ng/ul	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015081.D
Acq On : 15 May 2023 19:08
Operator : CG/JU
Sample : 02592-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREF4

Quant Time: May 16 01:41:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 16 01:39:21 2023
Response via : Initial Calibration

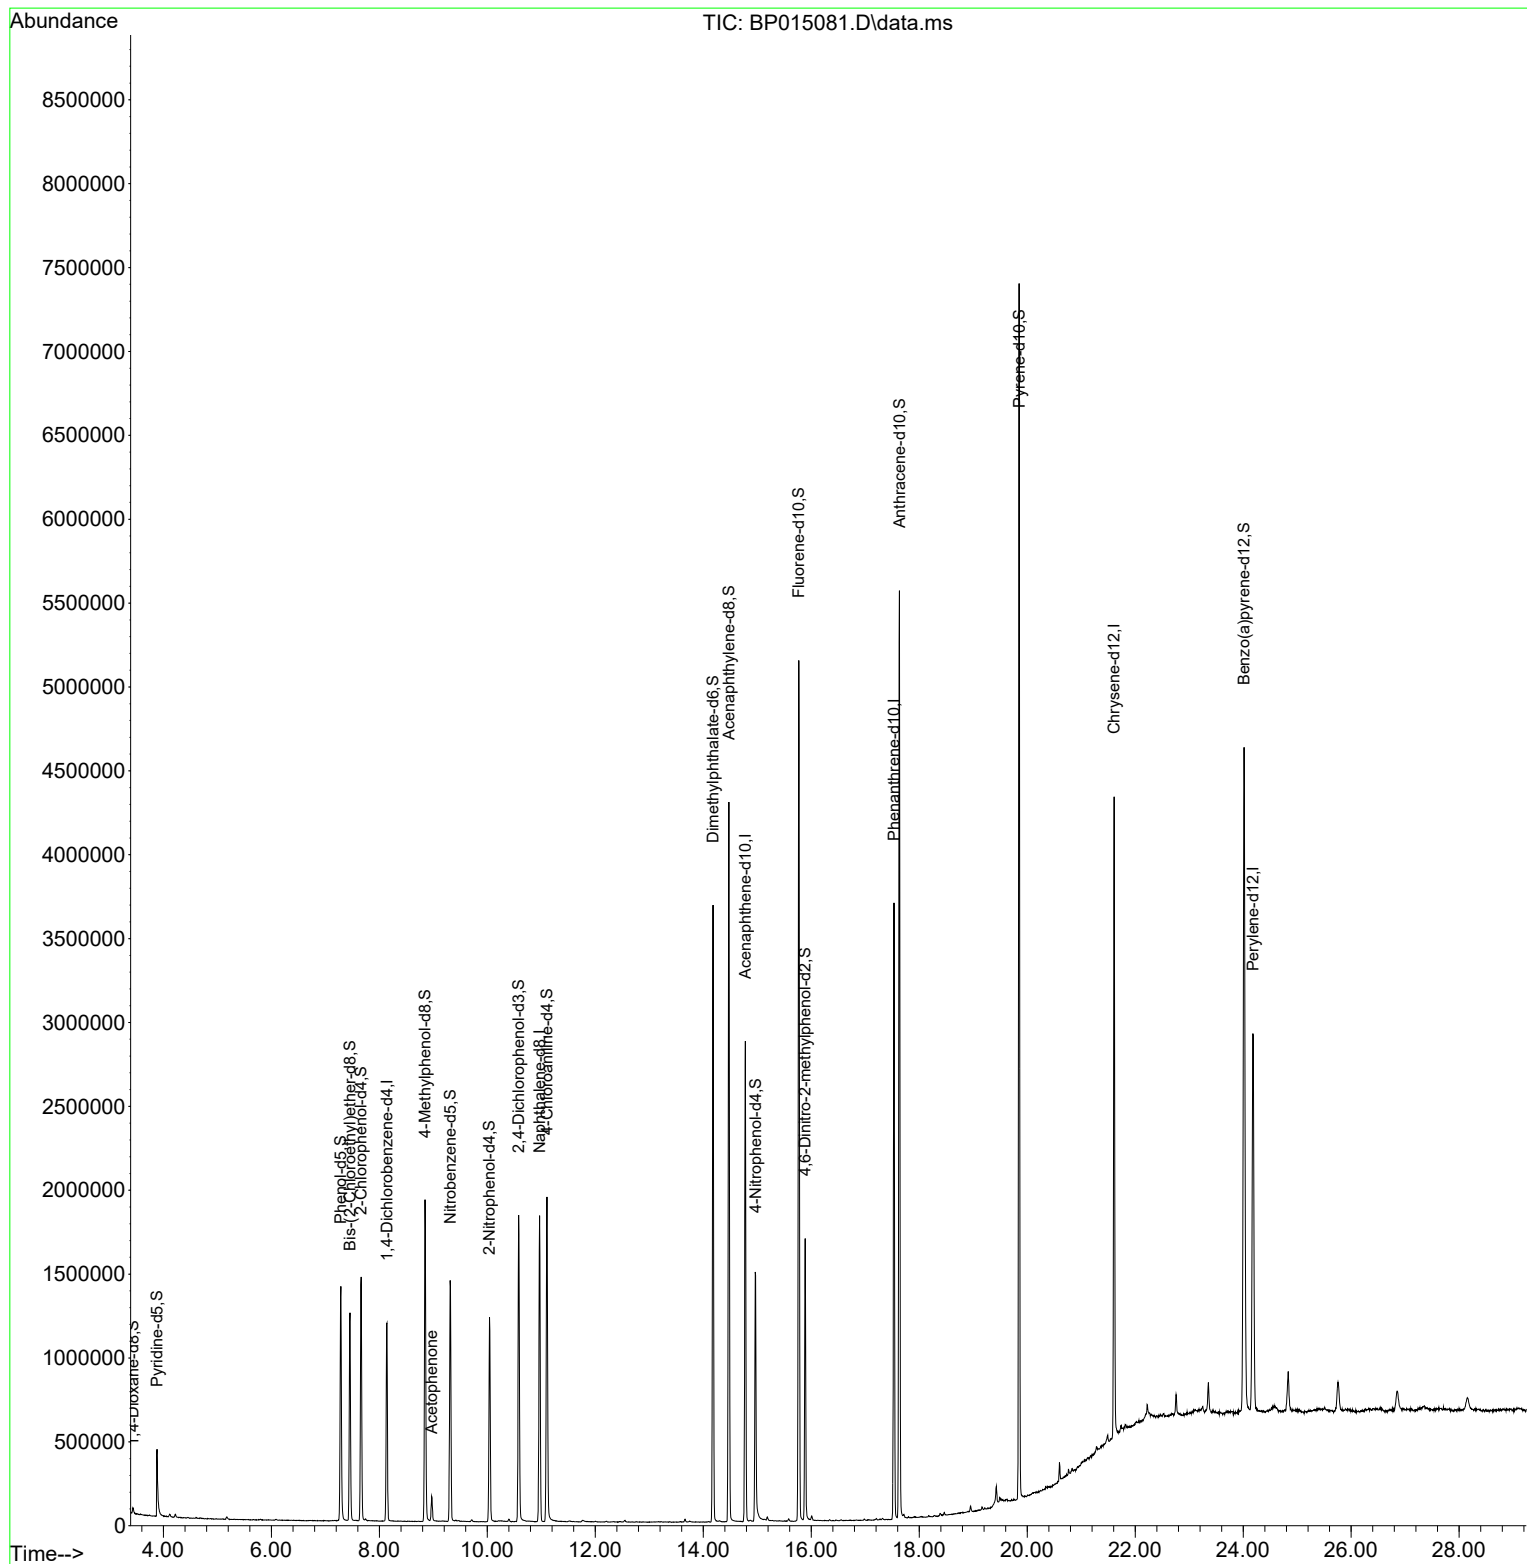

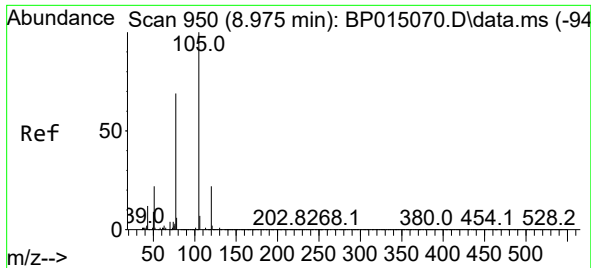

#16
 Acetophenone
 Concen: 2.127 ng/ul
 RT: 8.969 min Scan# 94
 Delta R.T. 0.000 min
 Lab File: BP015081.D
 Acq: 15 May 2023 19:08

Instrument :
 BNA_P
 ClientSampleId :
 JREF4

Tgt Ion:105 Resp: 81100
 Ion Ratio Lower Upper
 105 100
 77 78.7 59.4 89.2
 51 26.8 19.2 28.8

