

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015086.D
 Acq On : 15 May 2023 21:56
 Operator : CG/JU
 Sample : 02592-21
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREE6

Quant Time: May 16 01:42:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 16 01:39:21 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	309363	20.000	ng/ul	0.00
20) Naphthalene-d8	10.969	136	1418723	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.775	164	926703	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.533	188	2035520	20.000	ng/ul	0.00
79) Chrysene-d12	21.610	240	1735559	20.000	ng/ul	0.00
88) Perylene-d12	24.180	264	1742251	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.440	96	6019	0.756	ng/uL	0.00
4) Pyridine-d5	3.887	84	64434	2.855	ng/ul	0.01
7) Phenol-d5	7.281	99	524184	18.249	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.452	67	334453	20.161	ng/ul	0.00
11) 2-Chlorophenol-d4	7.657	132	414745	19.638	ng/ul	0.00
15) 4-Methylphenol-d8	8.846	113	457115	19.972	ng/ul	0.00
21) Nitrobenzene-d5	9.310	128	216070	19.382	ng/ul	0.00
24) 2-Nitrophenol-d4	10.040	143	237088	19.113	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.581	165	429786	19.201	ng/ul	0.00
31) 4-Chloroaniline-d4	11.104	131	608091	18.361	ng/ul	0.00
46) Dimethylphthalate-d6	14.181	166	1529520	21.842	ng/ul	0.00
49) Acenaphthylene-d8	14.469	160	1726896	21.562	ng/ul	0.00
54) 4-Nitrophenol-d4	14.963	143	235936	17.351	ng/ul	0.00
60) Fluorene-d10	15.769	176	1317714	22.300	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.886	200	198709	15.490	ng/ul	0.00
73) Anthracene-d10	17.628	188	2081278	22.329	ng/ul	0.00
81) Pyrene-d10	19.851	212	2384522	23.689	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.010	264	1975500	22.842	ng/ul	-0.01
Target Compounds						
16) Acetophenone	8.969	105	106188	2.973	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015086.D
Acq On : 15 May 2023 21:56
Operator : CG/JU
Sample : 02592-21
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREE6

Quant Time: May 16 01:42:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 16 01:39:21 2023
Response via : Initial Calibration

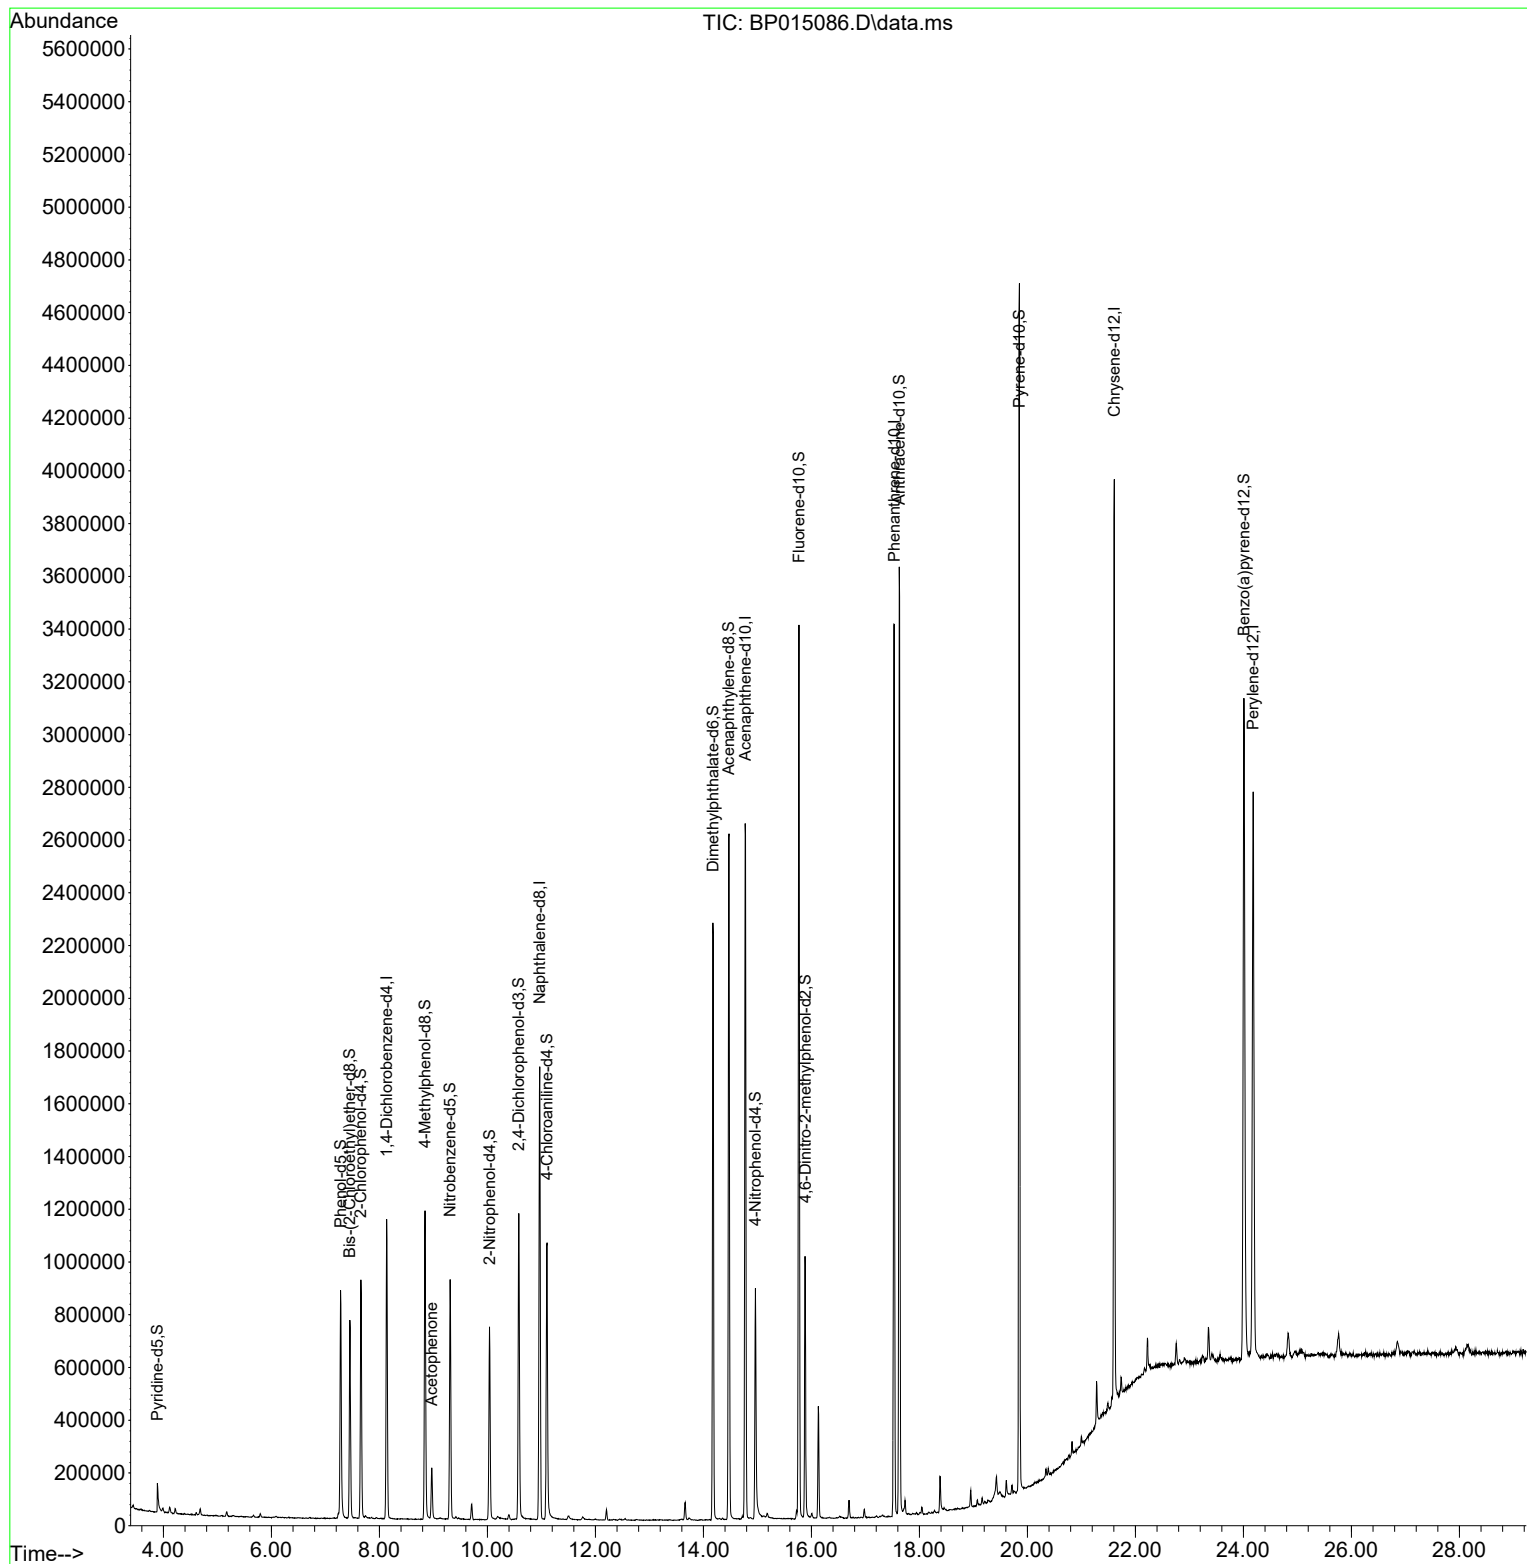

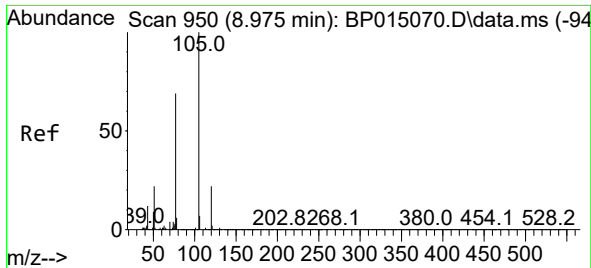

#16
 Acetophenone
 Concen: 2.973 ng/ul
 RT: 8.969 min Scan# 94
 Delta R.T. 0.000 min
 Lab File: BP015086.D
 Acq: 15 May 2023 21:56

Instrument :
 BNA_P
 ClientSampleId :
 JREE6

Tgt Ion:105 Resp: 106188
 Ion Ratio Lower Upper
 105 100
 77 74.0 59.4 89.2
 51 25.9 19.2 28.8

