

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015072.D
 Acq On : 15 May 2023 12:41
 Operator : CG/JU
 Sample : 02592-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JRED3

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 05/16/2023
 Supervised By : Yogesh Patel 05/16/2023

Quant Time: May 16 01:30:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 11 23:06:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.140	152	264631	20.000	ng/u1	0.00
20) Naphthalene-d8	10.969	136	1194934	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	800385	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.533	188	1786940	20.000	ng/u1	0.00
79) Chrysene-d12	21.610	240	1600292	20.000	ng/u1	-0.01
88) Perylene-d12	24.186	264	1763752	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	11734	1.723	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.287	99	196895	8.014	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.458	67	140505	9.901	ng/u1	0.00
11) 2-Chlorophenol-d4	7.663	132	167898	9.294	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	151444	7.735	ng/u1	-0.01
21) Nitrobenzene-d5	9.316	128	80278	8.550	ng/u1	0.00
24) 2-Nitrophenol-d4	10.046	143	82932	7.938	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	153910	8.164	ng/u1	0.00
31) 4-Chloroaniline-d4	11.104	131	195069	6.993	ng/u1	0.00
46) Dimethylphthalate-d6	14.181	166	741276	12.256	ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	728492	10.531	ng/u1	0.00
54) 4-Nitrophenol-d4	14.975	143	17201m	1.465	ng/u1	0.00
60) Fluorene-d10	15.769	176	606239	11.879	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.887	200	21980m	1.952	ng/u1	-0.01
73) Anthracene-d10	17.633	188	1038504	12.692	ng/u1	0.00
81) Pyrene-d10	19.851	212	1250779	13.476	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.015	264	1144131	13.068	ng/u1	-0.01
Target Compounds						
16) Acetophenone	8.975	105	78713	2.576	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015072.D
Acq On : 15 May 2023 12:41
Operator : CG/JU
Sample : 02592-02
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
JRED3

Quant Time: May 16 01:30:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 11 23:06:15 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/16/2023
Supervised By :Yogesh Patel 05/16/2023

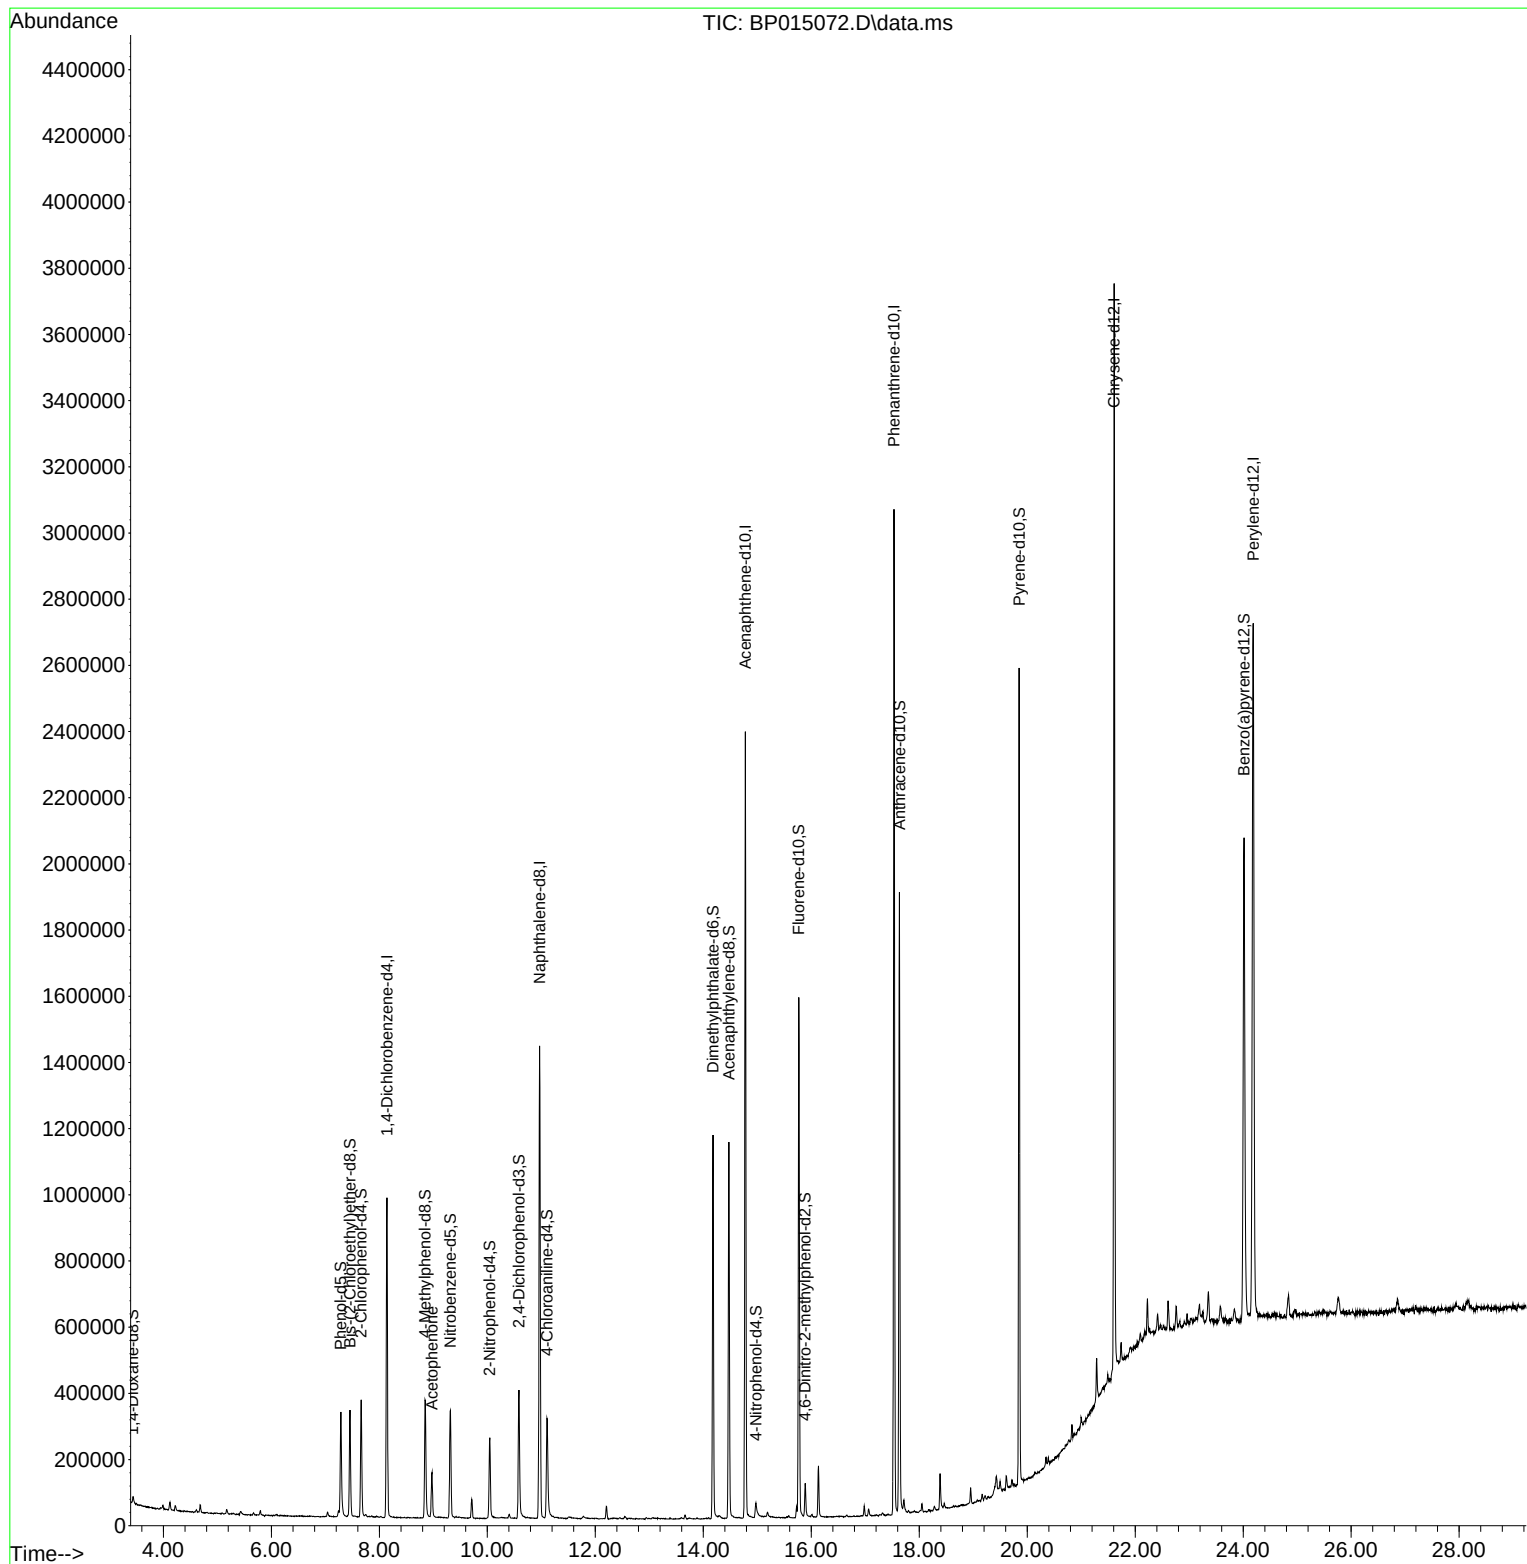

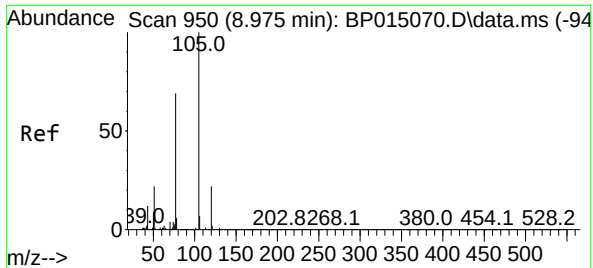

#16
Acetophenone
Concen: 2.576 ng/ul
RT: 8.975 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP015072.D
Acq: 15 May 2023 12:41

Instrument :
BNA_P
ClientSampleId :
JRED3

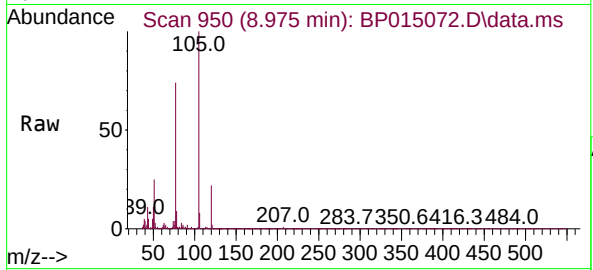

Tgt Ion:	105	Resp:	7871
Ion Ratio	Lower	Upper	
105	100		
77	74.5	59.4	89.2
51	25.1	19.2	28.8

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 05/16/2023
Supervised By :Yogesh Patel 05/16/2023

