

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015074.D
 Acq On : 15 May 2023 14:34
 Operator : CG/JU
 Sample : 02592-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JRED2

Quant Time: May 16 01:32:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 11 23:06:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.140	152	305790	20.000	ng/u1	0.00
20) Naphthalene-d8	10.975	136	1386545	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.787	164	912854	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.539	188	2043006	20.000	ng/u1	0.00
79) Chrysene-d12	21.616	240	1815308	20.000	ng/u1	0.00
88) Perylene-d12	24.198	264	2012798	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	3285	0.417	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.287	99	455237	16.034	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.458	67	302575	18.452	ng/u1	0.00
11) 2-Chlorophenol-d4	7.663	132	378267	18.120	ng/u1	0.00
15) 4-Methylphenol-d8	8.852	113	383337	16.944	ng/u1	0.00
21) Nitrobenzene-d5	9.316	128	185855	17.058	ng/u1	0.00
24) 2-Nitrophenol-d4	10.046	143	200696	16.555	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	360419	16.476	ng/u1	0.00
31) 4-Chloroaniline-d4	11.110	131	542572	16.763	ng/u1	0.00
46) Dimethylphthalate-d6	14.187	166	1389214	20.139	ng/u1	0.00
49) Acenaphthylene-d8	14.481	160	1504447	19.069	ng/u1	0.00
54) 4-Nitrophenol-d4	14.969	143	149569	11.166	ng/u1	0.00
60) Fluorene-d10	15.775	176	1154072	19.827	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.892	200	141346	10.978	ng/u1	0.00
73) Anthracene-d10	17.639	188	1835424	19.620	ng/u1	0.00
81) Pyrene-d10	19.857	212	2162629	20.541	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.027	264	2001208	20.029	ng/u1	0.00
Target Compounds						
16) Acetophenone	8.975	105	98258	2.783	ng/u1	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015074.D
Acq On : 15 May 2023 14:34
Operator : CG/JU
Sample : 02592-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JRED2

Quant Time: May 16 01:32:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 11 23:06:15 2023
Response via : Initial Calibration

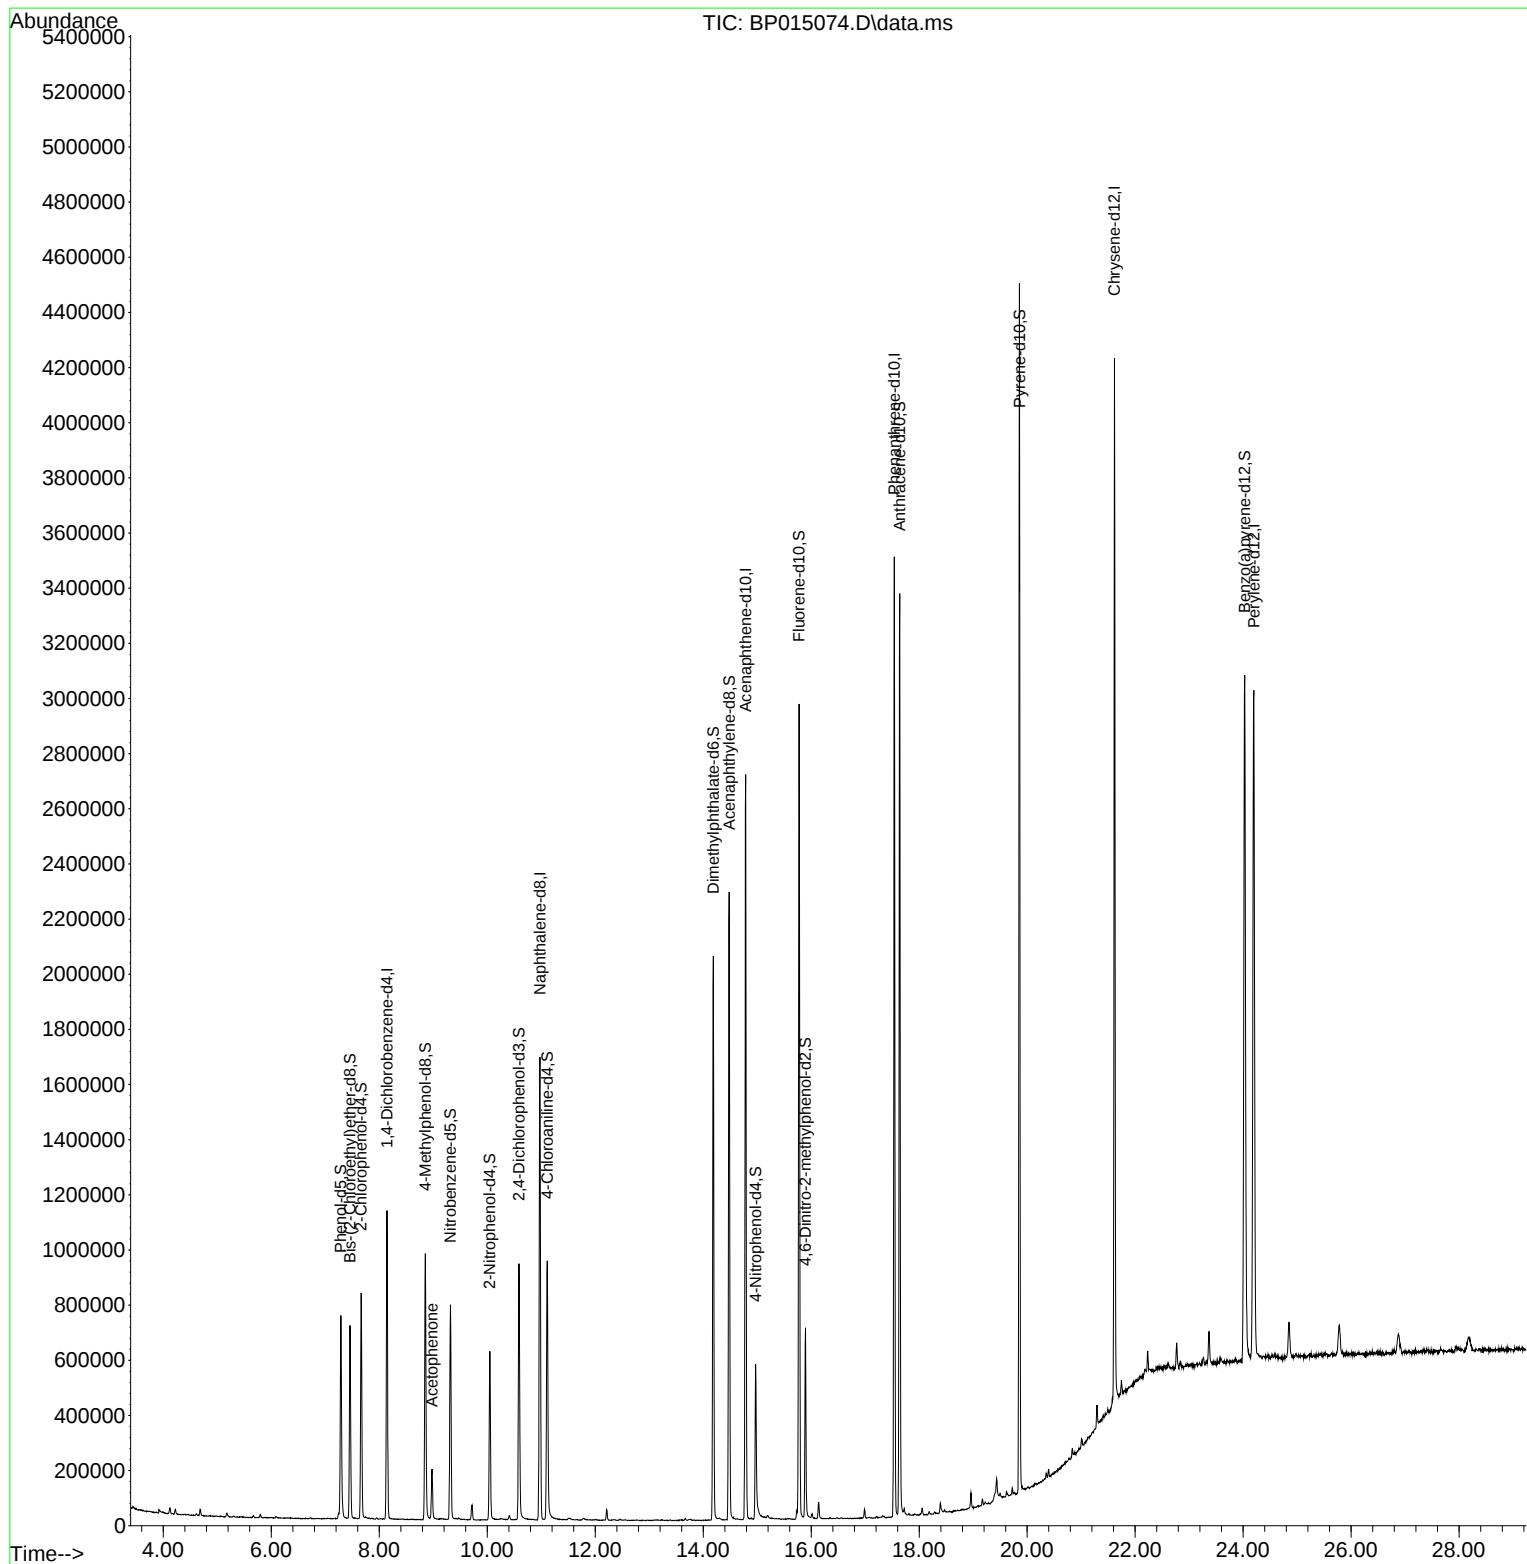

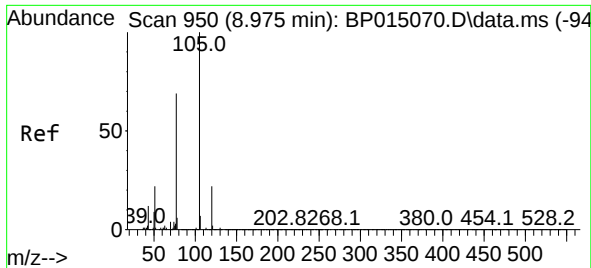

#16
 Acetophenone
 Concen: 2.783 ng/ul
 RT: 8.975 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BP015074.D
 Acq: 15 May 2023 14:34

Instrument :
 BNA_P
 ClientSampleId :
 JRED2

Tgt Ion:105 Resp: 98258
 Ion Ratio Lower Upper
 105 100
 77 78.9 59.4 89.2
 51 26.8 19.2 28.8

