

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015075.D
 Acq On : 15 May 2023 15:13
 Operator : CG/JU
 Sample : 02592-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JRED9

Quant Time: May 16 01:33:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 11 23:06:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.140	152	341501	20.000	ng/ul	0.00
20) Naphthalene-d8	10.969	136	1514251	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.781	164	1039931	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.540	188	2351740	20.000	ng/ul	0.00
79) Chrysene-d12	21.616	240	2161615	20.000	ng/ul	0.00
88) Perylene-d12	24.192	264	2398524	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.440	96	2620	0.298	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.287	99	525263	16.566	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.458	67	338157	18.466	ng/ul	0.00
11) 2-Chlorophenol-d4	7.664	132	433774	18.606	ng/ul	0.00
15) 4-Methylphenol-d8	8.852	113	446487	17.672	ng/ul	0.00
21) Nitrobenzene-d5	9.316	128	221201	18.590	ng/ul	0.00
24) 2-Nitrophenol-d4	10.046	143	247451	18.690	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.587	165	439918	18.414	ng/ul	0.00
31) 4-Chloroaniline-d4	11.110	131	660428	18.684	ng/ul	0.00
46) Dimethylphthalate-d6	14.181	166	1704110	21.685	ng/ul	0.00
49) Acenaphthylene-d8	14.481	160	1877654	20.892	ng/ul	0.00
54) 4-Nitrophenol-d4	14.969	143	227167	14.887	ng/ul	0.00
60) Fluorene-d10	15.775	176	1447992	21.837	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.893	200	219143	14.786	ng/ul	0.00
73) Anthracene-d10	17.634	188	2273561	21.113	ng/ul	0.00
81) Pyrene-d10	19.857	212	2630166	20.979	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.022	264	2442953	20.518	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.975	105	71574	1.815	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015075.D
Acq On : 15 May 2023 15:13
Operator : CG/JU
Sample : 02592-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JRED9


Quant Time: May 16 01:33:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 11 23:06:15 2023
Response via : Initial Calibration

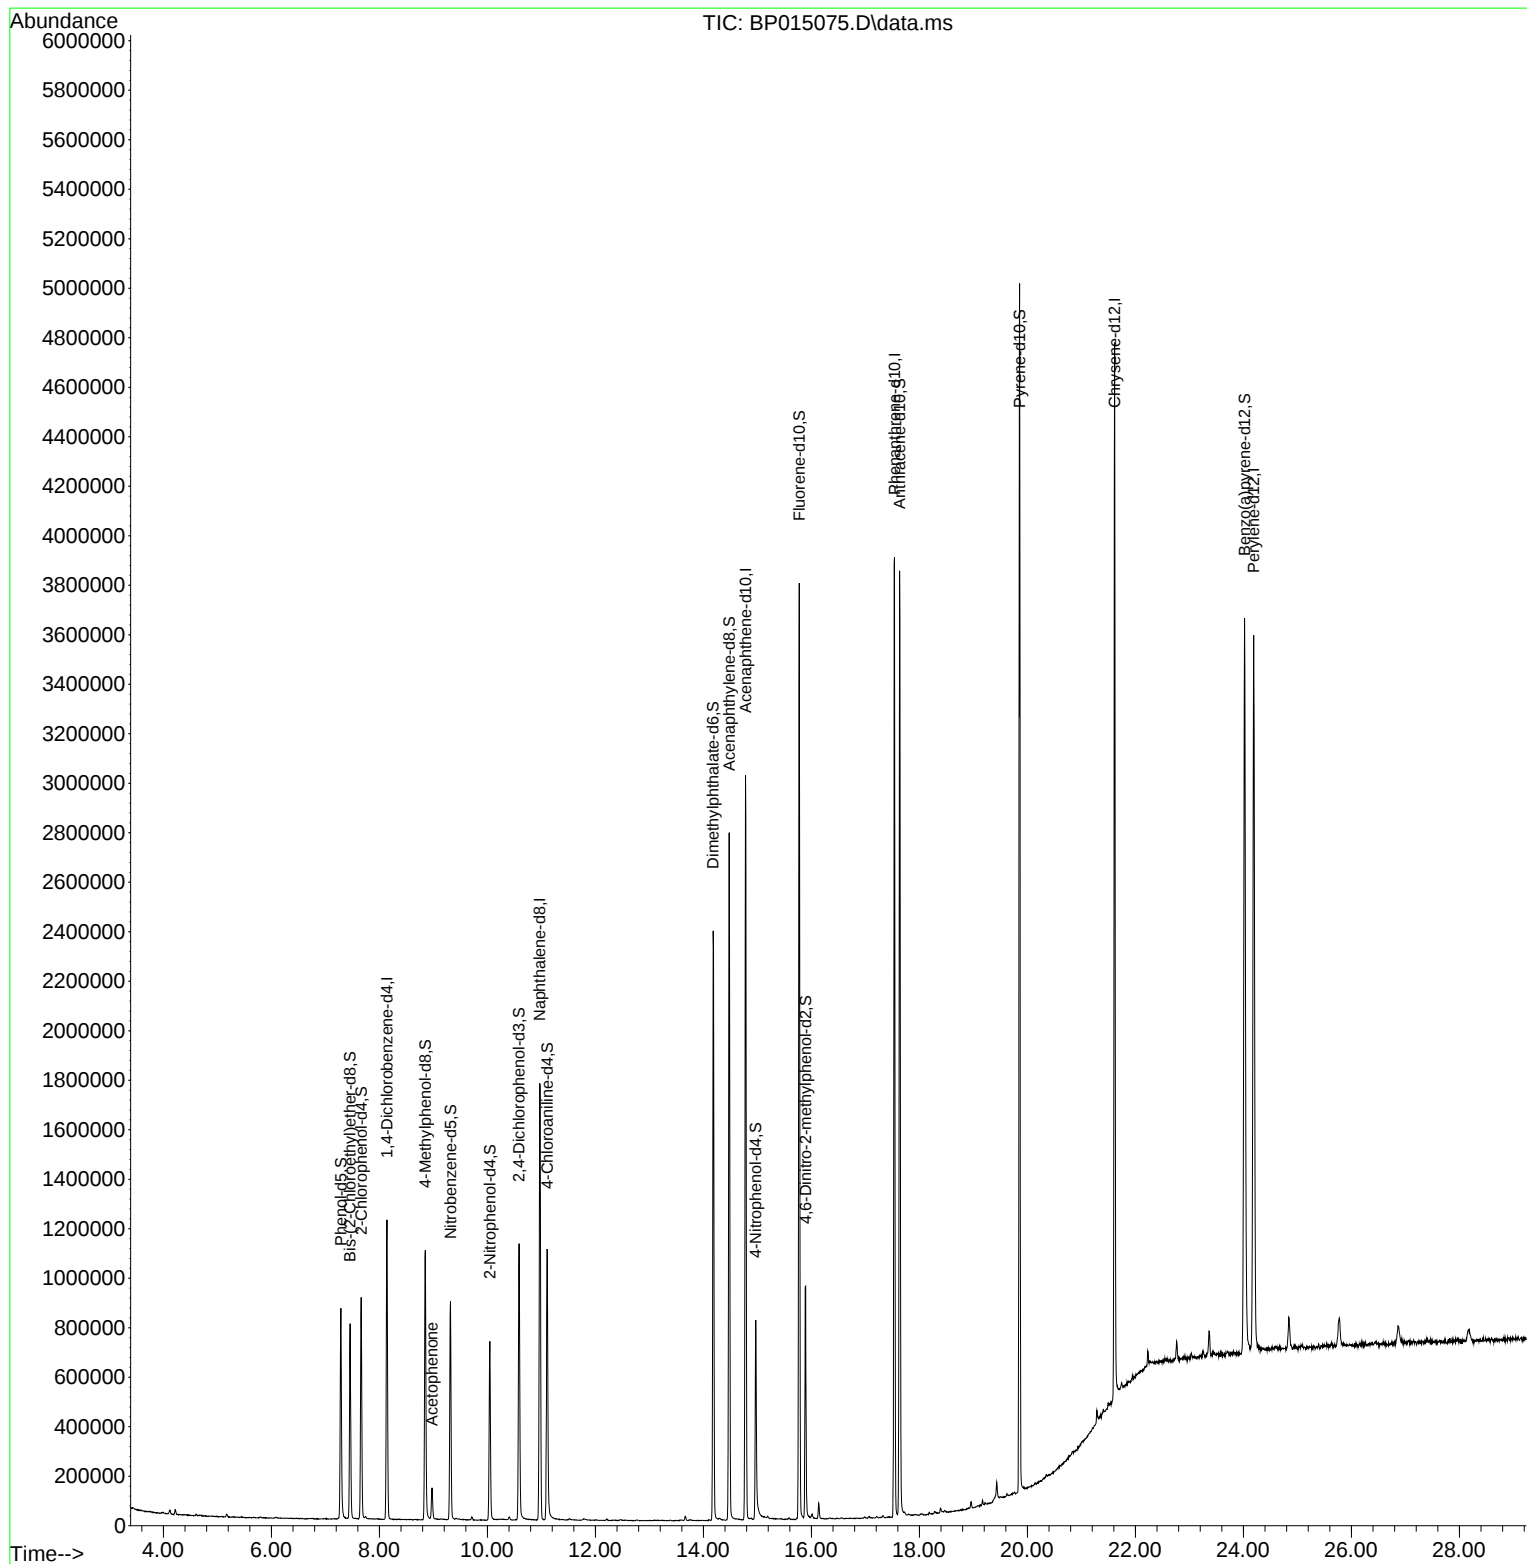

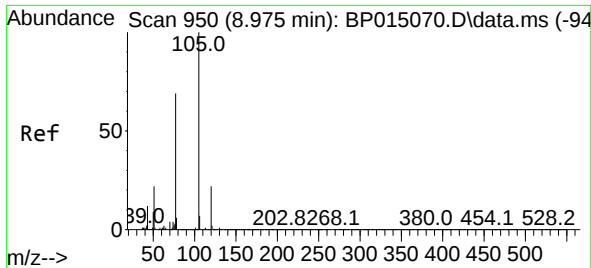

#16
 Acetophenone
 Concen: 1.815 ng/ul
 RT: 8.975 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BP015075.D
 Acq: 15 May 2023 15:13

Instrument :
 BNA_P
 ClientSampleId :
 JRED9

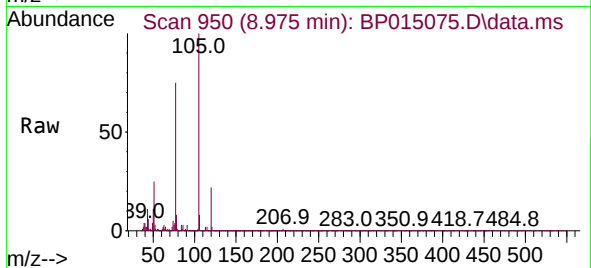

Tgt Ion:	105	Resp:	71574
Ion	Ratio	Lower	Upper
105	100		
77	74.5	59.4	89.2
51	25.4	19.2	28.8

