

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015080.D
 Acq On : 15 May 2023 18:35
 Operator : CG/JU
 Sample : 02592-26
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREK8

Quant Time: May 16 01:48:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 16 01:39:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.140	152	348941	20.000	ng/u1	0.00
20) Naphthalene-d8	10.969	136	1552322	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.781	164	991355	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.533	188	2129683	20.000	ng/u1	0.00
79) Chrysene-d12	21.610	240	1747631	20.000	ng/u1	0.00
88) Perylene-d12	24.186	264	1605648	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	24017	2.674	ng/uL	0.00
4) Pyridine-d5	3.881	84	222830	8.753	ng/u1	0.00
7) Phenol-d5	7.287	99	994285	30.689	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.457	67	612642	32.741	ng/u1	0.00
11) 2-Chlorophenol-d4	7.663	132	802632	33.694	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	707639	27.411	ng/u1	0.00
21) Nitrobenzene-d5	9.316	128	407730	33.426	ng/u1	0.00
24) 2-Nitrophenol-d4	10.040	143	445918	32.854	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.581	165	795092	32.464	ng/u1	0.00
31) 4-Chloroaniline-d4	11.104	131	847705	23.393	ng/u1	0.00
46) Dimethylphthalate-d6	14.181	166	2570332	34.311	ng/u1	0.00
49) Acenaphthylene-d8	14.475	160	2982621	34.812	ng/u1	0.00
54) 4-Nitrophenol-d4	14.963	143	419186	28.817	ng/u1	0.00
60) Fluorene-d10	15.769	176	2238528	35.413	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.886	200	393438	29.314	ng/u1	0.00
73) Anthracene-d10	17.633	188	3446437	35.341	ng/u1	0.00
81) Pyrene-d10	19.851	212	3948880	38.959	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.015	264	2931693	36.781	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.969	105	250207	6.210	ng/u1	97
86) Bis(2-ethylhexyl)phtha...	21.492	149	86469	1.062	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015080.D
Acq On : 15 May 2023 18:35
Operator : CG/JU
Sample : 02592-26
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREK8

Quant Time: May 16 01:48:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 16 01:39:21 2023
Response via : Initial Calibration




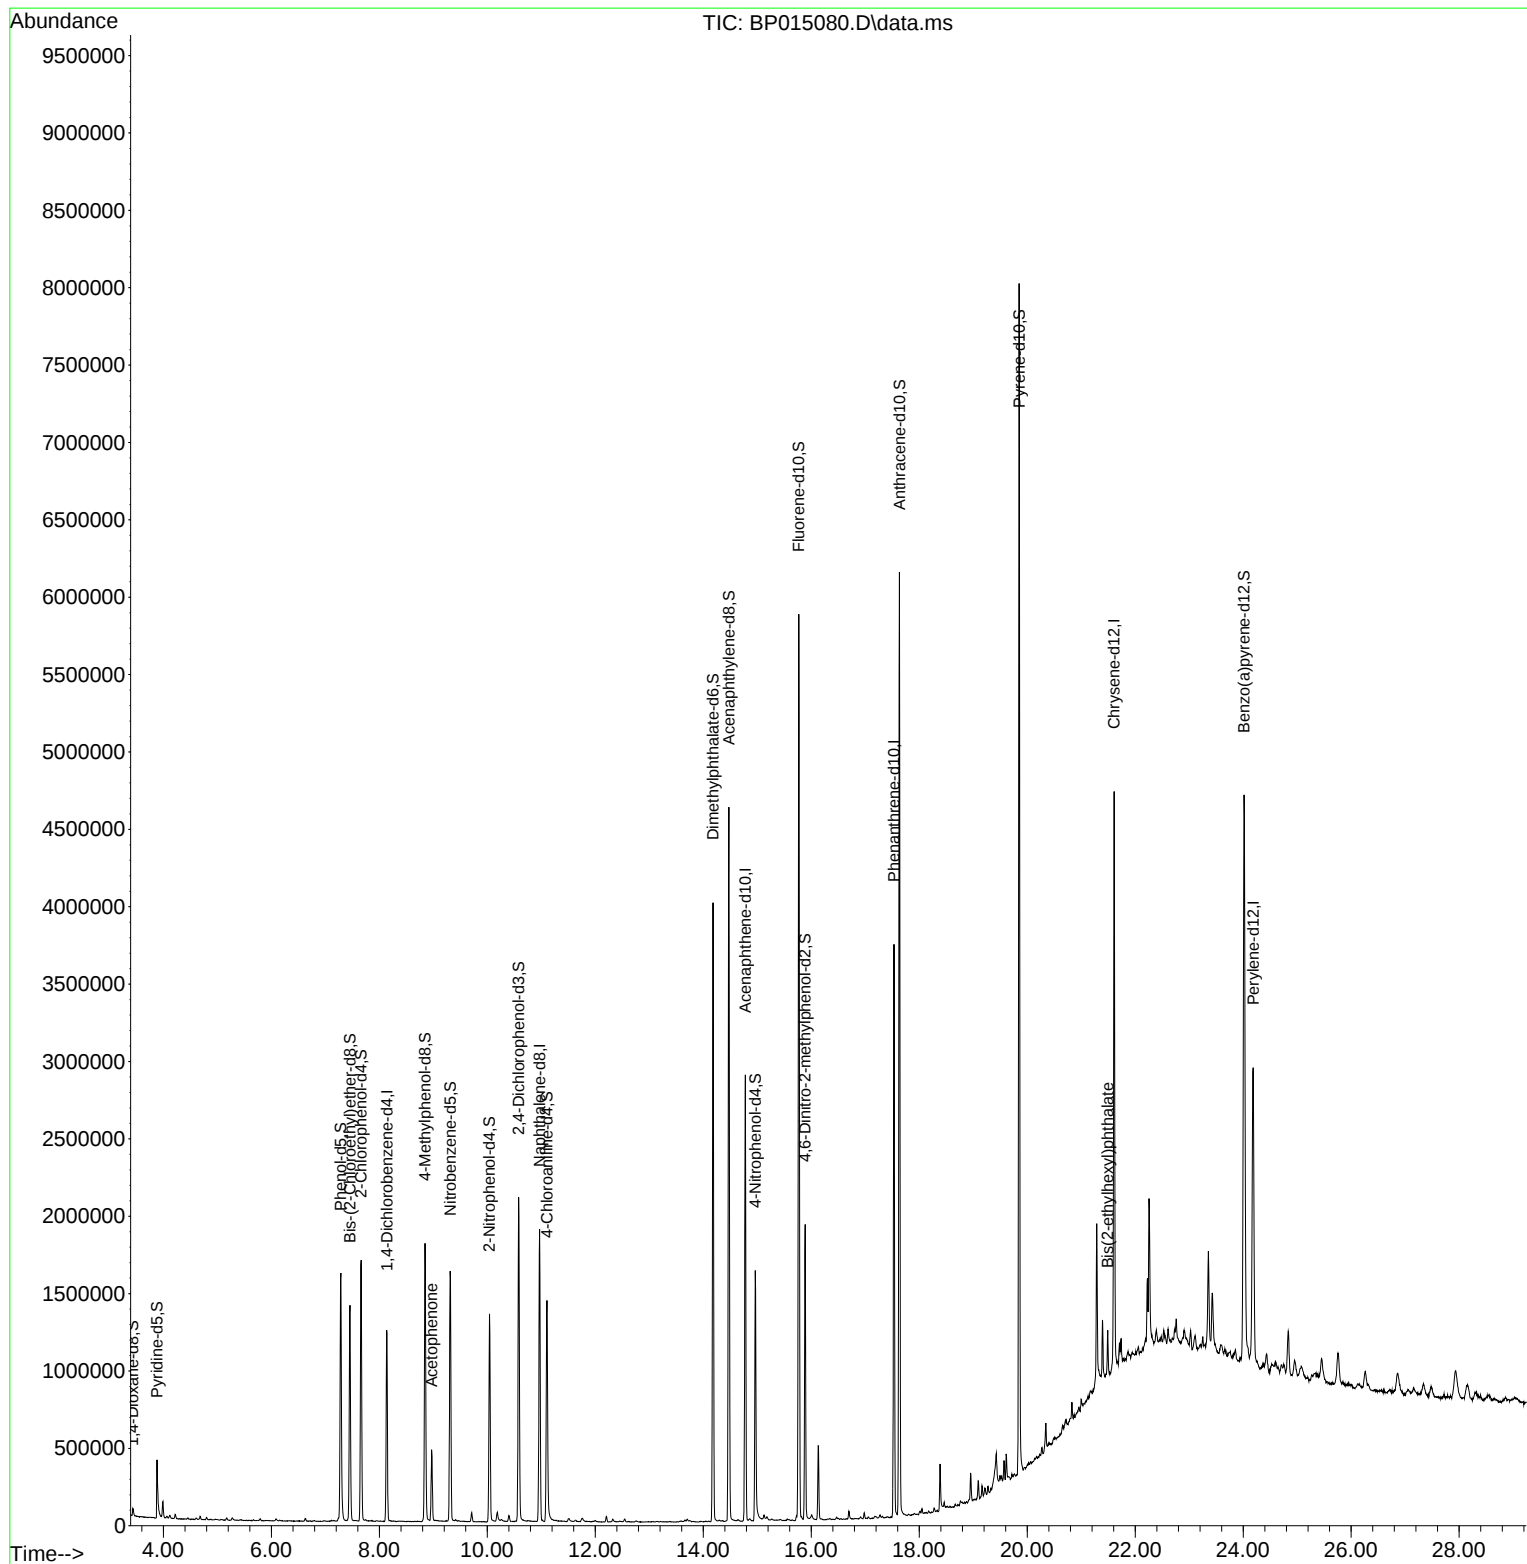


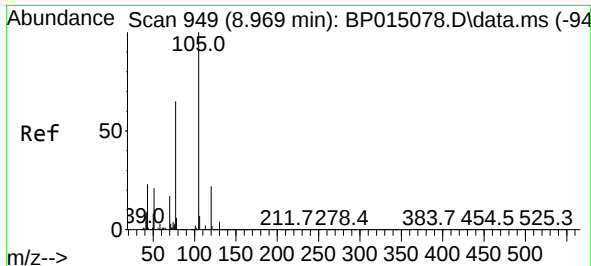

#16
Acetophenone
Concen: 6.210 ng/ul
RT: 8.969 min Scan# 949
Delta R.T. 0.000 min
Lab File: BP015080.D
Acq: 15 May 2023 18:35

Instrument :
BNA_P
ClientSampleId :
JREK8

Tgt Ion:105 Resp: 250207
Ion Ratio Lower Upper
105 100
77 75.6 59.4 89.2
51 27.3 19.2 28.8

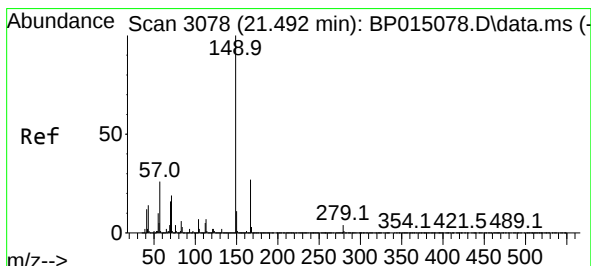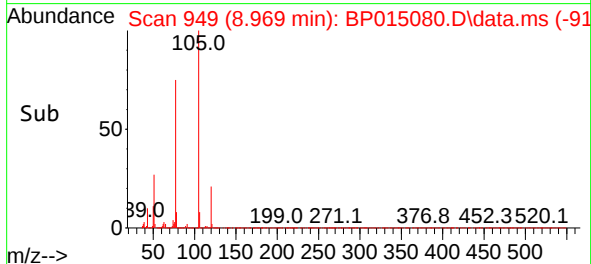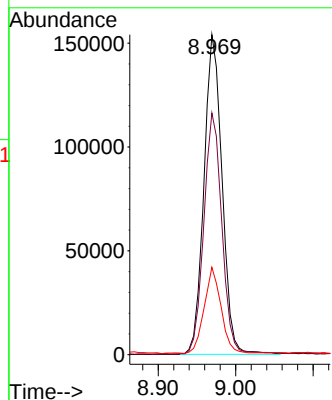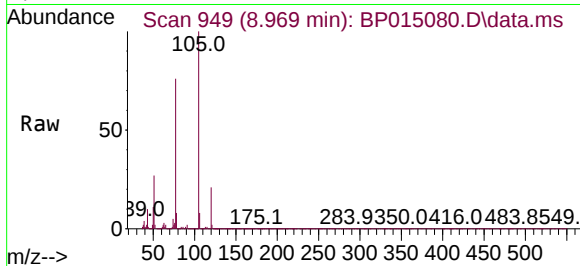

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.062 ng/ul
RT: 21.492 min Scan# 3078
Delta R.T. 0.000 min
Lab File: BP015080.D
Acq: 15 May 2023 18:35

Tgt Ion:149 Resp: 86469
Ion Ratio Lower Upper
149 100
167 28.5 21.8 32.6
279 4.5 3.2 4.8

