

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015090.D
 Acq On : 16 May 2023 00:10
 Operator : CG/JU
 Sample : 02592-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREG1

Quant Time: May 16 02:04:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 16 01:39:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	313835	20.000	ng/u1	0.00
20) Naphthalene-d8	10.963	136	1441629	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.775	164	961912	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.527	188	2114584	20.000	ng/u1	0.00
79) Chrysene-d12	21.604	240	1884007	20.000	ng/u1	0.00
88) Perylene-d12	24.174	264	2105421	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	260	0.032	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.281	99	379404	13.021	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.452	67	242436	14.406	ng/u1	0.00
11) 2-Chlorophenol-d4	7.657	132	297163	13.870	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	326938	14.081	ng/u1	0.00
21) Nitrobenzene-d5	9.310	128	153475	13.548	ng/u1	0.00
24) 2-Nitrophenol-d4	10.040	143	165705	13.146	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.581	165	303506	13.344	ng/u1	0.00
31) 4-Chloroaniline-d4	11.098	131	466792	13.871	ng/u1	0.00
46) Dimethylphthalate-d6	14.175	166	1111094	15.286	ng/u1	0.00
49) Acenaphthylene-d8	14.469	160	1260808	15.166	ng/u1	0.00
54) 4-Nitrophenol-d4	14.963	143	148752	10.539	ng/u1	0.00
60) Fluorene-d10	15.769	176	961949	15.684	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.881	200	126837	9.518	ng/u1	0.00
73) Anthracene-d10	17.627	188	1496097	15.451	ng/u1	0.00
81) Pyrene-d10	19.845	212	1686278	15.432	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.004	264	1581737	15.134	ng/u1	-0.02
Target Compounds						
					Qvalue	
16) Acetophenone	8.969	105	63720	1.758	ng/u1	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015090.D
Acq On : 16 May 2023 00:10
Operator : CG/JU
Sample : 02592-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG1

Quant Time: May 16 02:04:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 16 01:39:21 2023
Response via : Initial Calibration

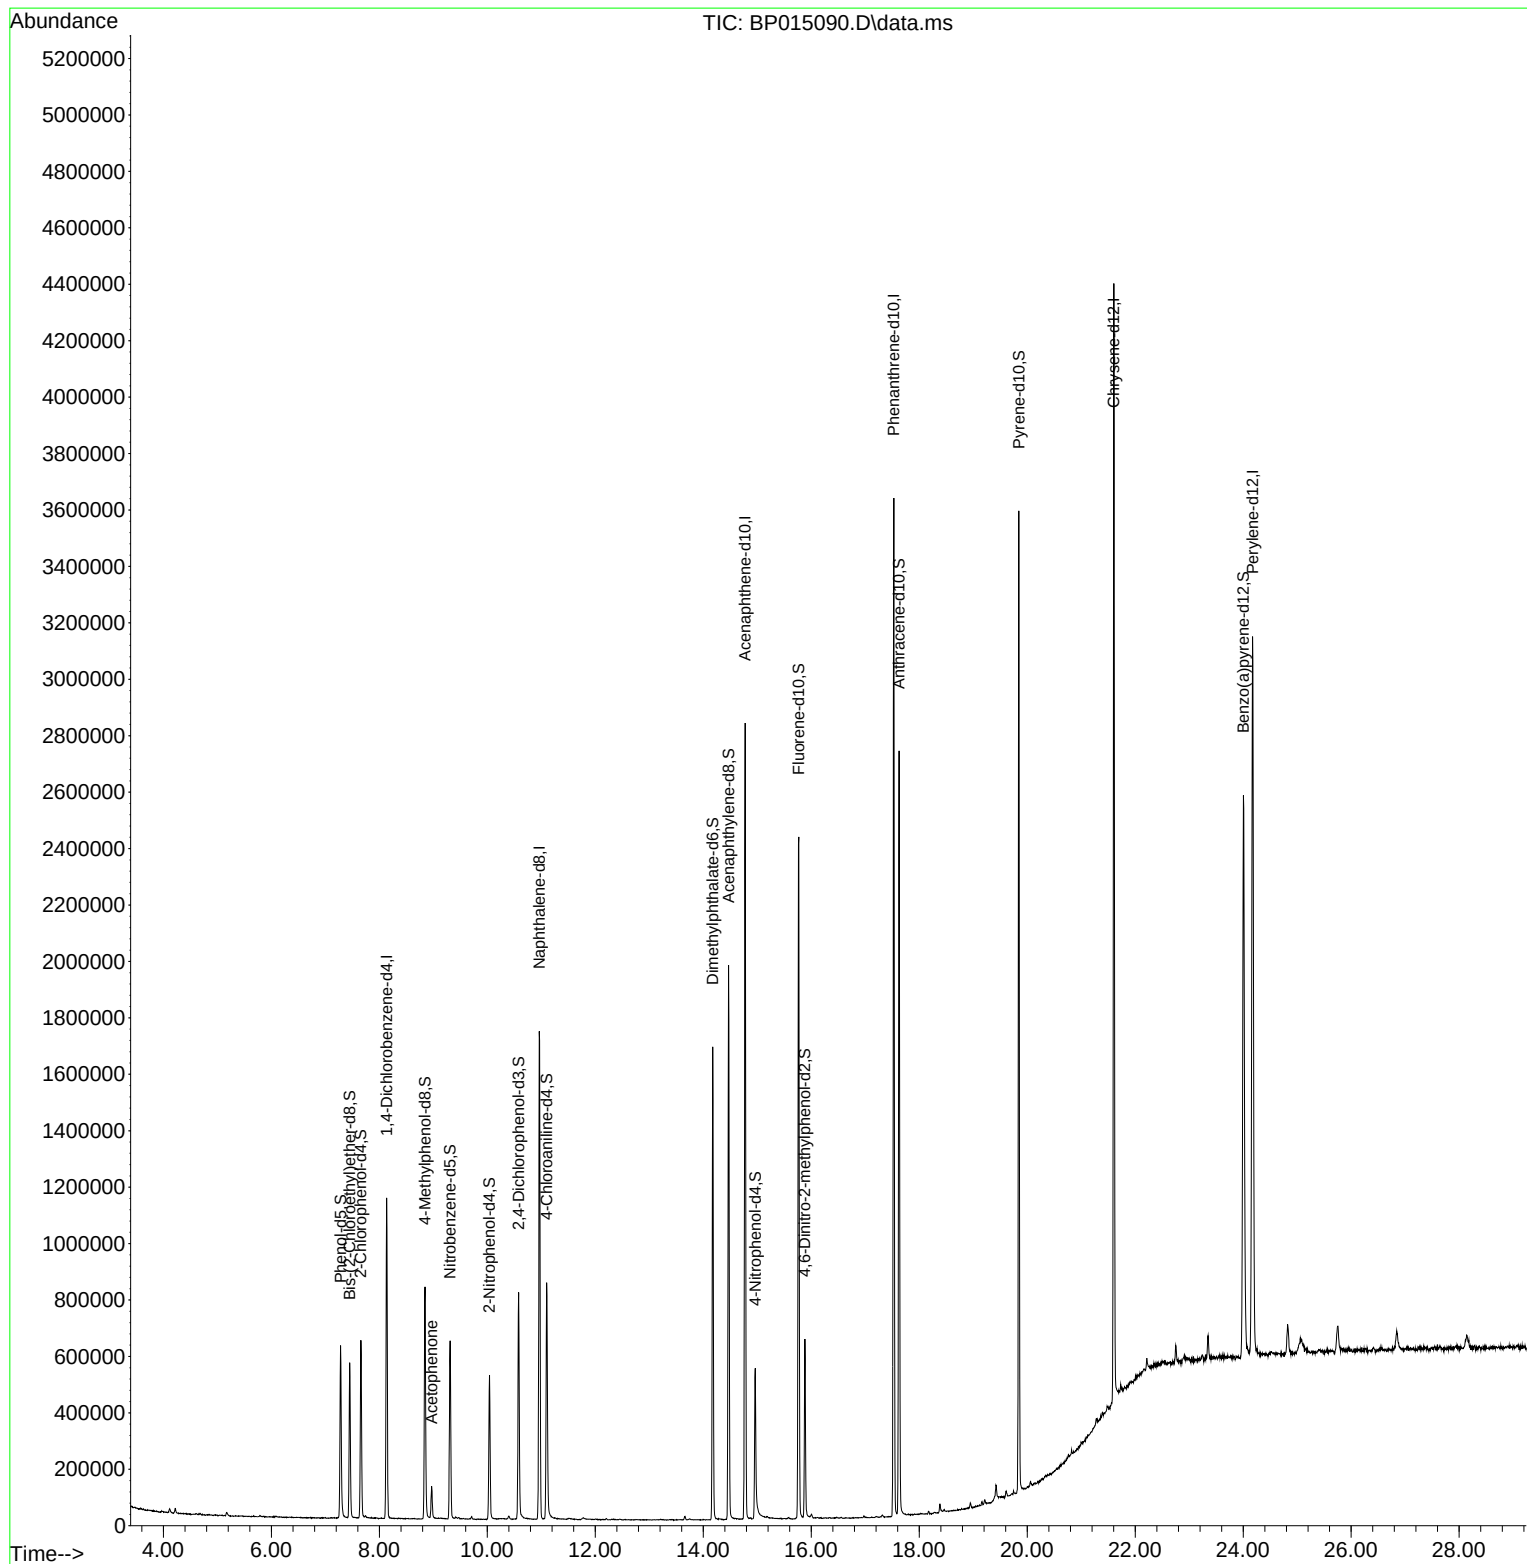

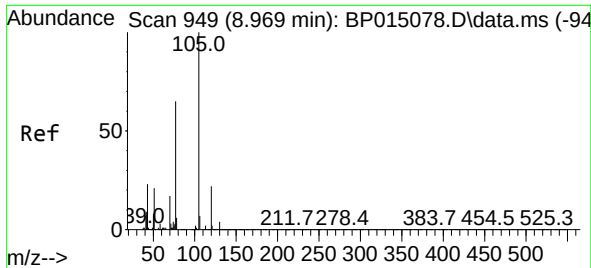

#16
 Acetophenone
 Concen: 1.758 ng/ul
 RT: 8.969 min Scan# 949
 Delta R.T. 0.000 min
 Lab File: BP015090.D
 Acq: 16 May 2023 00:10

Instrument :
 BNA_P
 ClientSampleId :
 JREG1

Tgt Ion:	105	Resp:	63720
Ion	Ratio	Lower	Upper
105	100		
77	78.0	59.4	89.2
51	27.9	19.2	28.8

