

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015091.D
 Acq On : 16 May 2023 00:44
 Operator : CG/JU
 Sample : 02592-22
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREE7

Quant Time: May 16 02:03:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 16 01:39:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	343540	20.000	ng/u1	0.00
20) Naphthalene-d8	10.963	136	1580066	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.775	164	1030438	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.528	188	2238250	20.000	ng/u1	0.00
79) Chrysene-d12	21.604	240	1894532	20.000	ng/u1	0.00
88) Perylene-d12	24.174	264	1948246	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	26058	2.947	ng/uL	0.00
4) Pyridine-d5	3.881	84	225524	8.998	ng/u1	0.00
7) Phenol-d5	7.281	99	917314	28.759	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.452	67	585148	31.763	ng/u1	0.00
11) 2-Chlorophenol-d4	7.658	132	721774	30.776	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	775589	30.515	ng/u1	0.00
21) Nitrobenzene-d5	9.310	128	388090	31.257	ng/u1	0.00
24) 2-Nitrophenol-d4	10.040	143	430772	31.181	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.581	165	738224	29.613	ng/u1	0.00
31) 4-Chloroaniline-d4	11.099	131	1119411	30.349	ng/u1	0.00
46) Dimethylphthalate-d6	14.181	166	2587300	33.228	ng/u1	0.00
49) Acenaphthylene-d8	14.469	160	2956435	33.198	ng/u1	0.00
54) 4-Nitrophenol-d4	14.963	143	433677	28.683	ng/u1	0.00
60) Fluorene-d10	15.769	176	2203573	33.538	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.881	200	382580	27.123	ng/u1	0.00
73) Anthracene-d10	17.628	188	3484119	33.994	ng/u1	0.00
81) Pyrene-d10	19.845	212	4028091	36.659	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	3390238	35.055	ng/u1	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.969	105	136482	3.441	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015091.D
Acq On : 16 May 2023 00:44
Operator : CG/JU
Sample : 02592-22
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREE7

Quant Time: May 16 02:03:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 16 01:39:21 2023
Response via : Initial Calibration

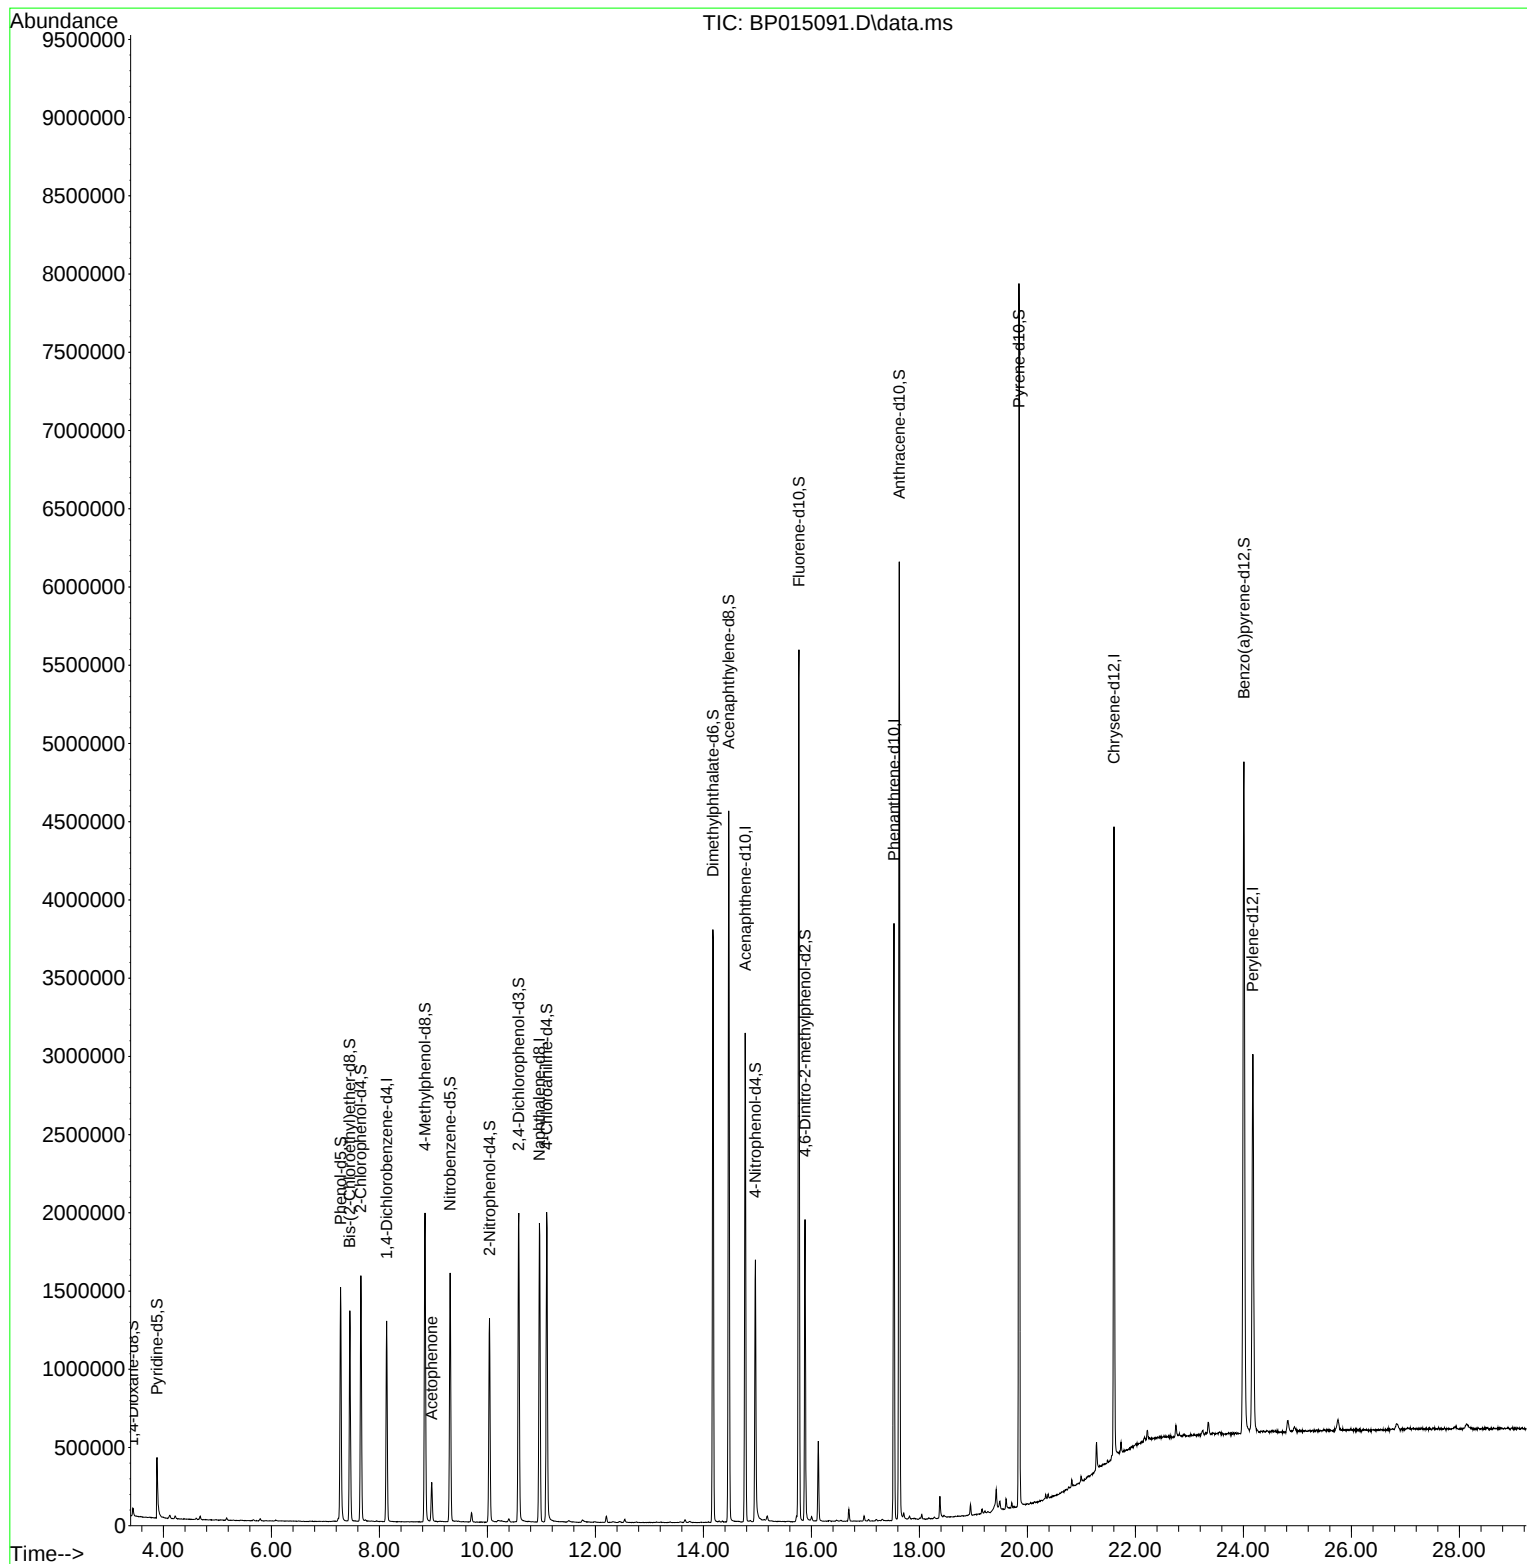

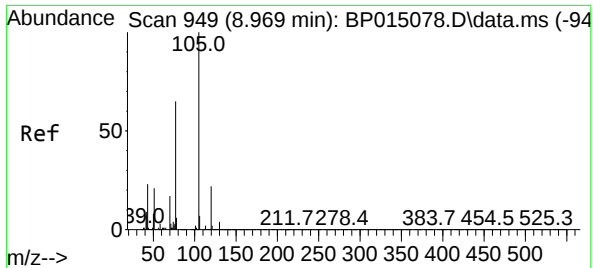

#16
 Acetophenone
 Concen: 3.441 ng/ul
 RT: 8.969 min Scan# 94
 Delta R.T. 0.000 min
 Lab File: BP015091.D
 Acq: 16 May 2023 00:44

Instrument :
 BNA_P
 ClientSampleId :
 JREE7

Tgt Ion:105 Resp: 136482
 Ion Ratio Lower Upper
 105 100
 77 73.8 59.4 89.2
 51 25.3 19.2 28.8

