

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015092.D
 Acq On : 16 May 2023 01:17
 Operator : CG/JU
 Sample : 02592-23
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREJ8

Quant Time: May 16 02:06:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 16 01:39:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	335480	20.000	ng/u1	0.00
20) Naphthalene-d8	10.963	136	1520118	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.775	164	1005613	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.528	188	2195079	20.000	ng/u1	0.00
79) Chrysene-d12	21.604	240	1878830	20.000	ng/u1	0.00
88) Perylene-d12	24.174	264	1900764	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	4121	0.477	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.281	99	460542	14.785	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.452	67	289396	16.087	ng/u1	0.00
11) 2-Chlorophenol-d4	7.658	132	360848	15.756	ng/u1	0.00
15) 4-Methylphenol-d8	8.846	113	395580	15.938	ng/u1	0.00
21) Nitrobenzene-d5	9.311	128	180273	15.092	ng/u1	0.00
24) 2-Nitrophenol-d4	10.040	143	196781	14.806	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.581	165	375328	15.650	ng/u1	0.00
31) 4-Chloroaniline-d4	11.099	131	487281	13.732	ng/u1	0.00
46) Dimethylphthalate-d6	14.175	166	1284460	16.903	ng/u1	0.00
49) Acenaphthylene-d8	14.469	160	1451130	16.697	ng/u1	0.00
54) 4-Nitrophenol-d4	14.963	143	178398	12.090	ng/u1	0.00
60) Fluorene-d10	15.763	176	1107286	17.269	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.881	200	162478	11.745	ng/u1	0.00
73) Anthracene-d10	17.628	188	1734838	17.260	ng/u1	0.00
81) Pyrene-d10	19.845	212	2045324	18.770	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.004	264	1721593	18.246	ng/u1	-0.02
Target Compounds						
					Qvalue	
16) Acetophenone	8.969	105	77373	1.997	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015092.D
Acq On : 16 May 2023 01:17
Operator : CG/JU
Sample : 02592-23
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREJ8

Quant Time: May 16 02:06:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 16 01:39:21 2023
Response via : Initial Calibration

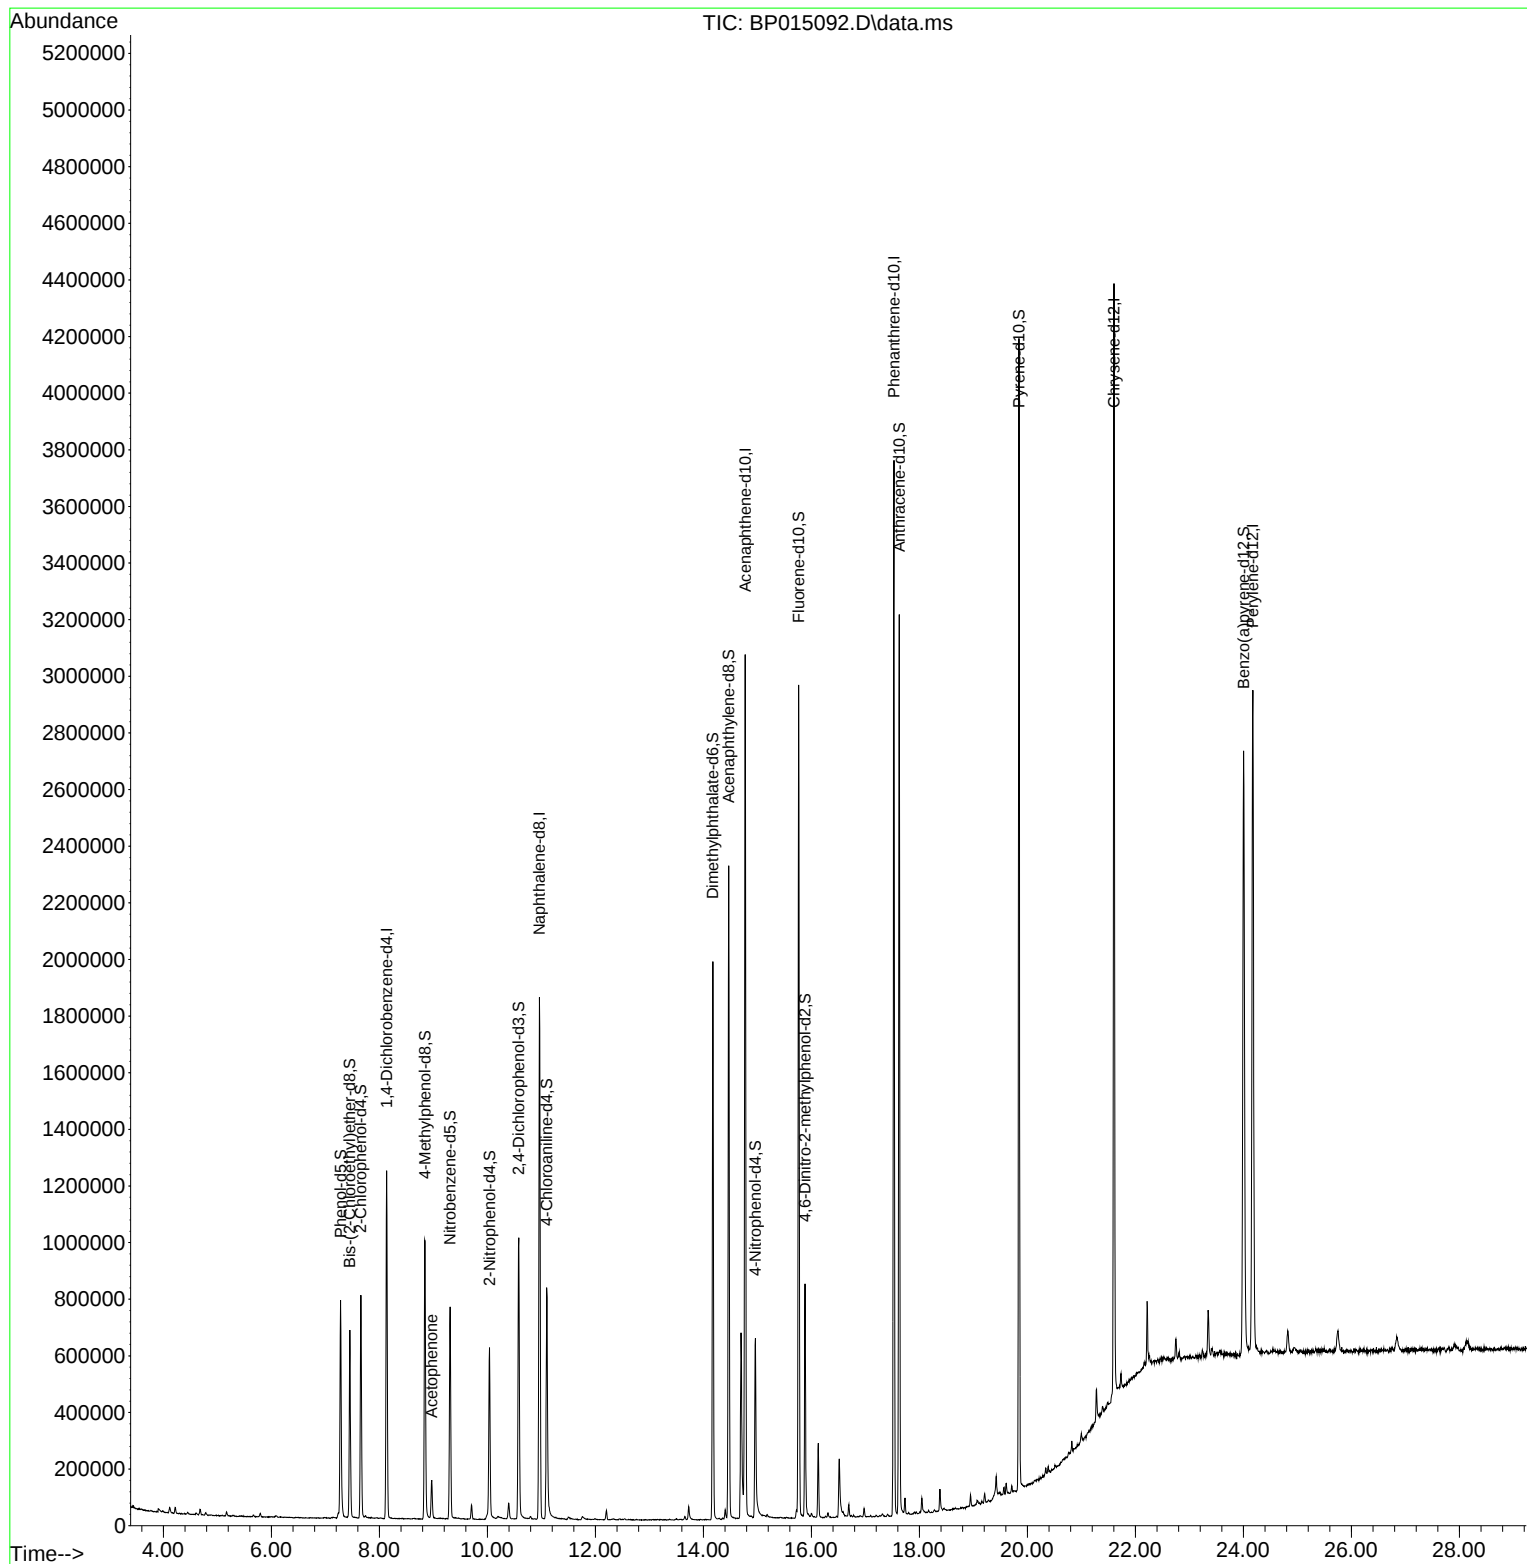

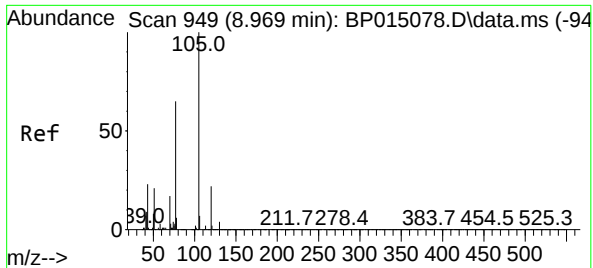

#16
 Acetophenone
 Concen: 1.997 ng/ul
 RT: 8.969 min Scan# 94
 Delta R.T. 0.000 min
 Lab File: BP015092.D
 Acq: 16 May 2023 01:17

Instrument :
 BNA_P
 ClientSampleId :
 JREJ8

Tgt Ion:	105	Resp:	77373
Ion	Ratio	Lower	Upper
105	100		
77	74.3	59.4	89.2
51	26.7	19.2	28.8

