

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015093.D
 Acq On : 16 May 2023 01:51
 Operator : CG/JU
 Sample : 02592-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREG2

Quant Time: May 16 03:01:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 16 01:39:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	318897	20.000	ng/ul	0.00
20) Naphthalene-d8	10.963	136	1457122	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.775	164	964108	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.528	188	2098123	20.000	ng/ul	0.00
79) Chrysene-d12	21.604	240	1799877	20.000	ng/ul	0.00
88) Perylene-d12	24.174	264	1870847	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.446	96	199	0.024	ng/uL	0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.281	99	386144	13.042	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.452	67	245037	14.329	ng/ul	0.00
11) 2-Chlorophenol-d4	7.657	132	305773	14.046	ng/ul	0.00
15) 4-Methylphenol-d8	8.840	113	332209	14.081	ng/ul	-0.01
21) Nitrobenzene-d5	9.310	128	150808	13.171	ng/ul	0.00
24) 2-Nitrophenol-d4	10.040	143	164011	12.873	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.581	165	308618	13.424	ng/ul	0.00
31) 4-Chloroaniline-d4	11.099	131	468078	13.761	ng/ul	0.00
46) Dimethylphthalate-d6	14.175	166	1076119	14.771	ng/ul	0.00
49) Acenaphthylene-d8	14.469	160	1217391	14.611	ng/ul	0.00
54) 4-Nitrophenol-d4	14.963	143	142819	10.096	ng/ul	0.00
60) Fluorene-d10	15.763	176	933650	15.188	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.881	200	117646	8.897	ng/ul	0.00
73) Anthracene-d10	17.628	188	1437737	14.965	ng/ul	0.00
81) Pyrene-d10	19.845	212	1620637	15.525	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.004	264	1368079	14.731	ng/ul	-0.02
Target Compounds						
					Qvalue	
16) Acetophenone	8.969	105	77893	2.115	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015093.D
Acq On : 16 May 2023 01:51
Operator : CG/JU
Sample : 02592-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG2

Quant Time: May 16 03:01:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 16 01:39:21 2023
Response via : Initial Calibration

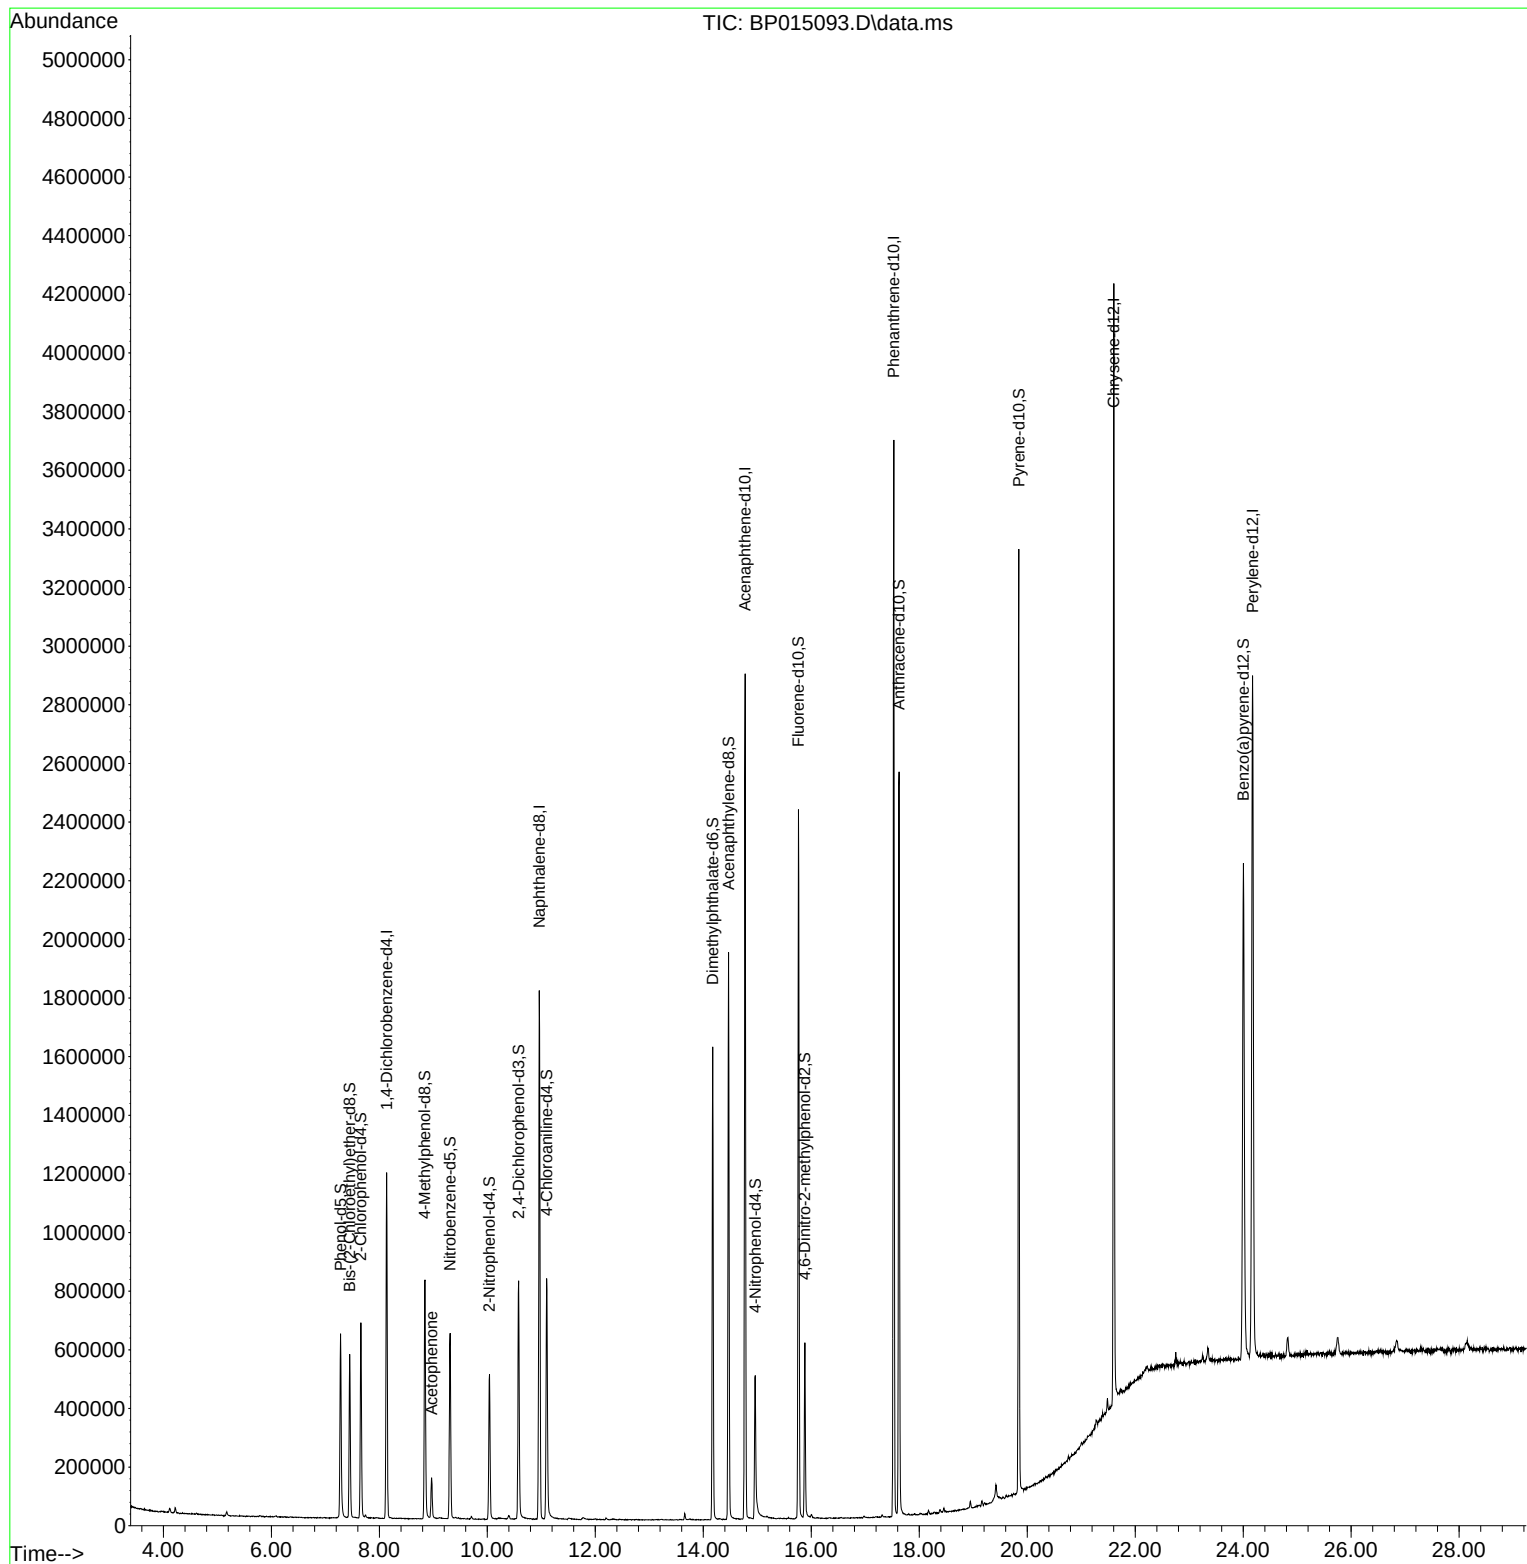

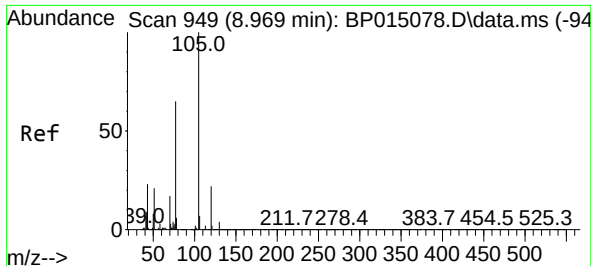

#16
Acetophenone
Concen: 2.115 ng/ul
RT: 8.969 min Scan# 94
Delta R.T. 0.000 min
Lab File: BP015093.D
Acq: 16 May 2023 01:51

Instrument :
BNA_P
ClientSampleId :
JREG2

Tgt Ion:105 Resp: 77893
Ion Ratio Lower Upper
105 100
77 77.5 59.4 89.2
51 24.8 19.2 28.8

