

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015073.D
 Acq On : 15 May 2023 13:48
 Operator : CG/JU
 Sample : 02592-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015073.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.440	5	9	15	rVB	30999	45498	0.88%	0.101%
2	3.881	81	84	99	rBV	345143	579944	11.20%	1.284%
3	4.122	122	125	133	rVB2	17817	29234	0.56%	0.065%
4	4.222	138	142	151	rVB	17955	27984	0.54%	0.062%
5	5.175	300	304	311	rVB2	13486	24679	0.48%	0.055%
6	7.287	653	663	674	rBV	393426	671079	12.96%	1.486%
7	7.458	686	692	702	rBV	371370	591698	11.42%	1.310%
8	7.663	720	727	737	rBV	424862	691981	13.36%	1.532%
9	7.746	737	741	745	rVB5	7909	11934	0.23%	0.026%
10	8.140	800	808	816	rBV	1039463	1692418	32.67%	3.748%
11	8.846	921	928	943	rBV	465991	840620	16.23%	1.861%
12	8.975	943	950	958	rVV	115892	201914	3.90%	0.447%
13	9.316	1000	1008	1020	rBV	388105	676968	13.07%	1.499%
14	9.422	1020	1026	1029	rBV8	3578	6559	0.13%	0.015%
15	9.710	1068	1075	1083	rVB2	10349	16545	0.32%	0.037%
16	10.046	1124	1132	1141	rBV	297185	520489	10.05%	1.153%
17	10.405	1187	1193	1202	rVB3	11757	21927	0.42%	0.049%
18	10.587	1217	1224	1245	rBV	457386	835887	16.14%	1.851%
19	10.969	1281	1289	1303	rBV	1597691	2627164	50.72%	5.818%
20	11.104	1305	1312	1328	rBV	463838	883054	17.05%	1.955%
21	11.775	1424	1426	1434	rBV8	3662	7056	0.14%	0.016%
22	12.199	1496	1498	1503	rBV5	4697	7295	0.14%	0.016%
23	12.457	1538	1542	1545	rBV6	3172	5724	0.11%	0.013%
24	12.551	1552	1558	1565	rBV5	8769	18236	0.35%	0.040%
25	13.663	1742	1747	1753	rVB3	10238	16778	0.32%	0.037%
26	14.181	1828	1835	1845	rBV	1080224	1530384	29.54%	3.389%
27	14.287	1851	1853	1860	rVB8	3603	6297	0.12%	0.014%
28	14.475	1877	1885	1899	rBV	1235573	1803369	34.81%	3.993%
29	14.781	1929	1937	1949	rBV	2528111	3764756	72.68%	8.337%
30	14.969	1962	1969	1993	rBV	243851	537671	10.38%	1.191%
31	15.187	2003	2006	2012	rVB5	11706	16044	0.31%	0.036%
32	15.587	2070	2074	2077	rVB	11670	15283	0.30%	0.034%
33	15.769	2099	2105	2112	rBV	1580208	2251609	43.47%	4.986%
34	15.887	2118	2125	2134	rBV	360655	534701	10.32%	1.184%
35	16.016	2142	2147	2149	rVB4	5624	7225	0.14%	0.016%
36	16.563	2235	2240	2242	rBV5	3833	5558	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015073.D
 Acq On : 15 May 2023 13:48
 Operator : CG/JU
 Sample : 02592-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	16.981	2306	2311	2314	rBV5	6604	9560	0.18%	0.021%
38	17.322	2365	2369	2374	rVB3	6642	8413	0.16%	0.019%
39	17.534	2398	2405	2415	rBV	3337260	4623686	89.26%	10.239%
40	17.634	2415	2422	2433	rVV	1801141	2592860	50.06%	5.742%
41	17.716	2434	2436	2443	rVB7	14170	22373	0.43%	0.050%
42	17.798	2448	2450	2456	rVB3	6921	10490	0.20%	0.023%
43	18.392	2548	2551	2555	rVB6	8920	11366	0.22%	0.025%
44	18.463	2560	2563	2568	rBV2	9694	13847	0.27%	0.031%
45	18.951	2643	2646	2651	rVB3	23191	27744	0.54%	0.061%
46	19.169	2680	2683	2686	rBV	13960	14871	0.29%	0.033%
47	19.428	2724	2727	2735	rVB9	35212	56782	1.10%	0.126%
48	19.851	2793	2799	2809	rBV	2303928	3046950	58.82%	6.747%
49	21.610	3093	3098	3108	rBV	3604981	4907990	94.75%	10.868%
50	24.016	3500	3507	3519	rVB2	1392191	3106672	59.97%	6.879%
51	24.186	3529	3536	3547	rVB	2421062	5180016	100.00%	11.471%




Sum of corrected areas: 45159182

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015073.D
Acq On : 15 May 2023 13:48
Operator : CG/JU
Sample : 02592-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

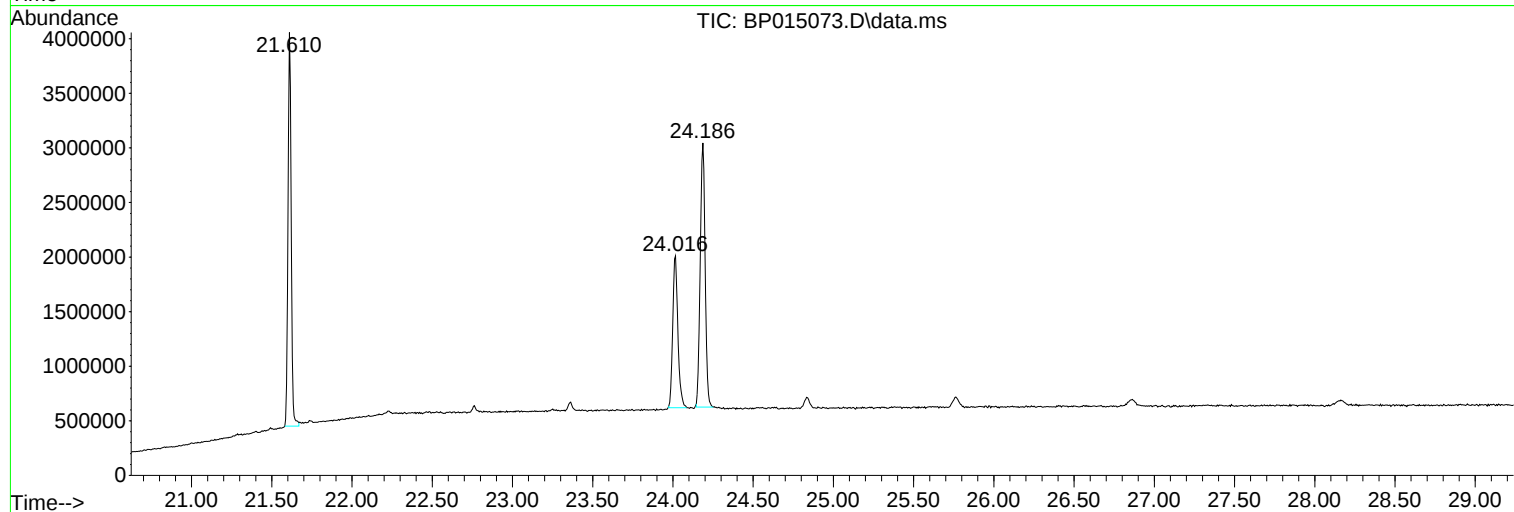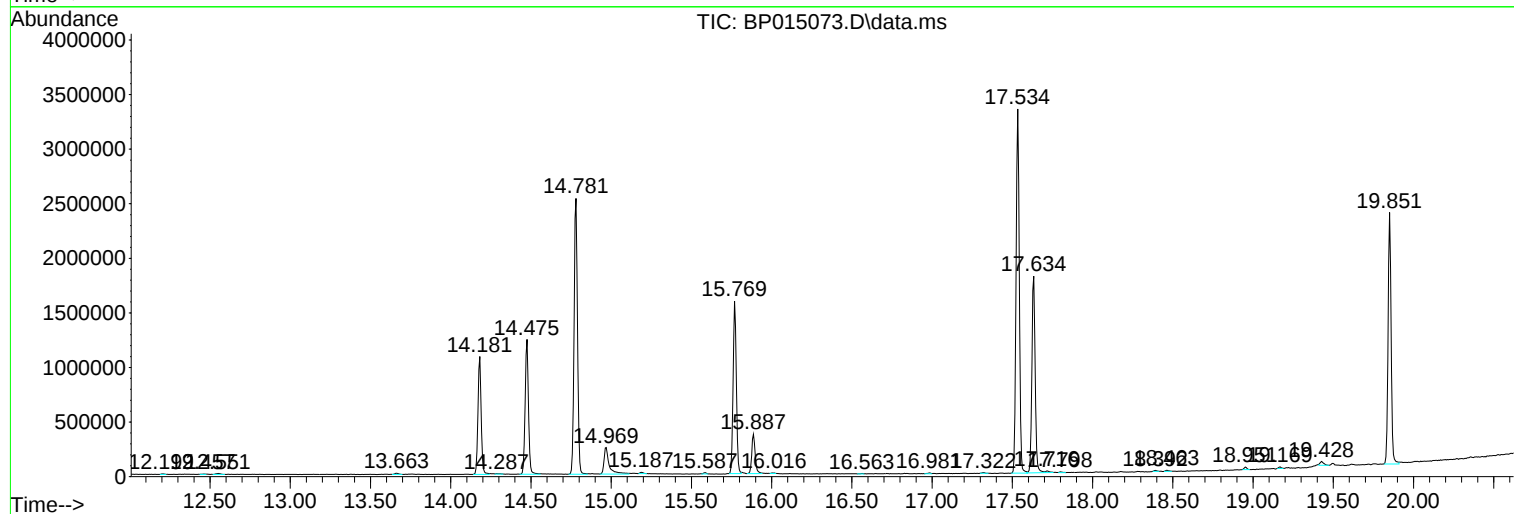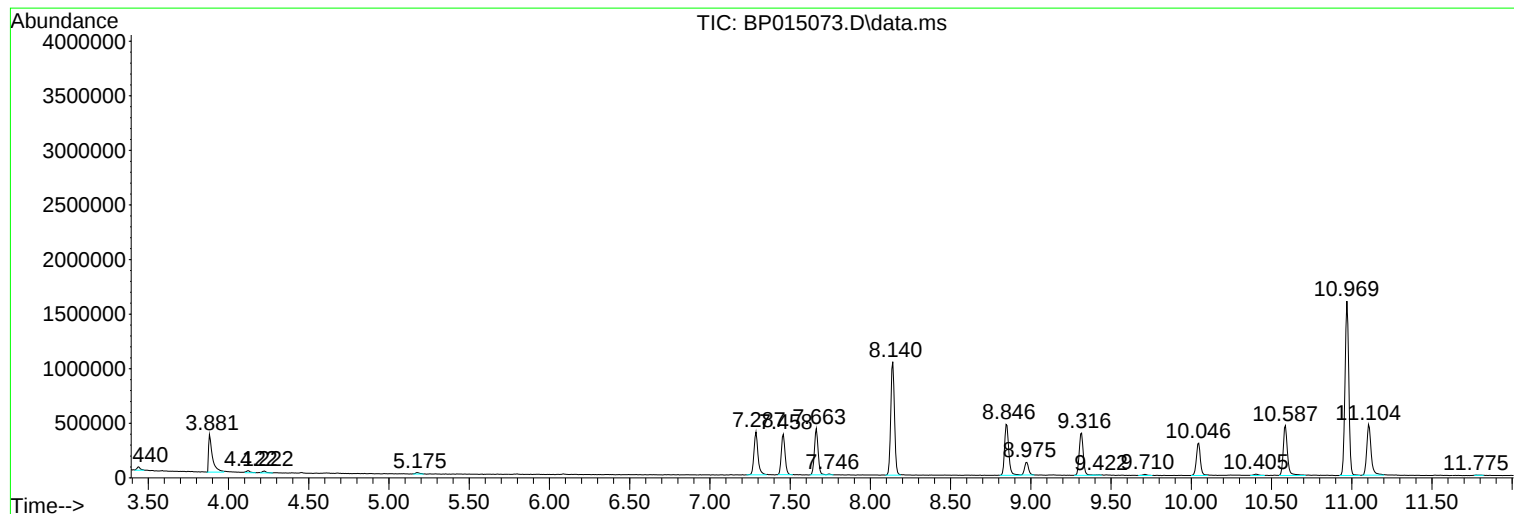

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015073.D
Acq On : 15 May 2023 13:48
Operator : CG/JU
Sample : 02592-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015073.D
Acq On : 15 May 2023 13:48
Operator : CG/JU
Sample : 02592-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc