

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015075.D
 Acq On : 15 May 2023 15:13
 Operator : CG/JU
 Sample : 02592-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JRED9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.123	120	125	133	rVB	18297	36485	0.55%	0.049%
2	4.217	137	141	146	rBV2	21164	33151	0.50%	0.044%
3	4.605	205	207	212	rVB6	6828	8043	0.12%	0.011%
4	5.175	300	304	309	rVB	12557	20662	0.31%	0.028%
5	5.799	405	410	412	rBV5	4448	7430	0.11%	0.010%
6	7.287	656	663	675	rBV	847055	1372319	20.65%	1.837%
7	7.458	685	692	702	rBV	786578	1216560	18.30%	1.628%
8	7.664	719	727	738	rBV	895012	1449200	21.80%	1.940%
9	7.746	738	741	747	rVB4	9396	14496	0.22%	0.019%
10	8.140	801	808	817	rBV	1209243	1924673	28.96%	2.576%
11	8.852	921	929	942	rBV	1090323	1873968	28.20%	2.508%
12	8.975	944	950	959	rVB	126143	215508	3.24%	0.288%
13	9.316	1001	1008	1020	rBV	880958	1457215	21.92%	1.950%
14	9.711	1071	1075	1080	rVB2	13482	21694	0.33%	0.029%
15	10.046	1124	1132	1143	rBV	721879	1193634	17.96%	1.598%
16	10.405	1188	1193	1202	rVB2	13412	27342	0.41%	0.037%
17	10.587	1217	1224	1241	rBV	1114850	1920608	28.90%	2.571%
18	10.969	1280	1289	1299	rBV	1765413	3033704	45.64%	4.061%
19	11.105	1305	1312	1330	rBV	1093383	2036515	30.64%	2.726%
20	11.522	1378	1383	1387	rBV8	5026	10095	0.15%	0.014%
21	11.781	1419	1427	1429	rBV9	6665	12122	0.18%	0.016%
22	12.210	1495	1500	1503	rBV4	6382	8799	0.13%	0.012%
23	13.669	1741	1748	1754	rBV2	17019	27992	0.42%	0.037%
24	14.104	1819	1822	1826	rBV6	4513	7930	0.12%	0.011%
25	14.181	1828	1835	1850	rVV	2382513	3479014	52.34%	4.657%
26	14.299	1850	1855	1860	rVB9	6568	15712	0.24%	0.021%
27	14.481	1878	1886	1903	rBV	2775783	4214675	63.41%	5.641%
28	14.781	1930	1937	1947	rBV	3008892	4474731	67.33%	5.989%
29	14.969	1962	1969	1990	rBV	804677	1366990	20.57%	1.830%
30	15.134	1995	1997	2002	rVV6	8879	16750	0.25%	0.022%
31	15.193	2004	2007	2013	rVB8	10477	17400	0.26%	0.023%
32	15.587	2071	2074	2078	rVB2	7211	9993	0.15%	0.013%
33	15.728	2094	2098	2099	rBV4	6424	7036	0.11%	0.009%
34	15.775	2099	2106	2119	rVV	3783057	5274955	79.37%	7.060%
35	15.893	2119	2126	2139	rVV	939759	1388671	20.89%	1.859%
36	16.016	2143	2147	2151	rVB3	17964	28148	0.42%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015075.D
 Acq On : 15 May 2023 15:13
 Operator : CG/JU
 Sample : 02592-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JRED9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	16.134	2162	2167	2173	rBV	62810	91735	1.38%	0.123%
38	16.563	2234	2240	2245	rBV9	4512	8460	0.13%	0.011%
39	16.987	2307	2312	2315	rBV6	6341	10883	0.16%	0.015%
40	17.069	2321	2326	2330	rBV8	7326	13232	0.20%	0.018%
41	17.210	2346	2350	2356	rVB9	6375	10972	0.17%	0.015%
42	17.322	2366	2369	2376	rVB3	9080	16576	0.25%	0.022%
43	17.540	2399	2406	2415	rBV	3878748	5563857	83.71%	7.447%
44	17.634	2416	2422	2435	rVV2	3812816	5606446	84.35%	7.504%
45	18.181	2512	2515	2518	rBV5	10262	13622	0.20%	0.018%
46	18.287	2530	2533	2537	rVB5	7076	9328	0.14%	0.012%
47	18.392	2548	2551	2557	rBV5	18616	30844	0.46%	0.041%
48	18.469	2561	2564	2567	rBV2	7399	10816	0.16%	0.014%
49	18.957	2643	2647	2653	rBV2	25803	35744	0.54%	0.048%
50	19.169	2681	2683	2687	rVB2	17932	16614	0.25%	0.022%
51	19.434	2724	2728	2736	rVB2	64171	99744	1.50%	0.134%
52	19.857	2794	2800	2811	rBV	4881680	6646374	100.00%	8.896%
53	21.616	3094	3099	3107	rBV	4248851	5784643	87.03%	7.743%
54	24.022	3501	3508	3525	rVB2	2954980	6440021	96.90%	8.620%
55	24.192	3530	3537	3550	rVB	2876964	6076989	91.43%	8.134%




Sum of corrected areas: 74711120

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015075.D
Acq On : 15 May 2023 15:13
Operator : CG/JU
Sample : 02592-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JRED9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

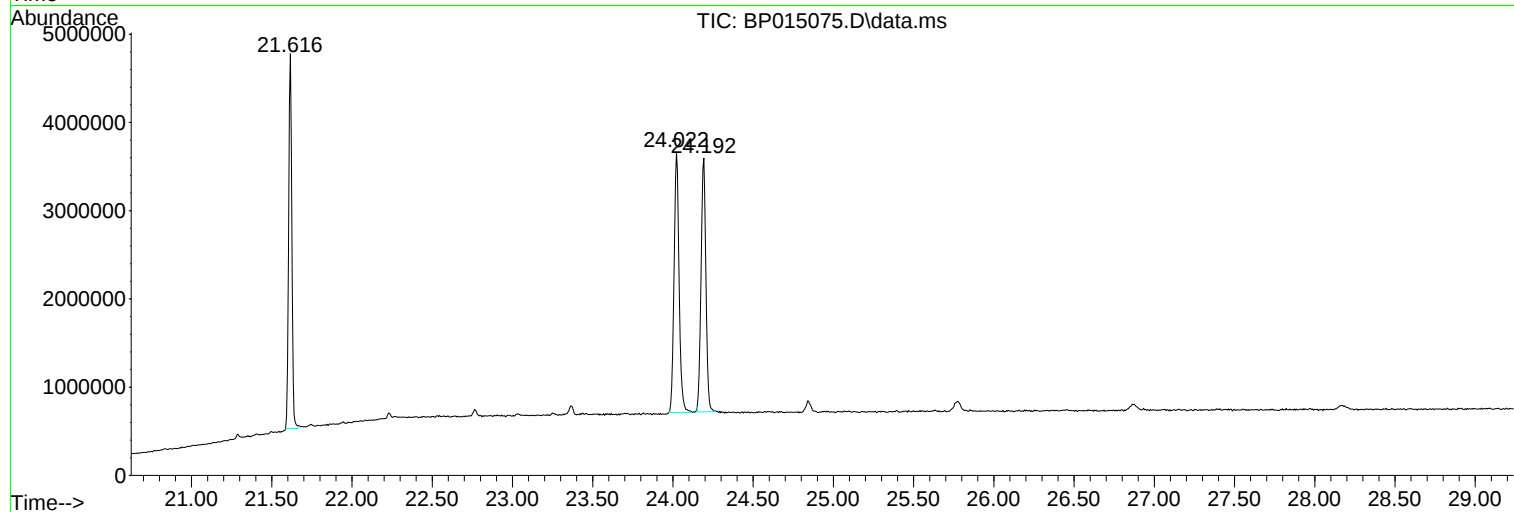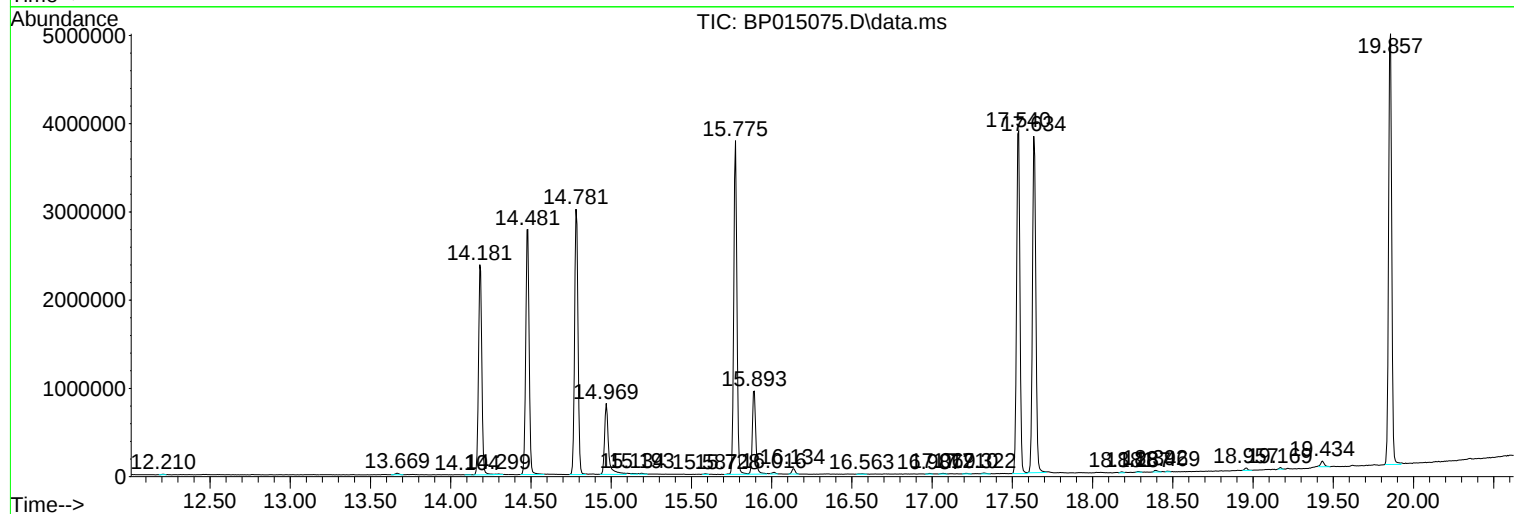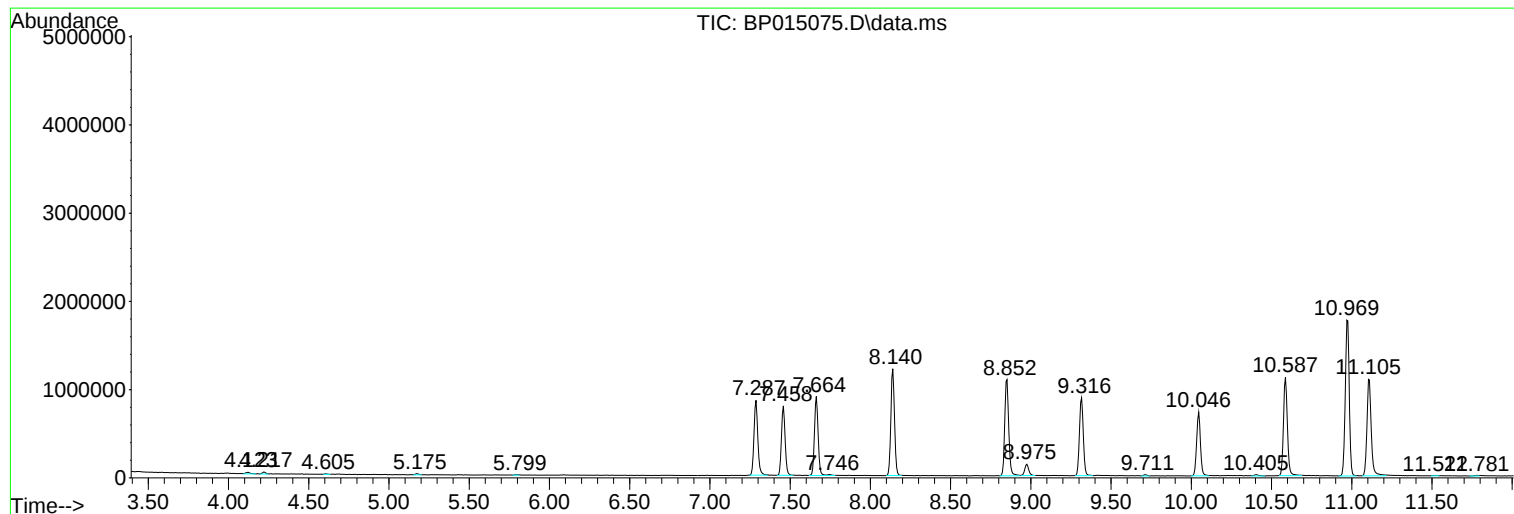

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015075.D
Acq On : 15 May 2023 15:13
Operator : CG/JU
Sample : 02592-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JRED9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015075.D
Acq On : 15 May 2023 15:13
Operator : CG/JU
Sample : 02592-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JRED9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------