

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015076.D
 Acq On : 15 May 2023 15:46
 Operator : CG/JU
 Sample : 02592-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015076.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.993	99	103	108	rVB	22209	28705	0.62%	0.052%
2	4.123	121	125	130	rVB	16927	28693	0.62%	0.052%
3	4.222	137	142	147	rBV	21317	31375	0.68%	0.057%
4	4.387	166	170	176	rBV4	16396	26718	0.58%	0.048%
5	4.452	177	181	187	rVB	27099	39478	0.86%	0.071%
6	4.881	250	254	259	rVB2	29138	42453	0.92%	0.076%
7	5.175	300	304	312	rVB2	13087	25325	0.55%	0.046%
8	5.281	320	322	327	rVB4	6353	6562	0.14%	0.012%
9	5.787	406	408	413	rVB6	3755	4747	0.10%	0.009%
10	6.081	456	458	466	rVB3	8588	11114	0.24%	0.020%
11	7.287	654	663	676	rBV	624981	1083756	23.51%	1.952%
12	7.458	685	692	700	rBV	577474	915283	19.85%	1.648%
13	7.558	705	709	714	rVB7	2614	5025	0.11%	0.009%
14	7.663	720	727	737	rBV	671882	1077973	23.38%	1.941%
15	7.740	737	740	745	rVB5	8303	13090	0.28%	0.024%
16	8.140	800	808	819	rBV	1003932	1654179	35.88%	2.979%
17	8.846	922	928	943	rBV	825398	1395960	30.28%	2.514%
18	8.969	943	949	959	rVB	186688	320944	6.96%	0.578%
19	9.110	969	973	974	rBV4	5969	7024	0.15%	0.013%
20	9.310	1000	1007	1020	rBV	640803	1085382	23.54%	1.955%
21	9.416	1020	1025	1032	rVV3	20294	36986	0.80%	0.067%
22	9.710	1070	1075	1080	rVB3	7884	12565	0.27%	0.023%
23	10.040	1123	1131	1145	rBV	500168	867952	18.82%	1.563%
24	10.199	1152	1158	1165	rBV2	17436	49169	1.07%	0.089%
25	10.405	1187	1193	1204	rVB2	31386	57359	1.24%	0.103%
26	10.581	1215	1223	1237	rVV	773596	1365557	29.62%	2.459%
27	10.969	1280	1289	1297	rBV	1553398	2588554	56.14%	4.662%
28	11.104	1304	1312	1325	rBV	816872	1469785	31.88%	2.647%
29	11.510	1374	1381	1386	rBV6	15414	34221	0.74%	0.062%
30	11.763	1418	1424	1433	rBV	12149	30984	0.67%	0.056%
31	12.204	1496	1499	1505	rBV7	4019	6331	0.14%	0.011%
32	12.328	1516	1520	1523	rBV6	5695	7819	0.17%	0.014%
33	12.751	1587	1592	1595	rBV7	3020	5282	0.11%	0.010%
34	13.663	1742	1747	1752	rVB3	11494	19863	0.43%	0.036%
35	14.181	1828	1835	1847	rBV	1783695	2425569	52.61%	4.368%
36	14.475	1878	1885	1897	rBV2	1982570	2929359	63.53%	5.276%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015076.D
 Acq On : 15 May 2023 15:46
 Operator : CG/JU
 Sample : 02592-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	14.781	1929	1937	1949	rBV	2514868	3717530	80.63%	6.695%
38	14.875	1951	1953	1959	rVB7	3243	5111	0.11%	0.009%
39	14.963	1962	1968	1989	rBV	527711	978624	21.23%	1.763%
40	15.587	2069	2074	2078	rVB	18782	25791	0.56%	0.046%
41	15.769	2099	2105	2116	rBV	2523667	3616021	78.43%	6.512%
42	15.887	2119	2125	2140	rVV	694061	978404	21.22%	1.762%
43	16.010	2142	2146	2154	rVB6	13601	23366	0.51%	0.042%
44	16.557	2232	2239	2242	rBV9	5797	8901	0.19%	0.016%
45	16.981	2307	2311	2318	rBV6	7384	11606	0.25%	0.021%
46	17.204	2346	2349	2355	rVB8	4886	7310	0.16%	0.013%
47	17.322	2365	2369	2374	rVV2	8346	14571	0.32%	0.026%
48	17.534	2398	2405	2415	rBV	3250376	4559737	98.89%	8.212%
49	17.634	2415	2422	2436	rVV	2687361	3887235	84.31%	7.001%
50	17.804	2447	2451	2454	rBV3	4714	5979	0.13%	0.011%
51	18.022	2484	2488	2492	rBV7	7594	15060	0.33%	0.027%
52	18.175	2512	2514	2518	rVB5	5914	5937	0.13%	0.011%
53	18.386	2548	2550	2557	rBV8	10892	18452	0.40%	0.033%
54	18.475	2561	2565	2566	rBV3	8047	12374	0.27%	0.022%
55	18.951	2642	2646	2650	rBV2	42417	54698	1.19%	0.099%
56	19.163	2679	2682	2687	rBV	29958	37965	0.82%	0.068%
57	19.428	2724	2727	2735	rVB5	63413	114993	2.49%	0.207%
58	19.851	2793	2799	2808	rBV	3412740	4453111	96.58%	8.020%
59	21.610	3093	3098	3107	rBV	3379347	4610705	100.00%	8.304%
60	24.016	3500	3507	3519	rBV2	1816452	4068864	88.25%	7.328%
61	24.186	3529	3536	3548	rVB	2132802	4581195	99.36%	8.251%




Sum of corrected areas: 55524681

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015076.D
Acq On : 15 May 2023 15:46
Operator : CG/JU
Sample : 02592-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

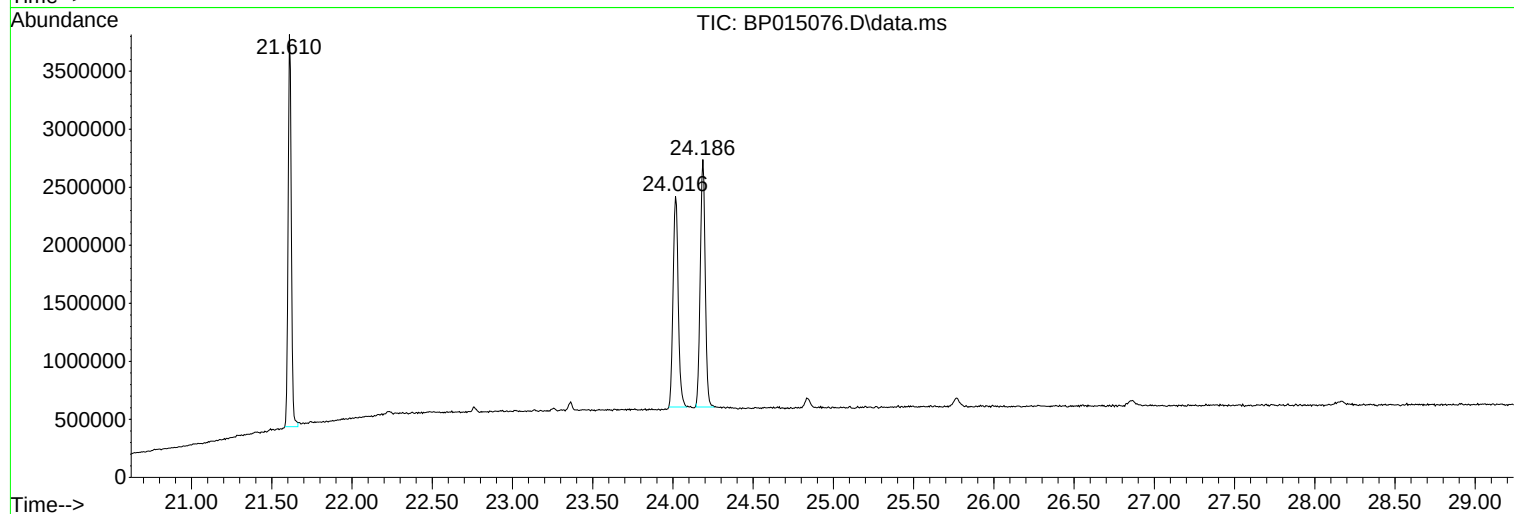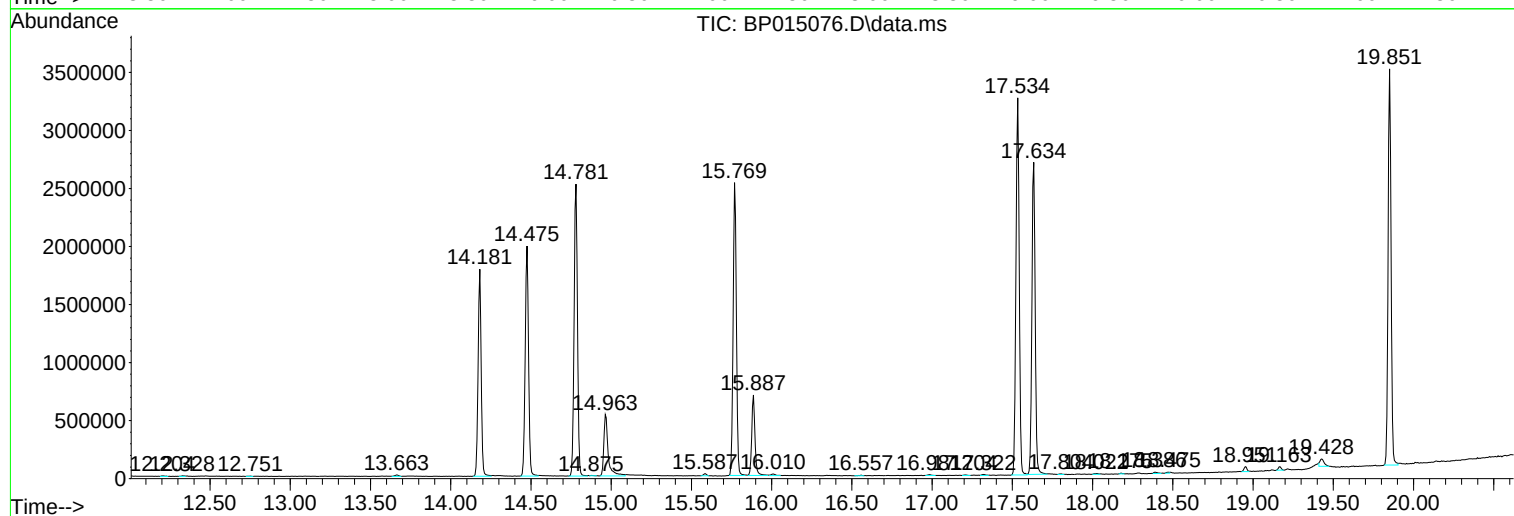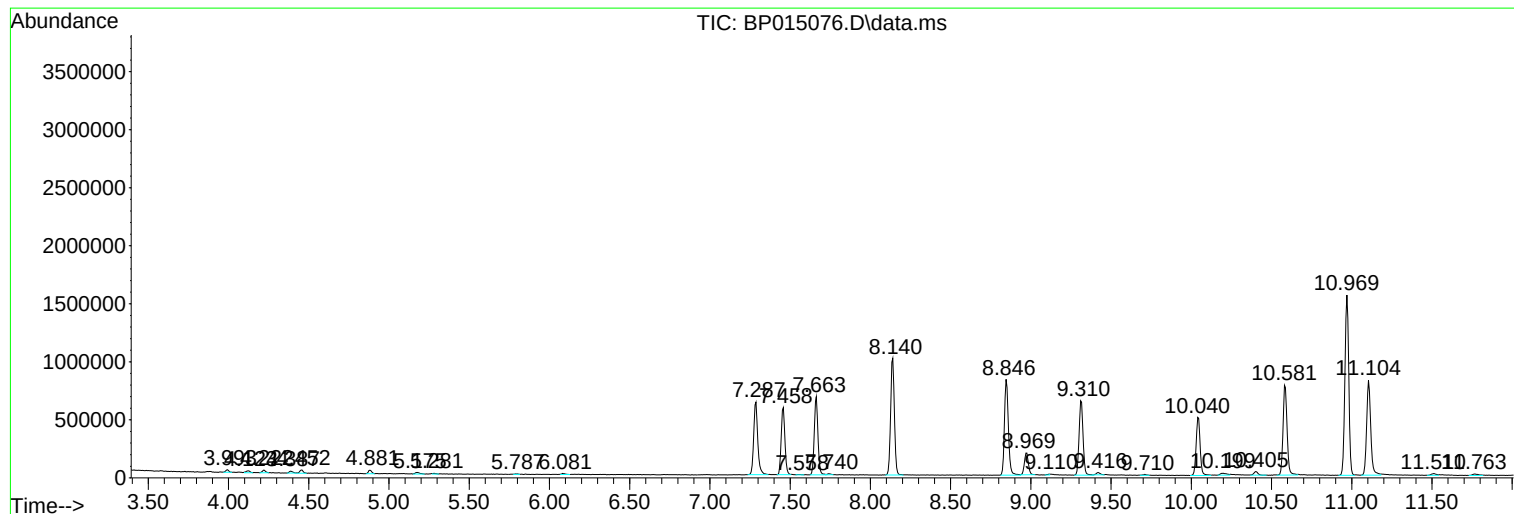

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015076.D
Acq On : 15 May 2023 15:46
Operator : CG/JU
Sample : 02592-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015076.D
Acq On : 15 May 2023 15:46
Operator : CG/JU
Sample : 02592-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc