

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015085.D
 Acq On : 15 May 2023 21:23
 Operator : CG/JU
 Sample : 02592-20
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	18	rVB	141689	203732	1.12%	0.119%
2	3.876	79	83	101	rBV	1858661	2882133	15.90%	1.679%
3	4.217	138	141	149	rVB	27996	43178	0.24%	0.025%
4	4.564	196	200	207	rBV	56837	74604	0.41%	0.043%
5	7.287	650	663	677	rBV	2897043	4778610	26.36%	2.783%
6	7.458	682	692	703	rVB	2575254	4030815	22.24%	2.348%
7	7.664	719	727	740	rBV	2966273	4823874	26.61%	2.809%
8	8.134	800	807	817	rBV	1327449	2108774	11.63%	1.228%
9	8.846	920	928	942	rBV	3882507	6579345	36.30%	3.832%
10	9.316	999	1008	1019	rBV	3022477	5013772	27.66%	2.920%
11	9.710	1069	1075	1082	rVB2	19064	27208	0.15%	0.016%
12	10.040	1123	1131	1144	rBV	2551318	4250609	23.45%	2.476%
13	10.581	1214	1223	1241	rBV	3862241	6601001	36.42%	3.844%
14	10.969	1281	1289	1297	rBV	1988209	3324618	18.34%	1.936%
15	11.105	1303	1312	1329	rBV	3978913	6968606	38.44%	4.059%
16	12.204	1494	1499	1505	rVB2	14518	21890	0.12%	0.013%
17	12.546	1551	1557	1569	rBV2	48989	93411	0.52%	0.054%
18	13.575	1726	1732	1737	rBV10	9225	24560	0.14%	0.014%
19	13.663	1742	1747	1752	rVV2	19408	32101	0.18%	0.019%
20	13.751	1752	1762	1768	rVV7	11927	28153	0.16%	0.016%
21	14.181	1827	1835	1849	rBV	7093754	10253468	56.57%	5.972%
22	14.299	1849	1855	1859	rVB9	10986	24000	0.13%	0.014%
23	14.475	1877	1885	1900	rBV2	8341614	12754737	70.36%	7.428%
24	14.581	1900	1903	1910	rVB4	9910	18715	0.10%	0.011%
25	14.775	1929	1936	1945	rBV	3003973	4590460	25.32%	2.673%
26	14.869	1948	1952	1961	rVB8	16015	30700	0.17%	0.018%
27	14.969	1961	1969	1993	rBV	3471346	5336391	29.44%	3.108%
28	15.181	2001	2005	2011	rVB6	30811	57177	0.32%	0.033%
29	15.769	2098	2105	2118	rVB	9742252	15111675	83.37%	8.801%
30	15.887	2118	2125	2136	rBV	3570385	4917810	27.13%	2.864%
31	16.010	2141	2146	2150	rVB	50884	76541	0.42%	0.045%
32	16.128	2161	2166	2177	rVB	214418	304717	1.68%	0.177%
33	16.551	2233	2238	2243	rBV7	12456	21071	0.12%	0.012%
34	16.981	2305	2311	2314	rBV5	12575	18550	0.10%	0.011%
35	17.204	2345	2349	2356	rVB5	14357	24042	0.13%	0.014%
36	17.322	2363	2369	2374	rVB2	10485	18727	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015085.D
 Acq On : 15 May 2023 21:23
 Operator : CG/JU
 Sample : 02592-20
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	17.534	2398	2405	2413	rBV	3687481	5443801	30.03%	3.170%
38	17.634	2415	2422	2433	rVV2	10733256	16014319	88.35%	9.327%
39	17.710	2433	2435	2447	rVV7	47390	86868	0.48%	0.051%
40	17.904	2466	2468	2476	rVB3	13209	18611	0.10%	0.011%
41	18.169	2510	2513	2517	rVB5	16633	20876	0.12%	0.012%
42	18.275	2527	2531	2535	rBV7	15561	23928	0.13%	0.014%
43	18.387	2545	2550	2558	rBV	278923	423846	2.34%	0.247%
44	18.457	2560	2562	2566	rVB	18711	24787	0.14%	0.014%
45	19.269	2697	2700	2704	rVB2	42512	48289	0.27%	0.028%
46	19.422	2722	2726	2732	rBV	152930	209700	1.16%	0.122%
47	19.492	2732	2738	2743	rBV	133028	210147	1.16%	0.122%
48	19.610	2754	2758	2764	rBV3	67470	97702	0.54%	0.057%
49	19.851	2792	2799	2813	rBV	13091253	18126577	100.00%	10.557%
50	20.345	2880	2883	2886	rVB	63408	67218	0.37%	0.039%
51	21.280	3039	3042	3049	rBV	295627	424354	2.34%	0.247%
52	21.604	3092	3097	3106	rBV	3654521	5160511	28.47%	3.005%
53	24.016	3498	3507	3518	rBV2	6847253	15225749	84.00%	8.868%
54	24.180	3528	3535	3550	rVB	2127875	4605606	25.41%	2.682%




Sum of corrected areas: 171702664

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015085.D
Acq On : 15 May 2023 21:23
Operator : CG/JU
Sample : 02592-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

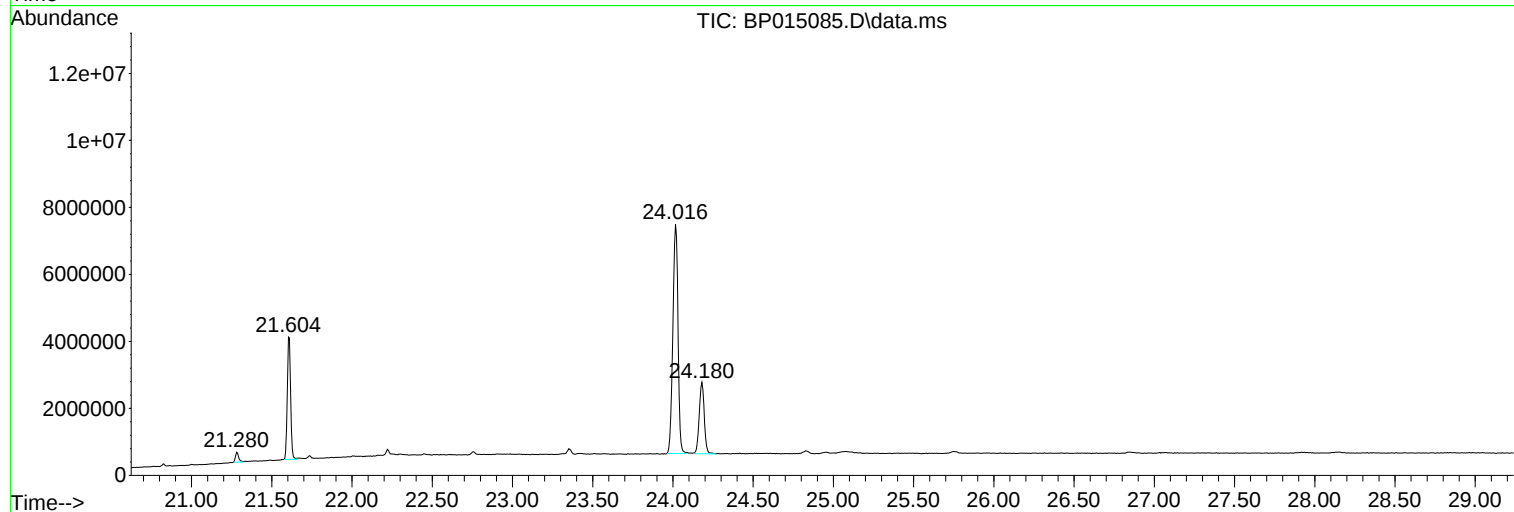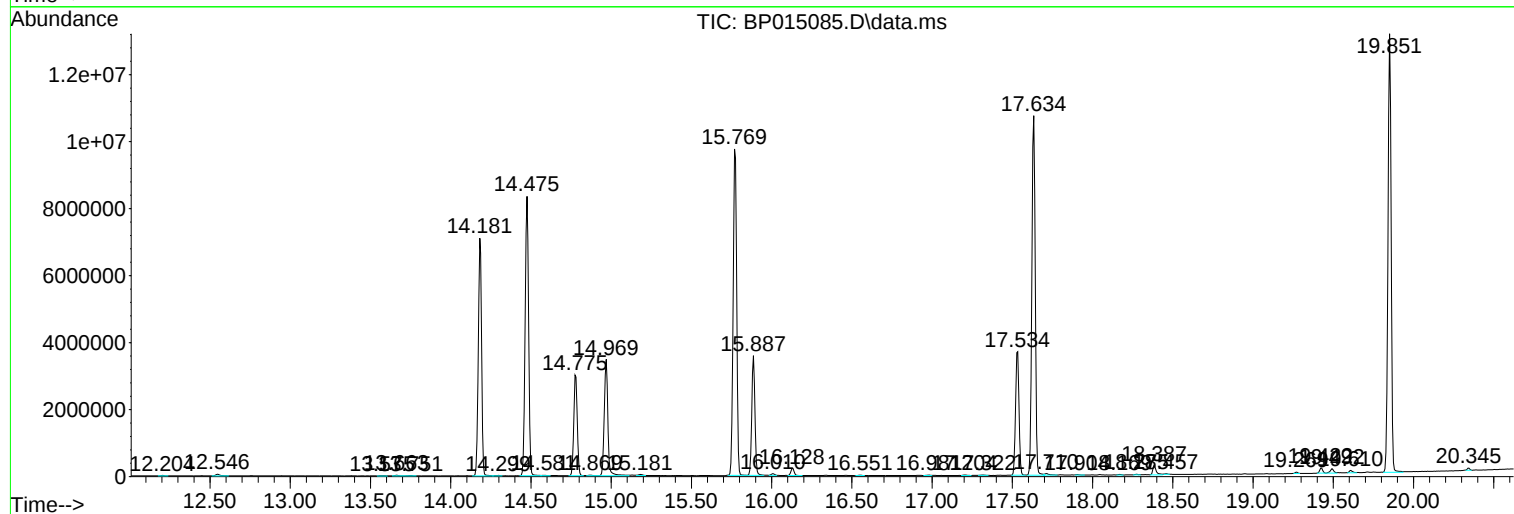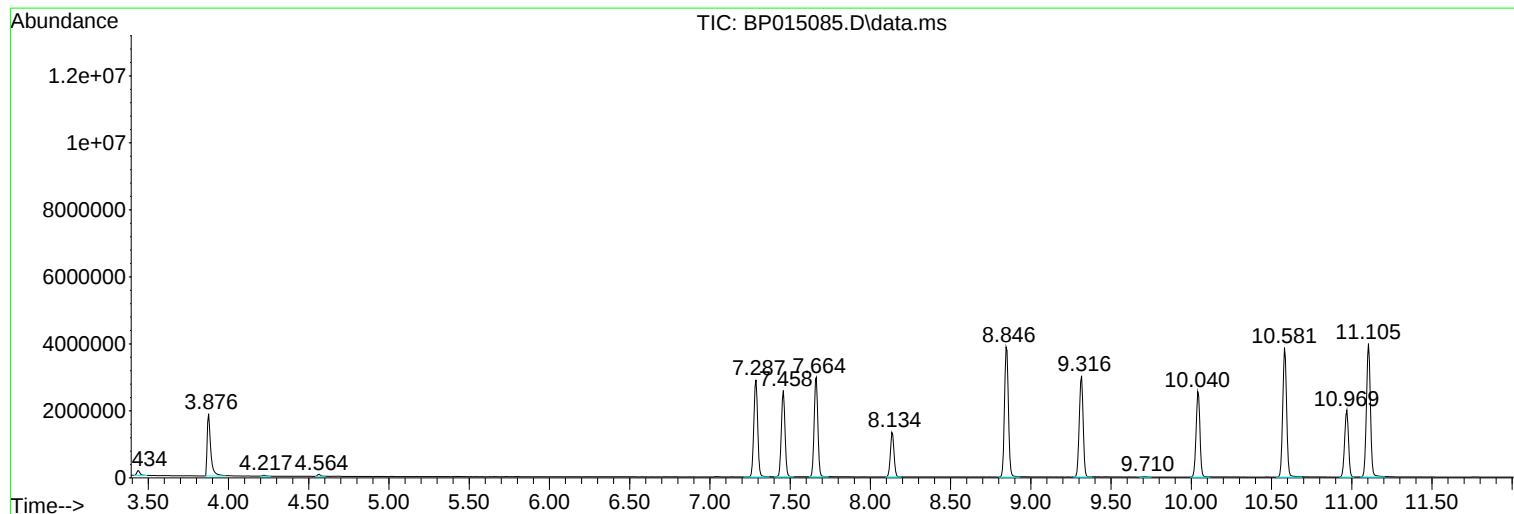

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015085.D
Acq On : 15 May 2023 21:23
Operator : CG/JU
Sample : 02592-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015085.D
Acq On : 15 May 2023 21:23
Operator : CG/JU
Sample : 02592-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc