

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015086.D
 Acq On : 15 May 2023 21:56
 Operator : CG/JU
 Sample : 02592-21
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.887	83	85	99	rBV	108634	177631	2.84%	0.251%
2	3.993	99	103	108	rVB2	18197	30794	0.49%	0.044%
3	4.117	120	124	131	rVB2	21815	33781	0.54%	0.048%
4	4.217	137	141	148	rVB2	19909	29778	0.48%	0.042%
5	4.611	205	208	212	rBV4	9161	12061	0.19%	0.017%
6	4.681	215	220	231	rVB	25391	44977	0.72%	0.064%
7	5.175	299	304	309	rBV	17296	27253	0.44%	0.039%
8	5.669	384	388	396	rVB	8090	12202	0.20%	0.017%
9	5.793	406	409	416	rVB	13556	18979	0.30%	0.027%
10	7.240	651	655	656	rBV	19981	23153	0.37%	0.033%
11	7.281	656	662	679	rVB	863671	1448543	23.15%	2.047%
12	7.452	685	691	702	rVB	750179	1195920	19.11%	1.690%
13	7.658	719	726	737	rBV	904113	1432063	22.89%	2.024%
14	7.740	737	740	746	rVB7	8027	12903	0.21%	0.018%
15	8.134	799	807	816	rBV	1136991	1811289	28.95%	2.560%
16	8.846	920	928	943	rBV	1170595	1930116	30.85%	2.728%
17	8.969	943	949	965	rVB	193946	331204	5.29%	0.468%
18	9.310	1000	1007	1020	rBV	908456	1470213	23.50%	2.078%
19	9.416	1020	1025	1030	rVV6	9318	18289	0.29%	0.026%
20	9.469	1030	1034	1038	rVB7	4880	7381	0.12%	0.010%
21	9.710	1069	1075	1080	rVB	59269	92816	1.48%	0.131%
22	10.040	1119	1131	1146	rBV	731923	1221828	19.53%	1.727%
23	10.187	1149	1156	1163	rBV5	10295	26738	0.43%	0.038%
24	10.399	1188	1192	1197	rVB3	16896	27117	0.43%	0.038%
25	10.581	1215	1223	1234	rBV	1160063	1946077	31.10%	2.751%
26	10.969	1279	1289	1302	rBV	1717710	2891620	46.21%	4.087%
27	11.104	1304	1312	1327	rBV	1048659	1937029	30.96%	2.738%
28	11.763	1416	1424	1430	rBV5	11440	27845	0.44%	0.039%
29	12.204	1494	1499	1504	rVB	40031	55898	0.89%	0.079%
30	12.445	1534	1540	1542	rBV7	5023	9244	0.15%	0.013%
31	12.551	1554	1558	1563	rVB7	6112	9873	0.16%	0.014%
32	13.663	1740	1747	1753	rVV	67151	106907	1.71%	0.151%
33	13.734	1756	1759	1766	rVB9	7593	15712	0.25%	0.022%
34	14.175	1828	1834	1849	rBV	2264893	3248063	51.91%	4.591%
35	14.292	1849	1854	1860	rVV10	5534	15038	0.24%	0.021%
36	14.357	1862	1865	1870	rVB2	6800	9549	0.15%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015086.D
 Acq On : 15 May 2023 21:56
 Operator : CG/JU
 Sample : 02592-21
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREE6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	14.475	1876	1885	1900	rBV	2600714	3965999	63.38%	5.606%
38	14.722	1922	1927	1930	rBV	12920	20815	0.33%	0.029%
39	14.775	1930	1936	1947	rVB	2636174	4086401	65.31%	5.776%
40	14.869	1949	1952	1958	rVB8	5332	9731	0.16%	0.014%
41	14.963	1961	1968	1983	rBV	874497	1448010	23.14%	2.047%
42	15.181	2001	2005	2016	rVB	17796	32986	0.53%	0.047%
43	15.728	2092	2098	2099	rBV	33827	43064	0.69%	0.061%
44	15.769	2099	2105	2117	rVV	3390189	4894087	78.21%	6.917%
45	15.881	2118	2124	2140	rVV	993924	1427439	22.81%	2.018%
46	16.010	2140	2146	2153	rVB4	17597	33601	0.54%	0.047%
47	16.128	2160	2166	2175	rBV	423766	586839	9.38%	0.829%
48	16.522	2230	2233	2236	rBV2	5572	7400	0.12%	0.010%
49	16.698	2257	2263	2269	rBV	68124	95185	1.52%	0.135%
50	16.981	2306	2311	2317	rBV	32164	46477	0.74%	0.066%
51	17.204	2347	2349	2355	rVB7	6991	8822	0.14%	0.012%
52	17.263	2355	2359	2361	rBV5	5082	6380	0.10%	0.009%
53	17.316	2365	2368	2373	rVB5	6607	10382	0.17%	0.015%
54	17.528	2398	2404	2414	rBV	3384419	4952428	79.15%	7.000%
55	17.628	2415	2421	2431	rVV	3597182	5293439	84.60%	7.482%
56	17.733	2433	2439	2446	rVB	53481	94674	1.51%	0.134%
57	17.945	2473	2475	2478	rVB4	7420	7489	0.12%	0.011%
58	18.010	2483	2486	2489	rVV5	7605	12566	0.20%	0.018%
59	18.045	2489	2492	2498	rVB3	27740	39425	0.63%	0.056%
60	18.175	2510	2514	2519	rBV7	7515	15277	0.24%	0.022%
61	18.380	2545	2549	2557	rBV2	138454	221815	3.54%	0.314%
62	18.951	2642	2646	2650	rVB	60015	68630	1.10%	0.097%
63	19.075	2664	2667	2671	rBV	21959	29876	0.48%	0.042%
64	19.163	2679	2682	2687	rBV2	23864	28745	0.46%	0.041%
65	19.427	2723	2727	2732	rVB5	67719	104672	1.67%	0.148%
66	19.610	2755	2758	2765	rBV3	58909	85616	1.37%	0.121%
67	19.716	2773	2776	2779	rVB2	30416	35145	0.56%	0.050%
68	19.851	2793	2799	2811	rBV	4576169	6257353	100.00%	8.844%
69	21.280	3039	3042	3051	rBV2	160442	243166	3.89%	0.344%
70	21.610	3092	3098	3107	rBV	3486562	4858679	77.65%	6.867%
71	24.010	3499	3506	3519	rVB2	2488066	5365124	85.74%	7.583%
72	24.180	3528	3535	3552	rVB	2138188	4601980	73.55%	6.505%




Sum of corrected areas: 70749601

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015086.D
Acq On : 15 May 2023 21:56
Operator : CG/JU
Sample : 02592-21
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

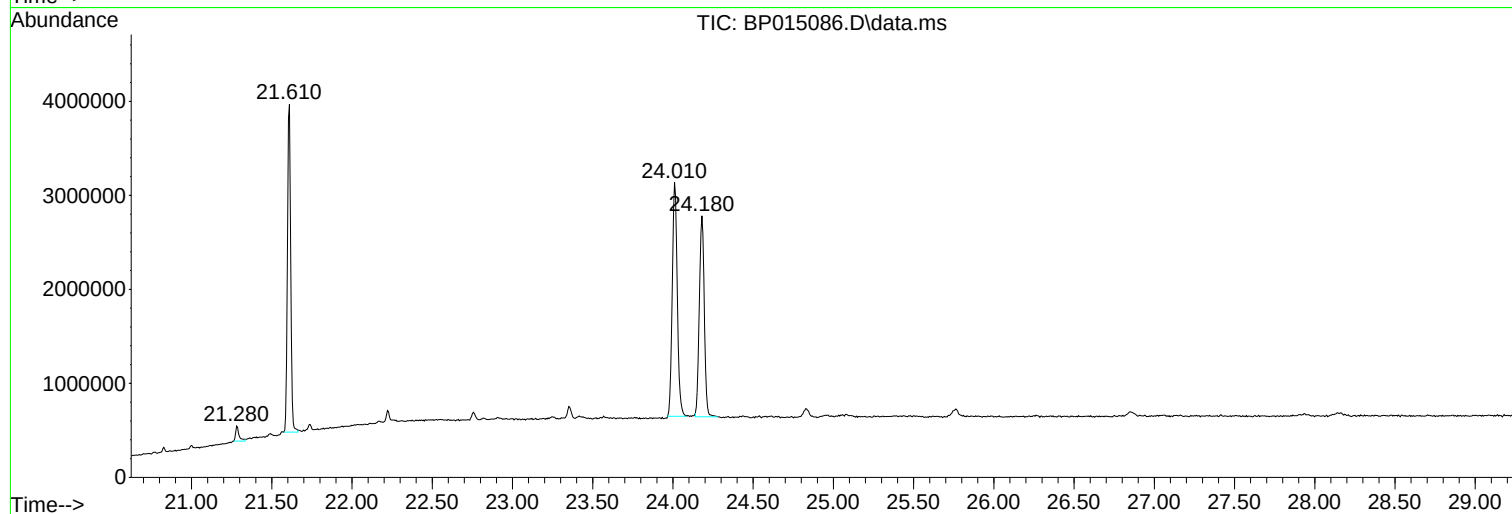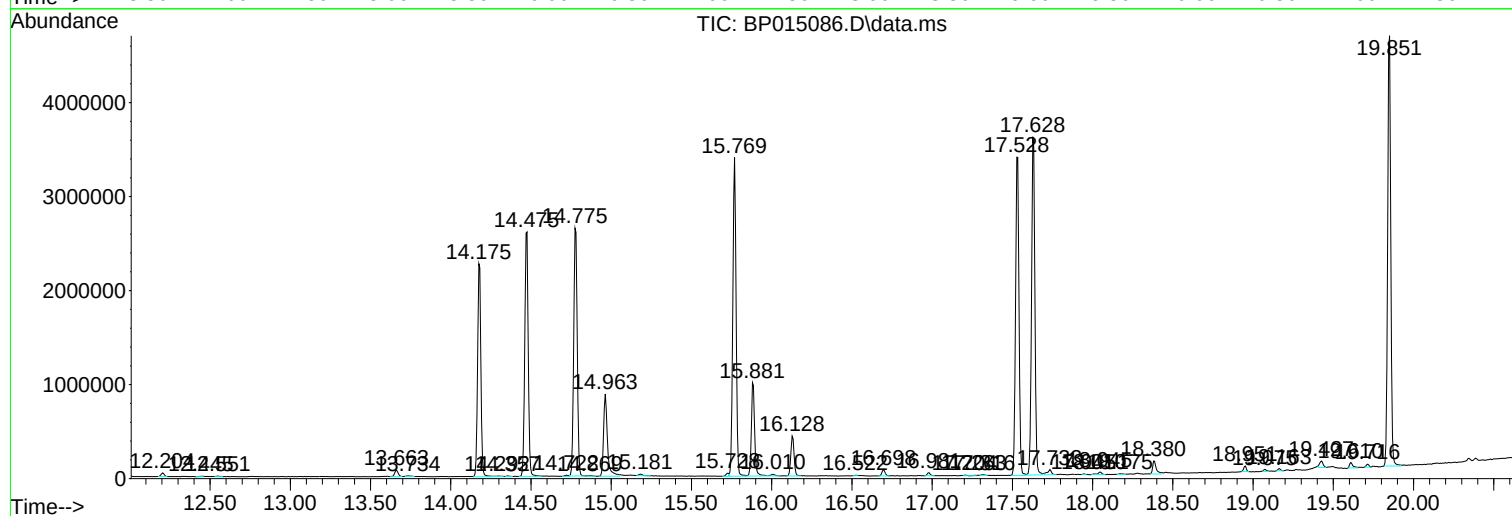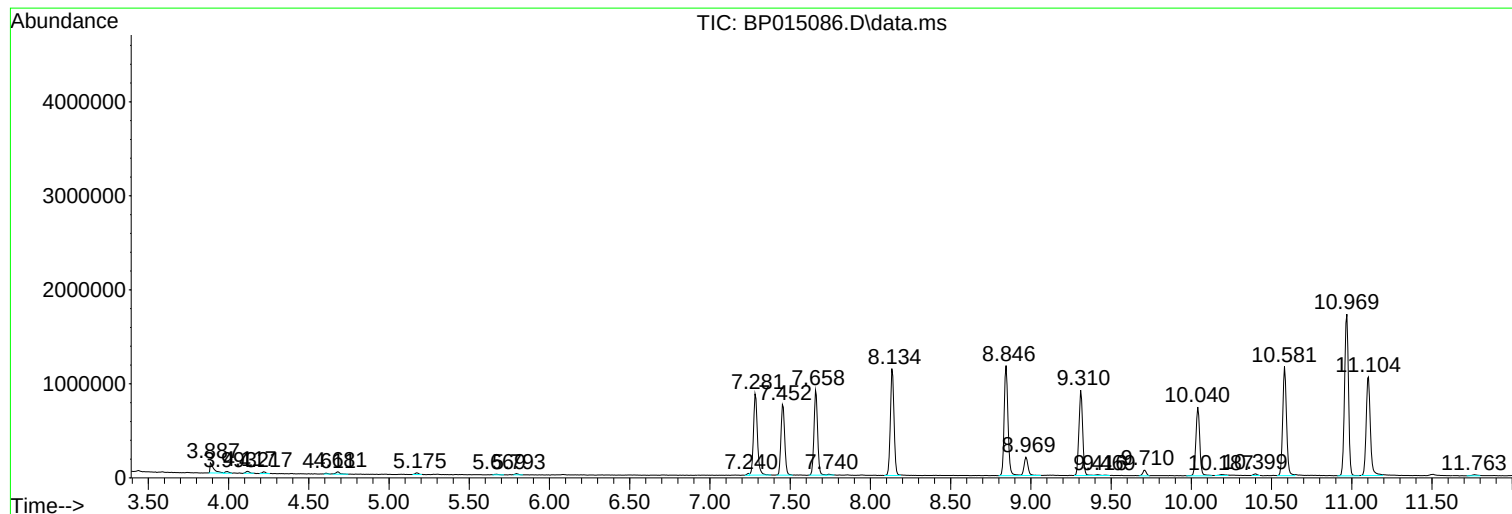

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015086.D
Acq On : 15 May 2023 21:56
Operator : CG/JU
Sample : 02592-21
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREE6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.128	2.87 ng/ul	586839	Acenaphthene-d10	14.775

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	95
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Benzophenone	182	C13H10O	000119-61-9	91

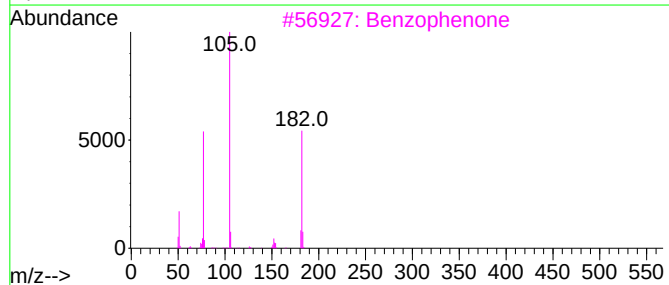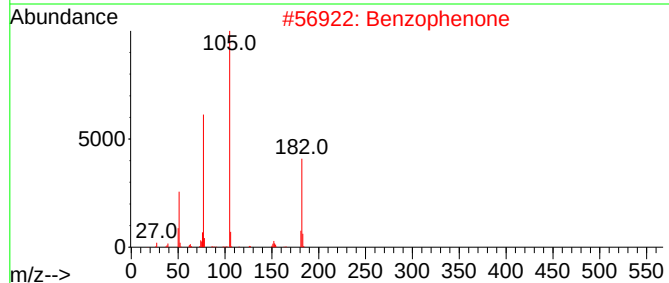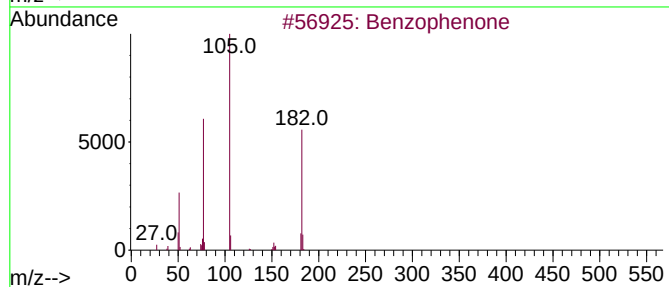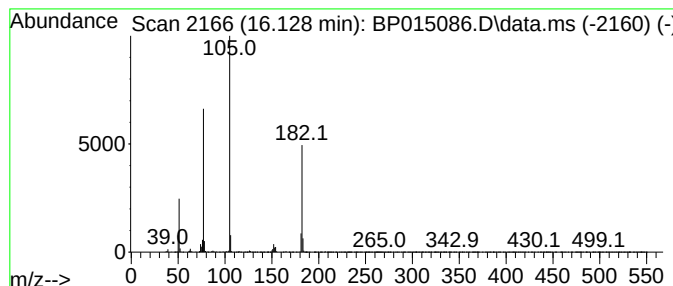

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015086.D
Acq On : 15 May 2023 21:56
Operator : CG/JU
Sample : 02592-21
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREE6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	16.128	2.9	ng/u1	586839	3	14.775	4086400	20.0