

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015090.D
 Acq On : 16 May 2023 00:10
 Operator : CG/JU
 Sample : 02592-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREG1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.116	121	124	133	rVB4	15123	27803	0.50%	0.048%
2	4.216	138	141	147	rVB	16908	24101	0.44%	0.042%
3	5.175	300	304	312	rVB2	13037	25908	0.47%	0.045%
4	7.281	653	662	678	rBV	611503	1045534	18.98%	1.802%
5	7.452	685	691	703	rVB	549180	864098	15.69%	1.490%
6	7.657	719	726	736	rBV	629966	1025949	18.63%	1.769%
7	7.740	737	740	744	rVB3	6817	9427	0.17%	0.016%
8	8.134	800	807	816	rBV	1136187	1831686	33.26%	3.158%
9	8.846	918	928	942	rBV	822658	1386409	25.17%	2.390%
10	8.969	944	949	958	rVB	113155	187872	3.41%	0.324%
11	9.310	1000	1007	1018	rBV	631636	1054196	19.14%	1.817%
12	9.416	1021	1025	1031	rVV9	6843	13984	0.25%	0.024%
13	9.463	1031	1033	1038	rVB6	4812	7957	0.14%	0.014%
14	9.710	1071	1075	1078	rVB3	9157	10362	0.19%	0.018%
15	10.040	1122	1131	1142	rBV	512795	863645	15.68%	1.489%
16	10.398	1187	1192	1200	rVB	10961	20351	0.37%	0.035%
17	10.581	1214	1223	1236	rBV	803673	1381490	25.08%	2.381%
18	10.963	1279	1288	1299	rBV	1729558	2931979	53.23%	5.054%
19	11.098	1304	1311	1325	rBV	836162	1496207	27.16%	2.579%
20	11.781	1418	1427	1432	rBV	7059	22241	0.40%	0.038%
21	12.204	1495	1499	1504	rVB4	4776	7011	0.13%	0.012%
22	12.451	1537	1541	1548	rVB10	2543	6274	0.11%	0.011%
23	13.663	1742	1747	1752	rVB2	12413	20616	0.37%	0.036%
24	14.175	1826	1834	1844	rBV	1676857	2340290	42.49%	4.034%
25	14.469	1877	1884	1898	rBV	1964960	2892720	52.52%	4.987%
26	14.775	1929	1936	1948	rBV	2821347	4229956	76.80%	7.292%
27	14.963	1961	1968	1990	rBV	532775	983387	17.85%	1.695%
28	15.175	2002	2004	2010	rVB7	5158	9085	0.16%	0.016%
29	15.586	2065	2074	2079	rBV9	5776	12495	0.23%	0.022%
30	15.769	2098	2105	2118	rBV	2413193	3582344	65.04%	6.175%
31	15.881	2118	2124	2137	rVV	634818	921619	16.73%	1.589%
32	16.004	2141	2145	2151	rVB5	13691	25382	0.46%	0.044%
33	16.122	2159	2165	2169	rVB9	3842	7681	0.14%	0.013%
34	16.557	2235	2239	2243	rVB6	4077	6650	0.12%	0.011%
35	16.975	2307	2310	2313	rBV4	5987	6836	0.12%	0.012%
36	17.316	2364	2368	2373	rBV4	7381	11665	0.21%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015090.D
Acq On : 16 May 2023 00:10
Operator : CG/JU
Sample : 02592-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Title : SVOA CALIBRATION

37	17.527	2397	2404	2414	rBV	3609863	5140693	93.33%	8.862%
38	17.627	2415	2421	2437	rVB	2706692	3818814	69.33%	6.583%
39	18.169	2510	2513	2517	rBV6	10193	14971	0.27%	0.026%
40	18.386	2546	2550	2558	rBV5	28703	48350	0.88%	0.083%
41	18.945	2642	2645	2650	rVB3	17652	23962	0.44%	0.041%
42	19.163	2679	2682	2685	rBV2	13758	17932	0.33%	0.031%
43	19.216	2688	2691	2694	rVV5	13362	19100	0.35%	0.033%
44	19.422	2723	2726	2734	rVB6	45927	72246	1.31%	0.125%
45	19.610	2755	2758	2764	rBV7	19881	31398	0.57%	0.054%
46	19.845	2793	2798	2808	rBV	3468298	4344950	78.88%	7.490%
47	21.604	3092	3097	3111	rBV	3954962	5358349	97.28%	9.237%
48	24.004	3498	3505	3516	rBV2	1971606	4315564	78.35%	7.439%
49	24.174	3527	3534	3545	rVB	2531478	5507993	100.00%	9.495%




Sum of corrected areas: 58009532

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015090.D
Acq On : 16 May 2023 00:10
Operator : CG/JU
Sample : 02592-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

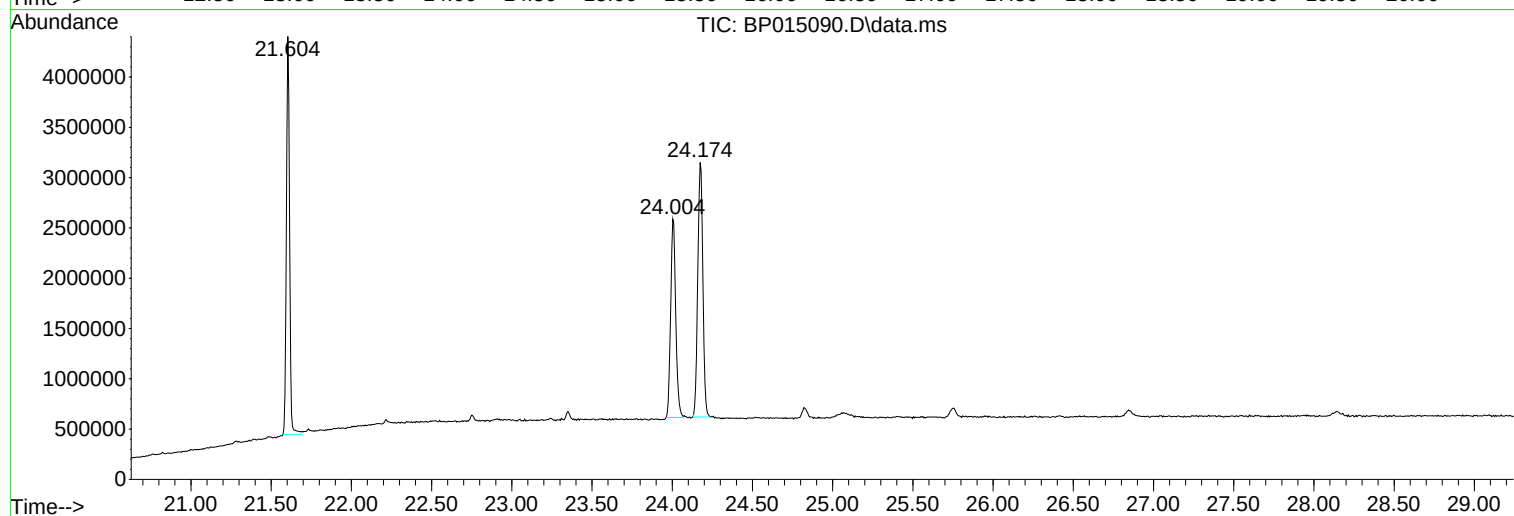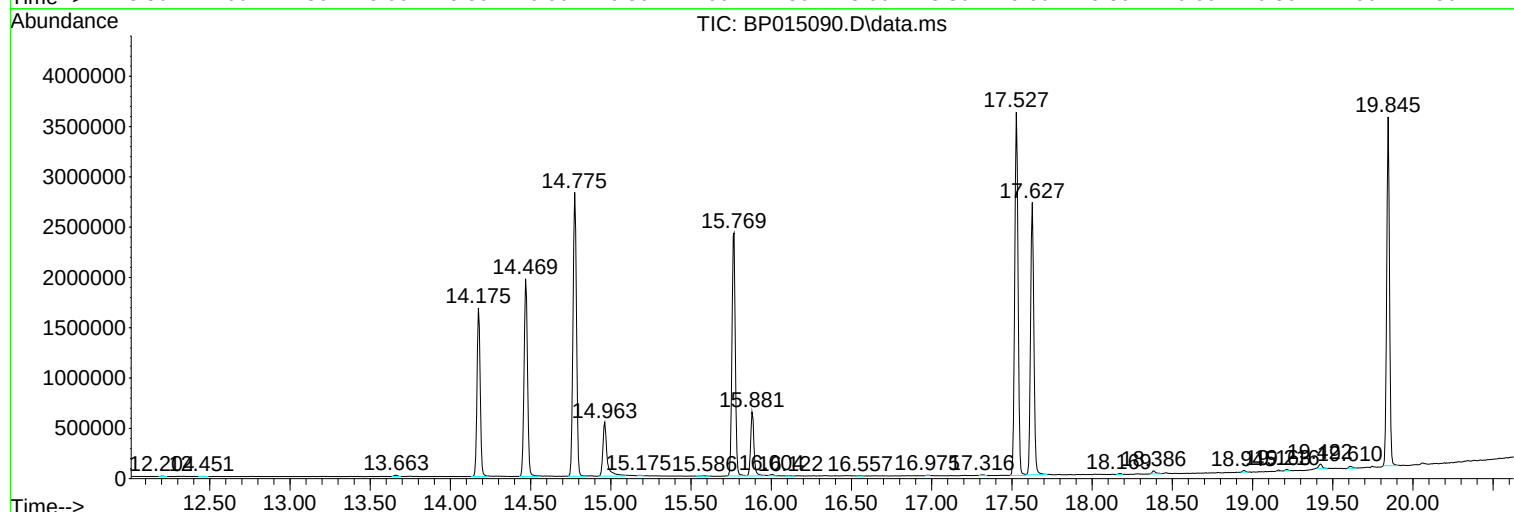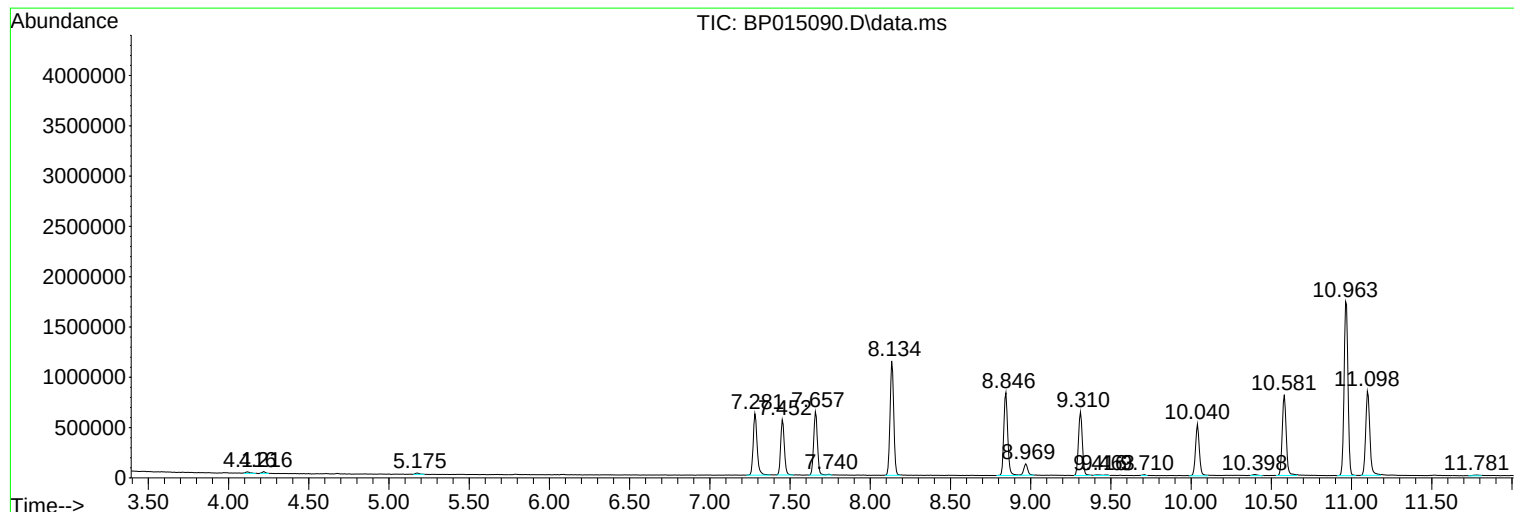

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015090.D
Acq On : 16 May 2023 00:10
Operator : CG/JU
Sample : 02592-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015090.D
Acq On : 16 May 2023 00:10
Operator : CG/JU
Sample : 02592-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------