

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015091.D
 Acq On : 16 May 2023 00:44
 Operator : CG/JU
 Sample : 02592-22
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	5	8	16	rVB	50552	71788	0.69%	0.068%
2	3.881	82	84	101	rBV	385818	609776	5.83%	0.577%
3	4.123	120	125	131	rVB2	22287	41183	0.39%	0.039%
4	4.217	138	141	148	rVB	18305	27989	0.27%	0.026%
5	4.611	205	208	212	rVB5	9047	12069	0.12%	0.011%
6	4.681	216	220	227	rVB	23838	38649	0.37%	0.037%
7	5.170	299	303	309	rBV	15015	21117	0.20%	0.020%
8	5.670	384	388	393	rVB3	6293	10618	0.10%	0.010%
9	5.793	404	409	413	rBV	15018	23339	0.22%	0.022%
10	7.240	650	655	656	rBV	18606	23159	0.22%	0.022%
11	7.281	656	662	676	rVB	1496007	2468179	23.59%	2.334%
12	7.452	684	691	704	rVB	1344822	2095479	20.03%	1.982%
13	7.658	719	726	736	rBV	1568867	2475655	23.66%	2.341%
14	7.740	738	740	744	rVB4	8247	10550	0.10%	0.010%
15	8.134	799	807	820	rBV	1282977	2020382	19.31%	1.911%
16	8.846	920	928	942	rBV	1974885	3269245	31.25%	3.092%
17	8.969	942	949	959	rVB	250577	410794	3.93%	0.388%
18	9.311	999	1007	1019	rBV	1590055	2579844	24.66%	2.440%
19	9.705	1068	1074	1081	rVB	59211	91236	0.87%	0.086%
20	10.040	1119	1131	1141	rBV	1303662	2170208	20.74%	2.052%
21	10.399	1187	1192	1199	rVB2	20096	36285	0.35%	0.034%
22	10.581	1215	1223	1237	rBV	1973192	3345047	31.97%	3.163%
23	10.963	1280	1288	1301	rVB	1910762	3218576	30.76%	3.044%
24	11.099	1301	1311	1333	rBV	1981249	3553748	33.96%	3.361%
25	11.510	1373	1381	1388	rBV	9181	24064	0.23%	0.023%
26	11.757	1417	1423	1436	rBV4	14201	42427	0.41%	0.040%
27	12.204	1493	1499	1504	rVB2	39943	60444	0.58%	0.057%
28	12.546	1549	1557	1563	rBV	21004	35598	0.34%	0.034%
29	13.657	1740	1746	1753	rBV2	17947	31936	0.31%	0.030%
30	13.751	1756	1762	1767	rVV5	6158	12075	0.12%	0.011%
31	14.175	1827	1834	1849	rBV	3790003	5468168	52.26%	5.171%
32	14.293	1849	1854	1859	rVV10	7819	15913	0.15%	0.015%
33	14.351	1859	1864	1868	rVB2	7551	10746	0.10%	0.010%
34	14.469	1876	1884	1902	rBV2	4545858	6762202	64.63%	6.395%
35	14.775	1929	1936	1946	rBV	3124647	4524811	43.25%	4.279%
36	14.869	1949	1952	1958	rVB8	8231	12108	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015091.D
 Acq On : 16 May 2023 00:44
 Operator : CG/JU
 Sample : 02592-22
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	14.963	1958	1968	1988	rBV	1674595	2670919	25.53%	2.526%
38	15.187	2000	2006	2012	rVB4	31384	56997	0.54%	0.054%
39	15.722	2092	2097	2098	rBV2	35221	37720	0.36%	0.036%
40	15.769	2098	2105	2118	rVV	5572826	8200334	78.37%	7.755%
41	15.881	2118	2124	2137	rVV	1928408	2651572	25.34%	2.507%
42	16.004	2141	2145	2151	rVB3	28036	44831	0.43%	0.042%
43	16.128	2160	2166	2180	rVB	512805	686900	6.57%	0.650%
44	16.340	2199	2202	2207	rVB7	7029	10981	0.10%	0.010%
45	16.463	2219	2223	2227	rBV7	7375	13628	0.13%	0.013%
46	16.692	2257	2262	2268	rBV	76591	105863	1.01%	0.100%
47	16.975	2305	2310	2317	rBV2	34174	49384	0.47%	0.047%
48	17.057	2320	2324	2330	rVB5	10630	14853	0.14%	0.014%
49	17.198	2344	2348	2353	rBV8	9604	16062	0.15%	0.015%
50	17.316	2363	2368	2372	rBV2	8812	14856	0.14%	0.014%
51	17.528	2397	2404	2413	rBV	3818787	5444672	52.04%	5.149%
52	17.628	2414	2421	2431	rVV2	6125896	8875845	84.83%	8.394%
53	17.710	2432	2435	2445	rVV4	42743	79886	0.76%	0.076%
54	17.816	2449	2453	2459	rVB6	19052	31607	0.30%	0.030%
55	18.045	2489	2492	2496	rVB2	29100	34583	0.33%	0.033%
56	18.175	2510	2514	2519	rBV7	8942	12256	0.12%	0.012%
57	18.381	2544	2549	2558	rBV	140815	211817	2.02%	0.200%
58	18.457	2559	2562	2564	rVV3	9168	10619	0.10%	0.010%
59	18.945	2641	2645	2650	rVB2	68849	85296	0.82%	0.081%
60	19.163	2678	2682	2687	rBV2	32367	46649	0.45%	0.044%
61	19.216	2687	2691	2693	rBV5	13056	16960	0.16%	0.016%
62	19.422	2722	2726	2732	rVB2	113988	166839	1.59%	0.158%
63	19.604	2754	2757	2761	rBV3	65080	83111	0.79%	0.079%
64	19.710	2772	2775	2779	rBV2	34844	39392	0.38%	0.037%
65	19.845	2792	2798	2810	rBV	7818066	10463016	100.00%	9.894%
66	21.280	3038	3042	3050	rBV	183164	297912	2.85%	0.282%
67	21.604	3092	3097	3107	rBV	4015258	5313785	50.79%	5.025%
68	24.010	3498	3506	3523	rVB2	4278342	9181769	87.75%	8.683%
69	24.174	3527	3534	3545	rVB	2406856	5150080	49.22%	4.870%




Sum of corrected areas: 105746401

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015091.D
Acq On : 16 May 2023 00:44
Operator : CG/JU
Sample : 02592-22
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

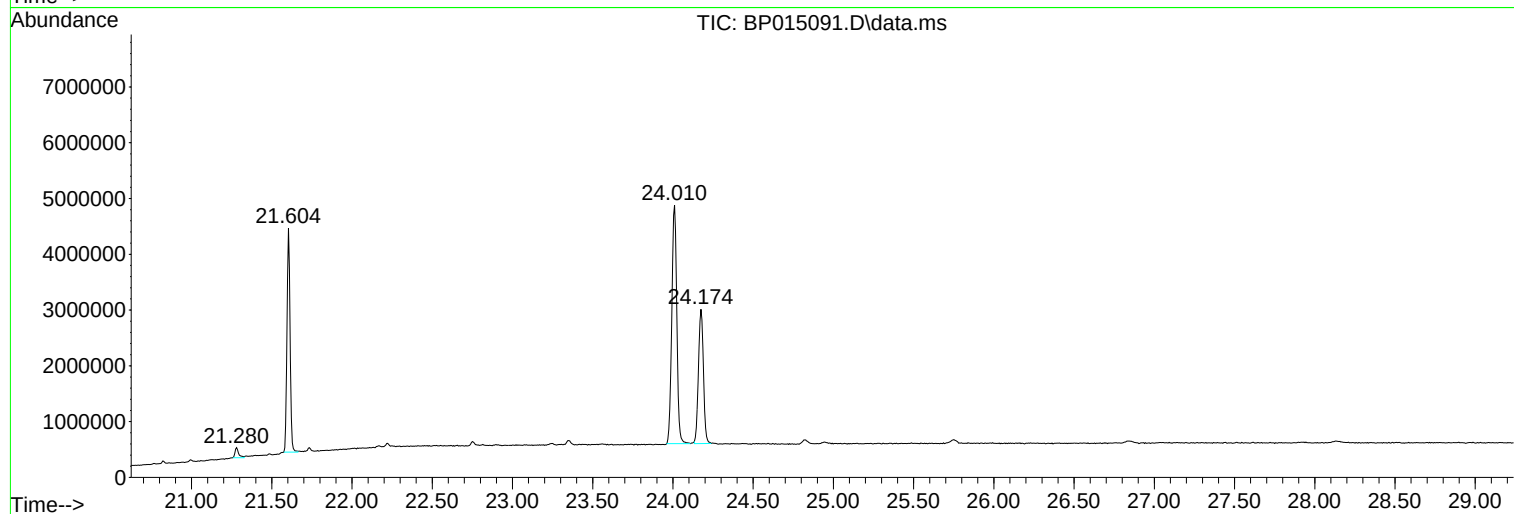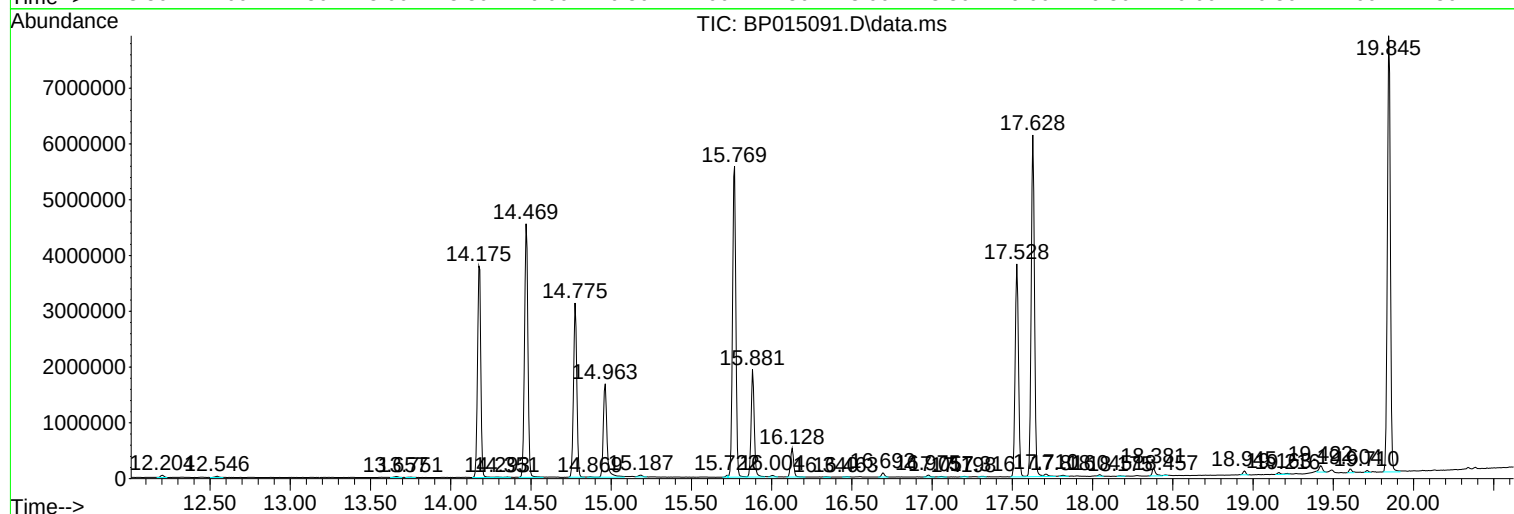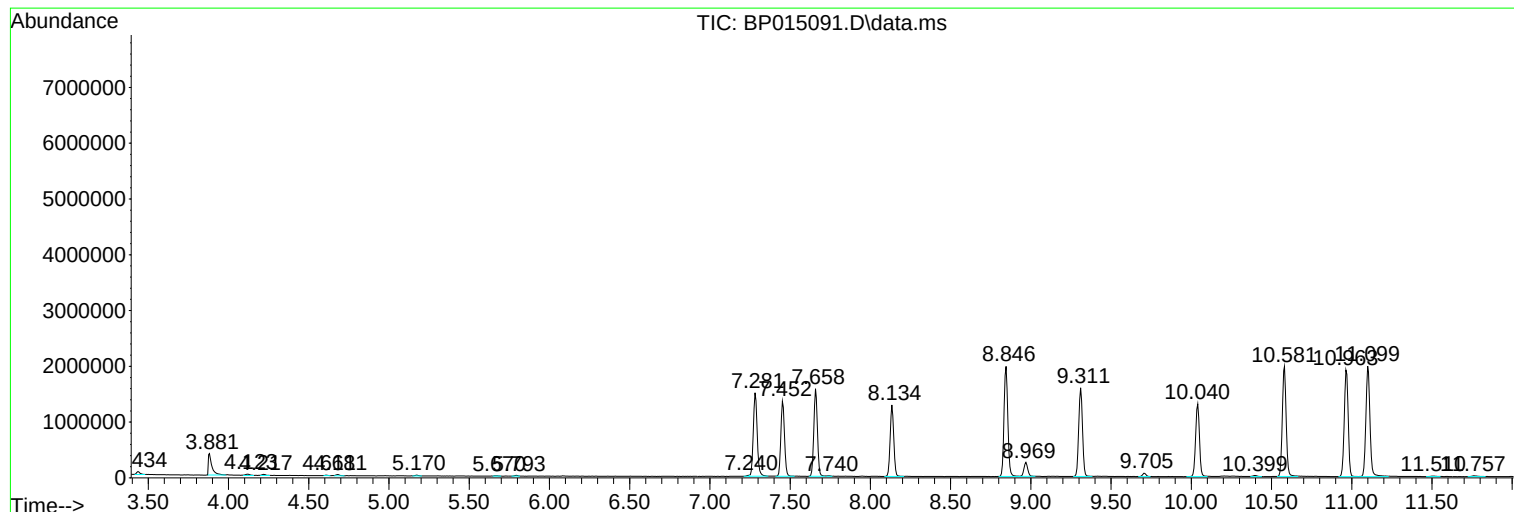

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015091.D
Acq On : 16 May 2023 00:44
Operator : CG/JU
Sample : 02592-22
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREE7










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.128	3.04 ng/ul	686900	Acenaphthene-d10	14.775

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	95
3			Benzophenone	182	C13H10O	000119-61-9	94
4			Benzophenone	182	C13H10O	000119-61-9	91
5			1,2,4,5-Tetroxane, 3,3,6,6-tetra...	396	C26H20O4	016204-36-7	64

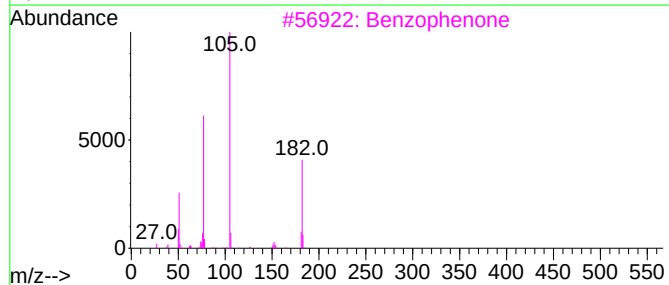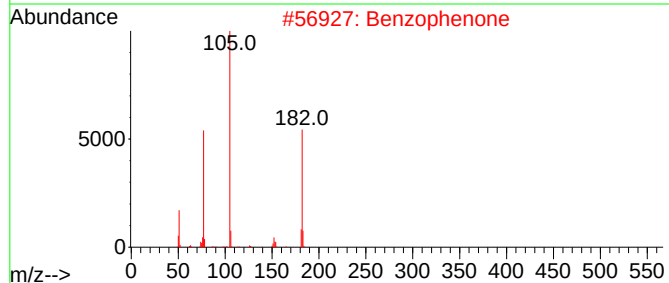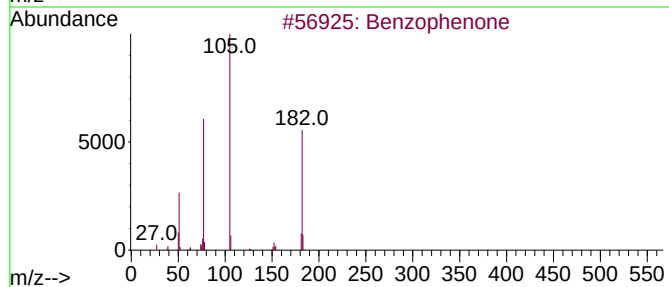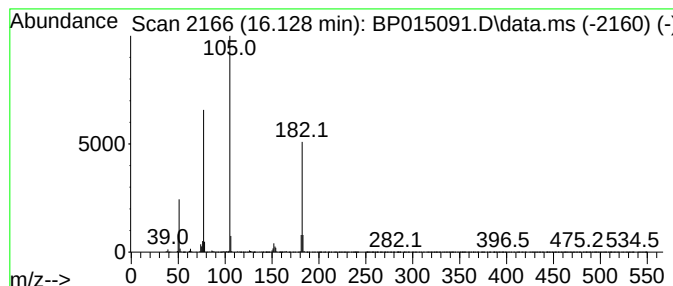

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015091.D
Acq On : 16 May 2023 00:44
Operator : CG/JU
Sample : 02592-22
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	16.128	3.0	ng/ul	686900	3	14.775	4524810	20.0