

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015093.D
 Acq On : 16 May 2023 01:51
 Operator : CG/JU
 Sample : 02592-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015093.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.117	121	124	132	rVB2	15561	26888	0.53%	0.048%
2	4.217	138	141	147	rVB	18665	27543	0.54%	0.049%
3	5.175	300	304	316	rVB4	15297	33047	0.65%	0.059%
4	7.281	652	662	676	rBV	628044	1064264	20.78%	1.900%
5	7.452	685	691	702	rVB	556472	873435	17.06%	1.559%
6	7.658	719	726	737	rBV	666333	1064275	20.78%	1.900%
7	7.740	737	740	747	rVB5	9368	15775	0.31%	0.028%
8	8.134	799	807	816	rBV	1179388	1868863	36.50%	3.336%
9	8.846	919	928	942	rBV	815710	1406969	27.48%	2.512%
10	8.969	943	949	958	rVB	136574	234494	4.58%	0.419%
11	9.310	1000	1007	1017	rBV	632039	1044666	20.40%	1.865%
12	9.704	1069	1074	1080	rVB5	9332	14119	0.28%	0.025%
13	10.040	1123	1131	1142	rBV	495054	849396	16.59%	1.516%
14	10.393	1184	1191	1199	rVB4	11728	24824	0.48%	0.044%
15	10.581	1215	1223	1237	rVV	811871	1407465	27.49%	2.512%
16	10.963	1281	1288	1297	rBV	1802875	2973335	58.07%	5.308%
17	11.099	1303	1311	1327	rBV	820114	1501385	29.32%	2.680%
18	11.510	1376	1381	1385	rBV7	5204	12049	0.24%	0.022%
19	11.775	1419	1426	1431	rBV6	7463	20233	0.40%	0.036%
20	12.198	1494	1498	1506	rBV6	6697	11619	0.23%	0.021%
21	13.657	1741	1746	1753	rBV	21697	33189	0.65%	0.059%
22	14.175	1826	1834	1848	rBV	1613905	2280992	44.55%	4.072%
23	14.469	1876	1884	1898	rBV	1934375	2815540	54.98%	5.026%
24	14.775	1928	1936	1947	rBV	2883421	4244107	82.88%	7.576%
25	14.963	1961	1968	1987	rBV	488900	931400	18.19%	1.663%
26	15.175	2003	2004	2009	rVB5	5527	7353	0.14%	0.013%
27	15.398	2034	2042	2045	rBV9	2379	5866	0.11%	0.010%
28	15.763	2098	2104	2118	rBV	2415329	3470528	67.78%	6.195%
29	15.881	2118	2124	2137	rVV	597831	848993	16.58%	1.516%
30	16.004	2141	2145	2153	rVB3	12342	23221	0.45%	0.041%
31	16.975	2305	2310	2314	rBV8	7158	13883	0.27%	0.025%
32	17.198	2344	2348	2351	rBV6	3214	5297	0.10%	0.009%
33	17.316	2364	2368	2373	rVB2	7570	10029	0.20%	0.018%
34	17.528	2397	2404	2414	rBV	3672371	5117429	99.94%	9.135%
35	17.628	2414	2421	2433	rVV	2531314	3659629	71.47%	6.533%
36	18.169	2510	2513	2519	rBV8	13277	20078	0.39%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
 Data File : BP015093.D
 Acq On : 16 May 2023 01:51
 Operator : CG/JU
 Sample : 02592-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JREG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	18.386	2546	2550	2554	rBV6	11601	19482	0.38%	0.035%
38	18.457	2559	2562	2565	rVB	12437	15313	0.30%	0.027%
39	18.945	2642	2645	2652	rVB2	22734	30794	0.60%	0.055%
40	19.163	2678	2682	2686	rBV4	19340	29725	0.58%	0.053%
41	19.422	2723	2726	2731	rVB4	40100	57823	1.13%	0.103%
42	19.845	2792	2798	2807	rBV	3217454	4225517	82.52%	7.543%
43	21.604	3092	3097	3109	rBV	3805528	5120586	100.00%	9.141%
44	24.004	3498	3505	3515	rBV2	1662676	3614906	70.60%	6.453%
45	24.174	3527	3534	3548	rVB	2313156	4942556	96.52%	8.823%




Sum of corrected areas: 56018880

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015093.D
Acq On : 16 May 2023 01:51
Operator : CG/JU
Sample : 02592-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

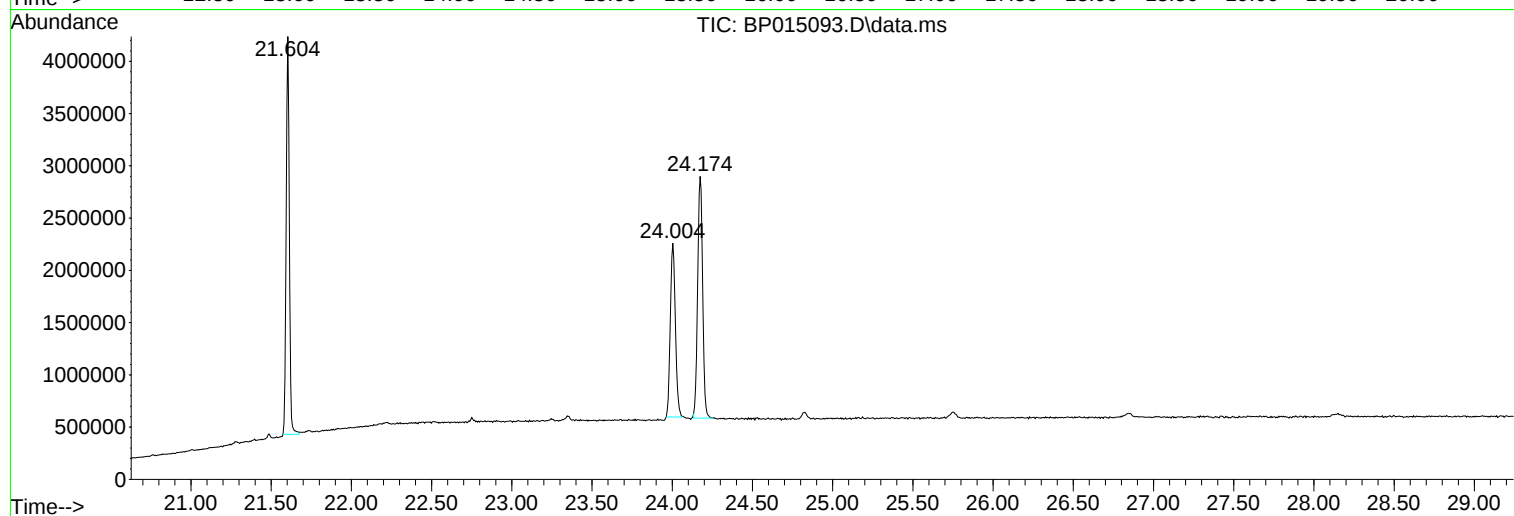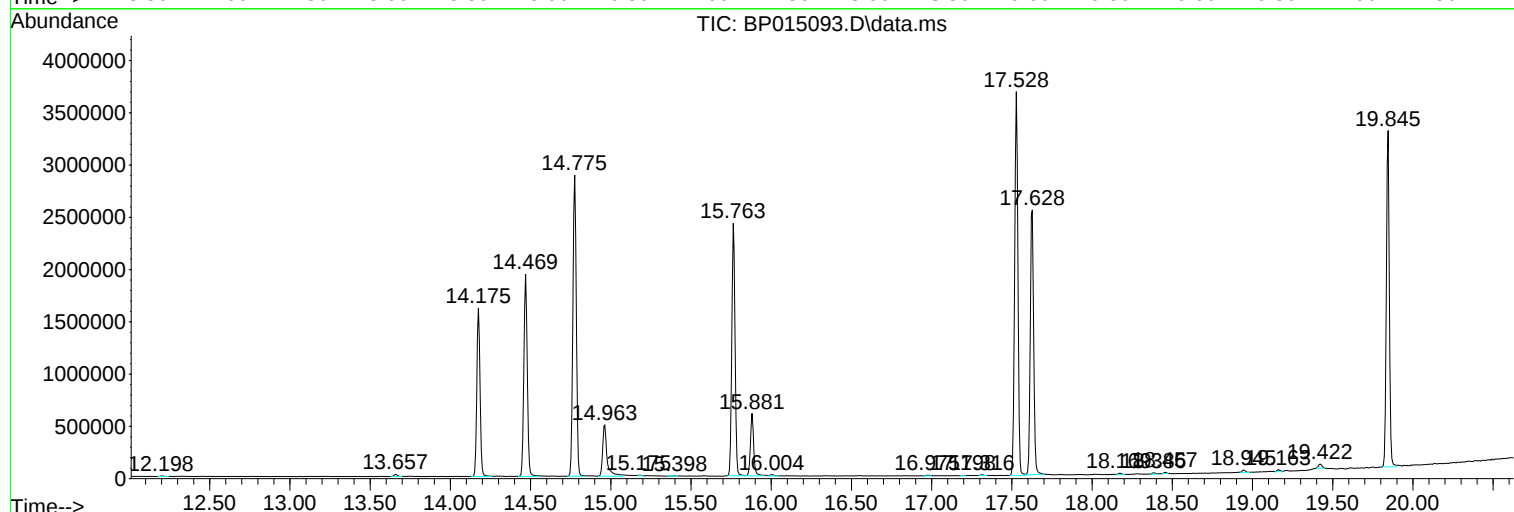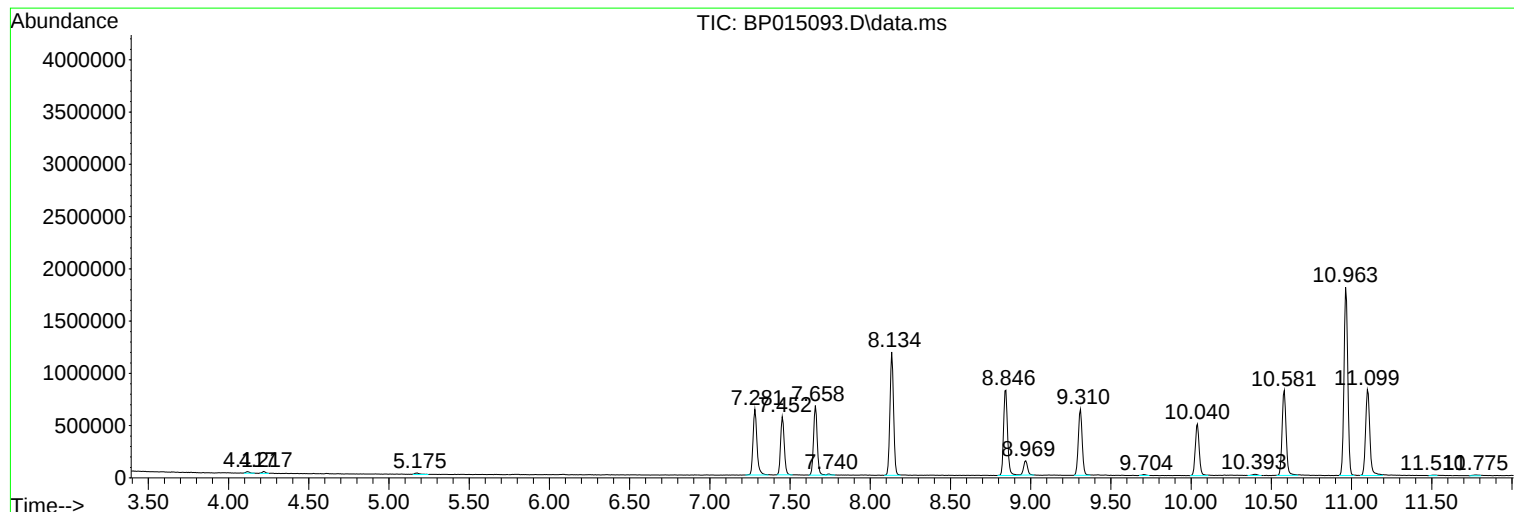

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015093.D
Acq On : 16 May 2023 01:51
Operator : CG/JU
Sample : 02592-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051523\
Data File : BP015093.D
Acq On : 16 May 2023 01:51
Operator : CG/JU
Sample : 02592-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JREG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc