
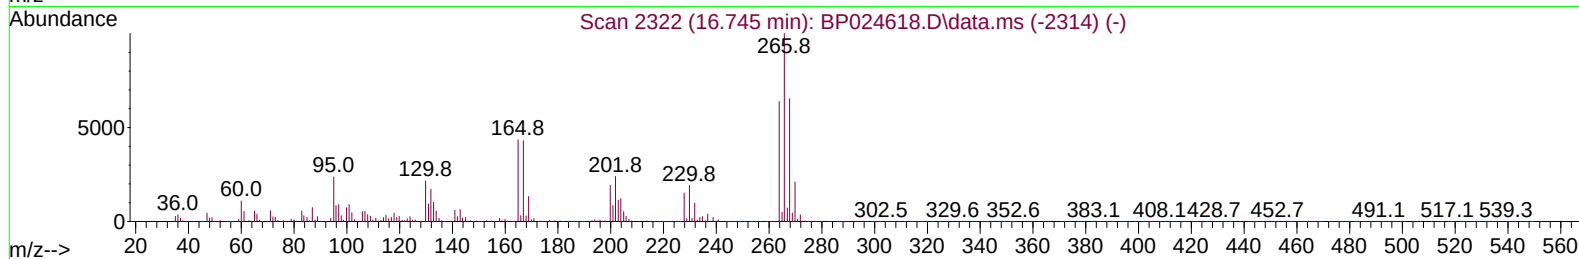
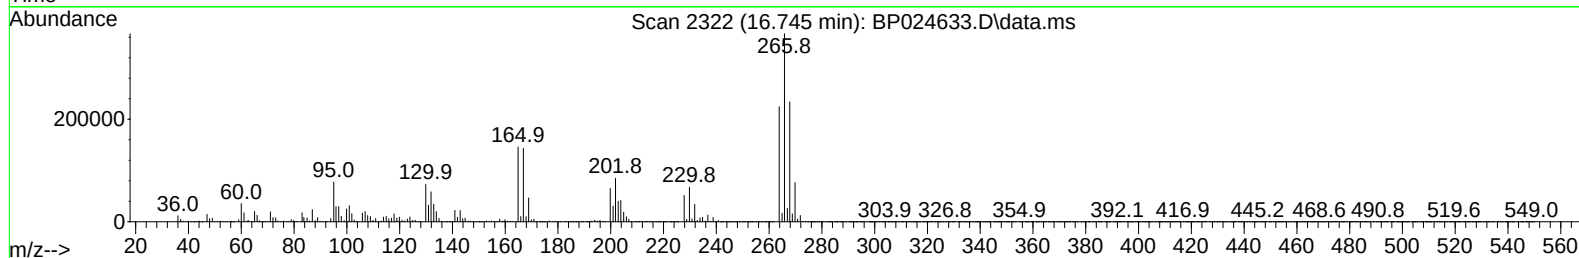


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024633.D
Acq On : 15 May 2025 11:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 13:40:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

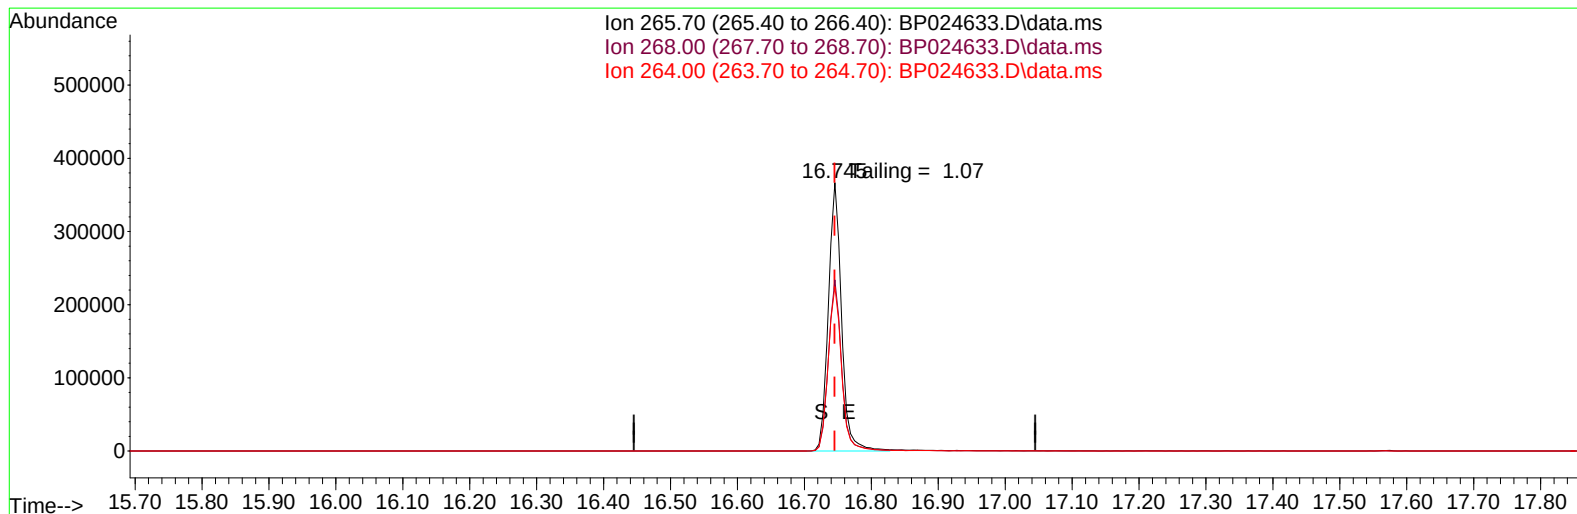

TIC: BP024633.D\data.ms

(70) Pentachlorophenol (C)




16.745min (+ 0.000) 9498.09 ng

response 503182

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.72
264.00	63.90	61.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024633.D
Acq On : 15 May 2025 11:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 13:40:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 13 16:21:39 2025
Response via : Initial Calibration

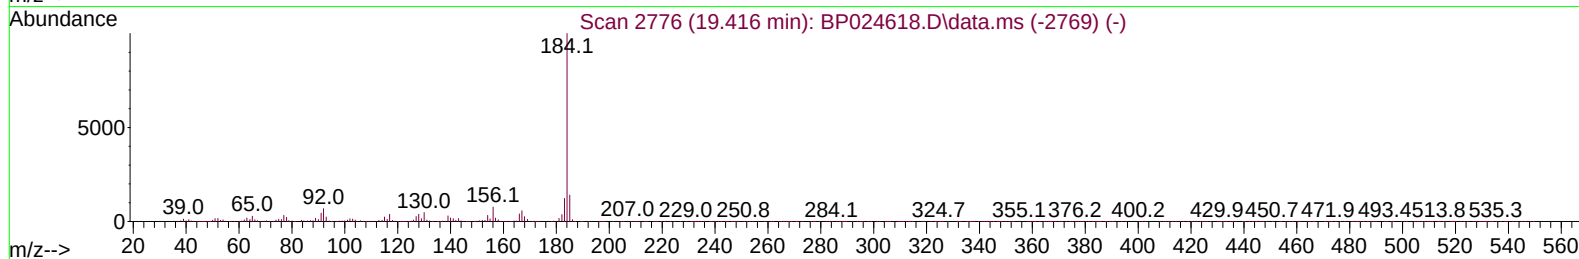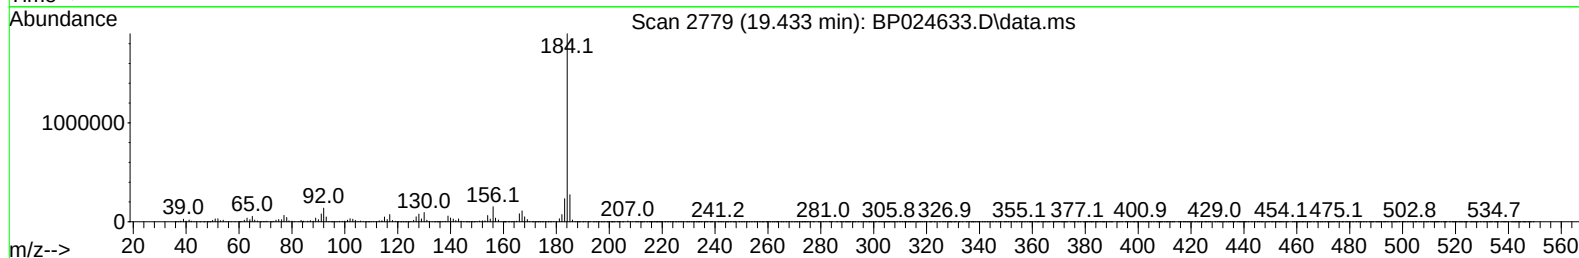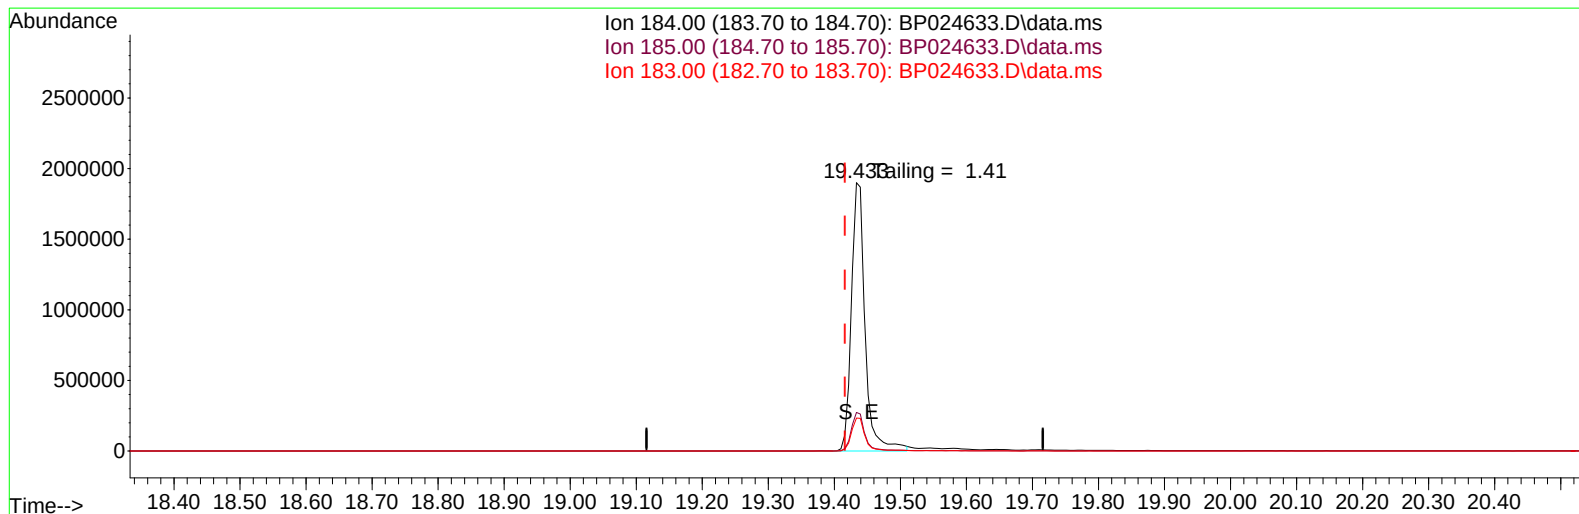

TIC: BP024633.D\data.ms

(77) Benzidine**19.433min (+ 0.017) 2596.29 ng****response 2759335**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.40
183.00	12.30	12.29
0.00	0.00	0.00