

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
 Data File : BP024640.D
 Acq On : 15 May 2025 16:40
 Operator : RC/JU
 Sample : Q1984-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-PCS-TC-33-050725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024640.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.823	290	295	311	rVB	203003	286738	3.14%	0.698%
2	5.281	367	373	392	rBV	2138212	3148256	34.53%	7.663%
3	6.852	631	640	654	rBV	2093908	3300440	36.20%	8.034%
4	7.658	769	777	788	rBV	545139	885414	9.71%	2.155%
5	8.811	965	973	993	rBV	1159029	1970270	21.61%	4.796%
6	10.428	1240	1248	1262	rBV	762629	1327698	14.56%	3.232%
7	12.904	1661	1669	1682	rBV	3331284	5101441	55.95%	12.417%
8	14.293	1897	1905	1912	rBV	1197516	1717656	18.84%	4.181%
9	15.675	2133	2140	2148	rBV	254587	368889	4.05%	0.898%
10	15.810	2155	2163	2184	rBV	2912352	4577072	50.20%	11.141%
11	17.087	2373	2380	2387	rBV2	1394999	2063860	22.63%	5.024%
12	17.498	2445	2450	2465	rBV2	53334	129289	1.42%	0.315%
13	18.028	2534	2540	2548	rBV	540391	838363	9.19%	2.041%
14	18.469	2610	2615	2620	rBV	125064	157993	1.73%	0.385%
15	19.357	2762	2766	2780	rBV	137798	265644	2.91%	0.647%
16	19.810	2837	2843	2858	rBV	7197904	9118230	100.00%	22.194%
17	21.192	3073	3078	3090	rBV	311435	677127	7.43%	1.648%
18	21.522	3128	3134	3140	rBV	1586652	2556432	28.04%	6.223%
19	24.804	3683	3692	3705	rBV2	837080	2592477	28.43%	6.310%




Sum of corrected areas: 41083289

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024640.D
Acq On : 15 May 2025 16:40
Operator : RC/JU
Sample : Q1984-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-33-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

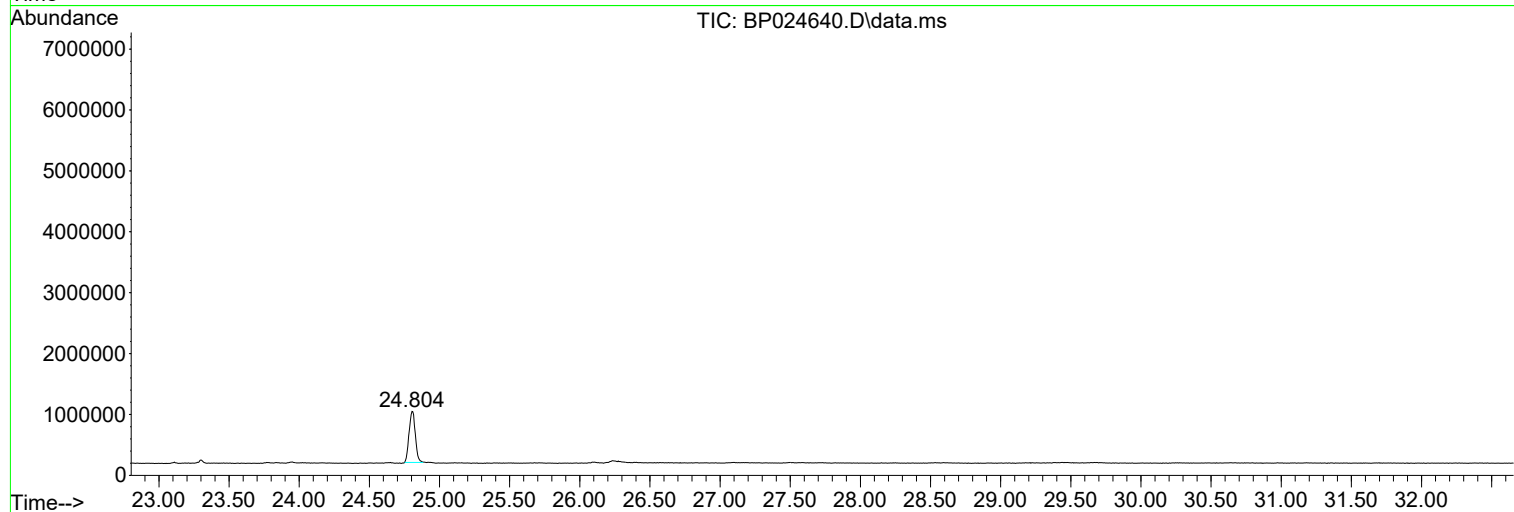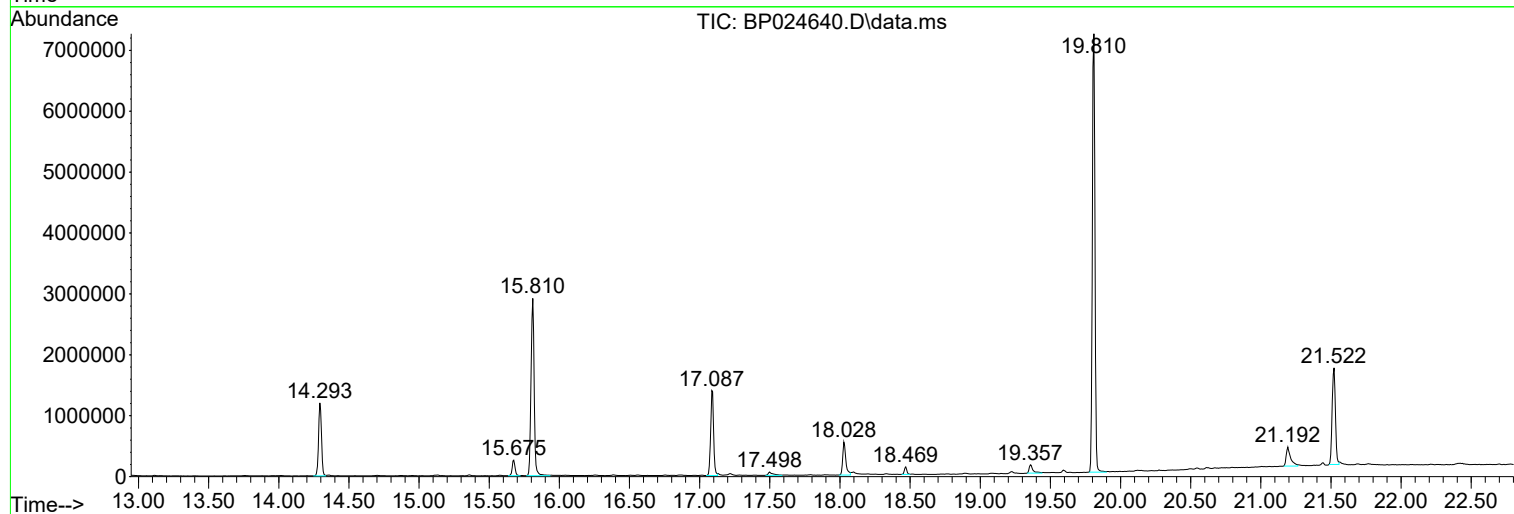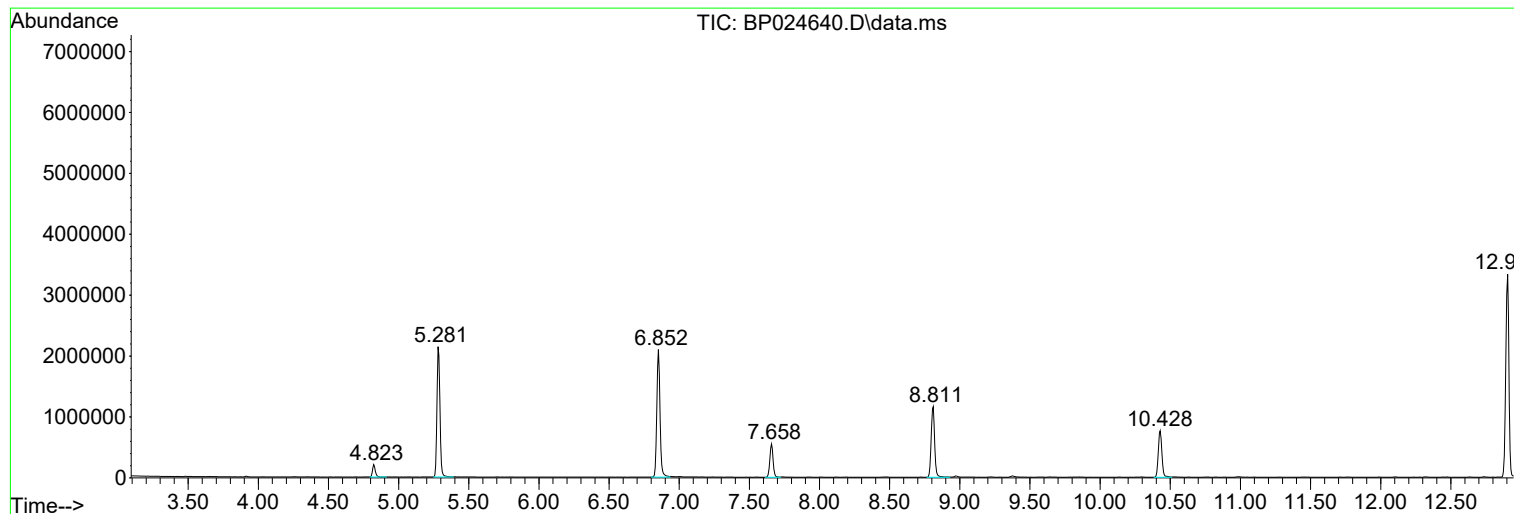

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024640.D
Acq On : 15 May 2025 16:40
Operator : RC/JU
Sample : Q1984-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-33-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024640.D
Acq On : 15 May 2025 16:40
Operator : RC/JU
Sample : Q1984-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-33-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc