

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
 Data File : BP024643.D
 Acq On : 15 May 2025 18:42
 Operator : RC/JU
 Sample : Q1984-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-TS-25-050725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.828	290	296	307	rBV	140015	212081	2.86%	0.436%
2	5.287	367	374	391	rBV	1599057	2418927	32.64%	4.977%
3	6.852	632	640	662	rBV	1719949	2810190	37.91%	5.782%
4	7.657	767	777	788	rBV	585371	975436	13.16%	2.007%
5	8.810	964	973	993	rBV	1075775	1835283	24.76%	3.776%
6	10.428	1241	1248	1262	rBV	839068	1477569	19.94%	3.040%
7	12.898	1661	1668	1686	rBV	2930289	4387367	59.19%	9.026%
8	13.475	1760	1766	1772	rBV2	73438	113616	1.53%	0.234%
9	14.292	1897	1905	1912	rBV	1306750	1983154	26.76%	4.080%
10	15.675	2134	2140	2147	rBV	242522	341028	4.60%	0.702%
11	15.804	2156	2162	2178	rBV	2794121	4176068	56.34%	8.592%
12	17.092	2374	2381	2386	rBV2	1713497	2416040	32.60%	4.971%
13	17.133	2386	2388	2393	rVB	71046	90612	1.22%	0.186%
14	17.957	2525	2528	2533	rBV	60631	78264	1.06%	0.161%
15	18.033	2535	2541	2563	rVV	1053553	1614590	21.78%	3.322%
16	18.333	2588	2592	2596	rBV2	204838	270280	3.65%	0.556%
17	19.110	2718	2724	2735	rVB5	81720	185738	2.51%	0.382%
18	19.221	2737	2743	2748	rBV	196271	383129	5.17%	0.788%
19	19.363	2763	2767	2775	rBV2	215748	336035	4.53%	0.691%
20	19.598	2803	2807	2811	rVB	145273	177304	2.39%	0.365%
21	19.816	2839	2844	2856	rVB	6242657	7411915	100.00%	15.249%
22	20.039	2879	2882	2885	rBV	71601	80715	1.09%	0.166%
23	20.492	2955	2959	2963	rVB2	380312	456124	6.15%	0.938%
24	20.663	2984	2988	2995	rBV	130447	233896	3.16%	0.481%
25	21.198	3075	3079	3093	rVB	465487	846736	11.42%	1.742%
26	21.527	3128	3135	3140	rBV	1808454	2944833	39.73%	6.059%
27	22.404	3279	3284	3287	rBV	293551	484313	6.53%	0.996%
28	23.962	3541	3549	3558	rBV	911375	2044438	27.58%	4.206%
29	24.815	3686	3694	3703	rBV	1156796	2581440	34.83%	5.311%
30	26.115	3906	3915	3923	rBV	601212	1761371	23.76%	3.624%
31	30.286	4615	4624	4626	rBV2	497437	1234006	16.65%	2.539%
32	30.768	4699	4706	4723	rVB3	411337	1761864	23.77%	3.625%
33	32.386	4975	4981	4982	rBV5	263005	481278	6.49%	0.990%




Sum of corrected areas: 48605640

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024643.D
Acq On : 15 May 2025 18:42
Operator : RC/JU
Sample : Q1984-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-25-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

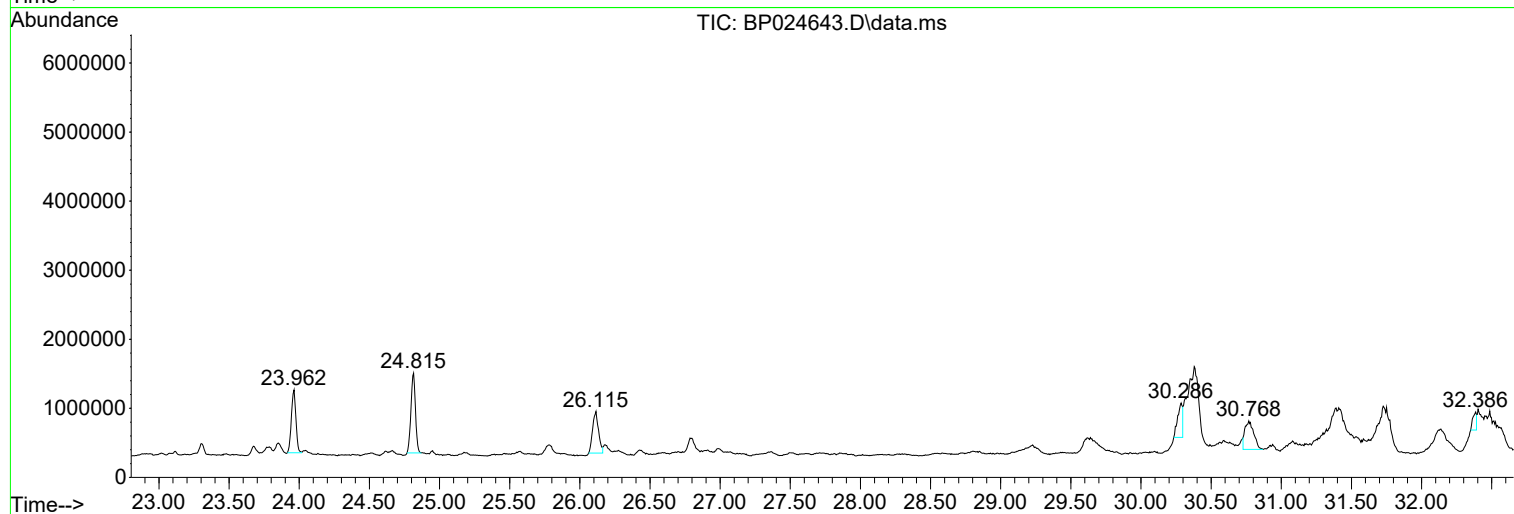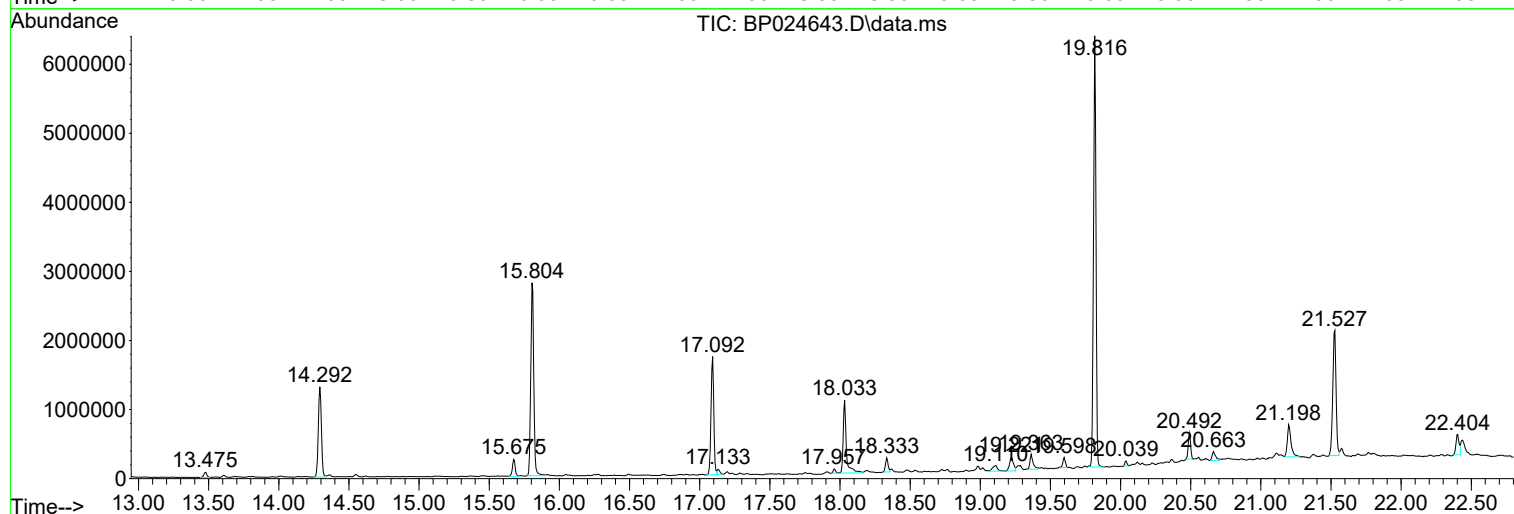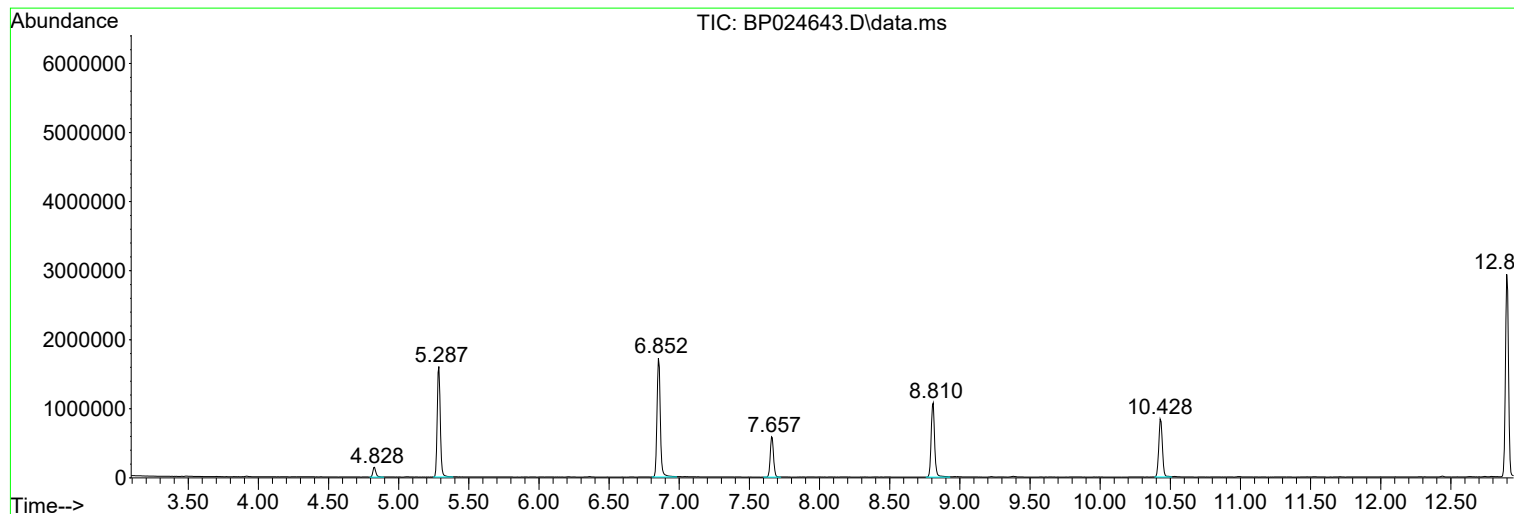

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024643.D
Acq On : 15 May 2025 18:42
Operator : RC/JU
Sample : Q1984-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-25-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024643.D
Acq On : 15 May 2025 18:42
Operator : RC/JU
Sample : Q1984-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-25-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------