

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
 Data File : BP024644.D
 Acq On : 15 May 2025 19:23
 Operator : RC/JU
 Sample : Q1984-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-TS-26-050725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.828	290	296	306	rBV	189012	266011	4.55%	0.552%
2	5.287	367	374	392	rBV	1990556	2882360	49.34%	5.979%
3	6.852	631	640	659	rBV	1801336	2990938	51.20%	6.204%
4	7.658	770	777	787	rBV	628597	1019032	17.44%	2.114%
5	8.805	965	972	988	rBV	1075080	1955357	33.47%	4.056%
6	10.428	1240	1248	1263	rBV	878688	1489416	25.50%	3.090%
7	12.899	1660	1668	1683	rBV	3068446	4368214	74.78%	9.061%
8	13.475	1759	1766	1774	rBV	96983	147615	2.53%	0.306%
9	14.293	1897	1905	1912	rBV	1253729	1886994	32.30%	3.914%
10	14.551	1944	1949	1955	rVB4	39391	61644	1.06%	0.128%
11	15.681	2135	2141	2152	rBV	233074	331186	5.67%	0.687%
12	15.804	2156	2162	2175	rBV	2611675	3686682	63.11%	7.647%
13	16.275	2235	2242	2250	rVB8	32464	70966	1.21%	0.147%
14	17.087	2374	2380	2386	rBV2	1387869	2097485	35.91%	4.351%
15	17.140	2386	2389	2394	rVB2	51417	63928	1.09%	0.133%
16	17.192	2394	2398	2402	rBV2	39299	60770	1.04%	0.126%
17	17.957	2525	2528	2532	rVB2	63277	72386	1.24%	0.150%
18	18.034	2532	2541	2556	rBV	1095273	1834572	31.41%	3.806%
19	18.334	2587	2592	2596	rBV2	227009	318732	5.46%	0.661%
20	18.475	2612	2616	2622	rBV4	46949	92886	1.59%	0.193%
21	18.981	2700	2702	2705	rBV4	49347	60901	1.04%	0.126%
22	19.110	2718	2724	2730	rVB5	84764	199341	3.41%	0.414%
23	19.216	2737	2742	2748	rBV	190664	417860	7.15%	0.867%
24	19.263	2748	2750	2758	rVB5	82353	180434	3.09%	0.374%
25	19.357	2763	2766	2777	rVB2	220253	399273	6.84%	0.828%
26	19.592	2803	2806	2810	rVB	109346	139438	2.39%	0.289%
27	19.816	2838	2844	2850	rBV	4876334	5841428	100.00%	12.117%
28	20.033	2875	2881	2885	rBV2	322738	584427	10.00%	1.212%
29	20.063	2885	2886	2890	rVB2	98185	59734	1.02%	0.124%
30	20.298	2921	2926	2933	rBV4	173371	415182	7.11%	0.861%
31	20.486	2954	2958	2963	rBV2	407897	520277	8.91%	1.079%
32	20.651	2983	2986	2994	rVB	143046	208840	3.58%	0.433%
33	21.192	3074	3078	3086	rBV	407989	632168	10.82%	1.311%
34	21.516	3127	3133	3139	rBV2	1489056	2578383	44.14%	5.348%
35	22.386	3277	3281	3284	rBV	269459	386012	6.61%	0.801%
36	23.939	3539	3545	3553	rBV	1078339	2044623	35.00%	4.241%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024644.D
Acq On : 15 May 2025 19:23
Operator : RC/JU
Sample : Q1984-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-26-050725

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	24.792	3682	3690	3700	rBV	1100389	2740551	46.92%	5.685%
38	25.751	3851	3853	3866	rVB2	233817	611209	10.46%	1.268%
39	26.086	3904	3910	3920	rBV	631930	1494764	25.59%	3.101%
40	30.262	4612	4620	4621	rBV	669402	1322182	22.63%	2.743%
41	30.280	4621	4623	4625	rVV2	242417	279350	4.78%	0.579%
42	31.709	4864	4866	4867	rBV	283863	183577	3.14%	0.381%
43	32.374	4970	4979	4981	rBV4	457803	1210868	20.73%	2.512%




Sum of corrected areas: 48207996

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024644.D
Acq On : 15 May 2025 19:23
Operator : RC/JU
Sample : Q1984-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-26-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

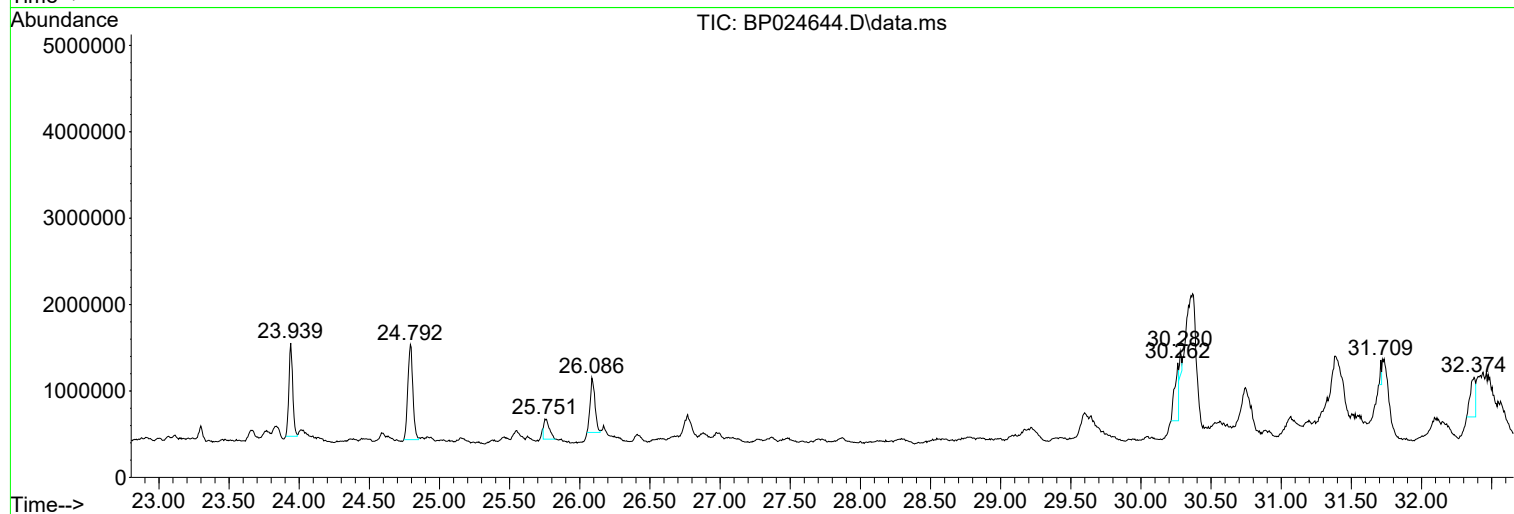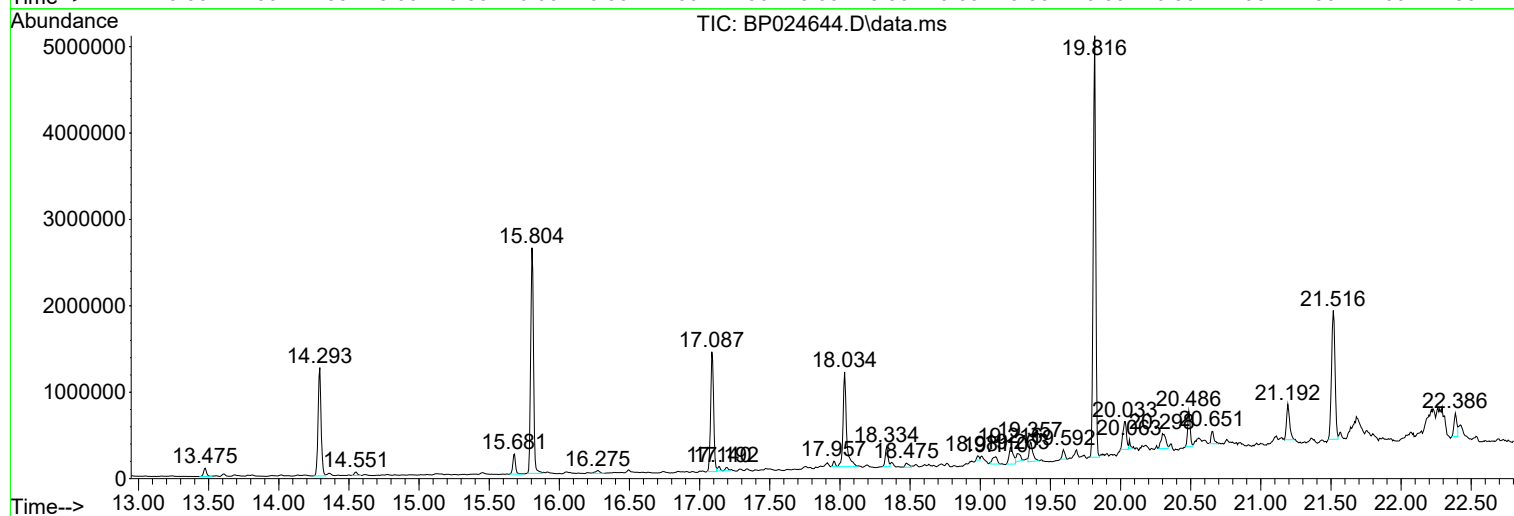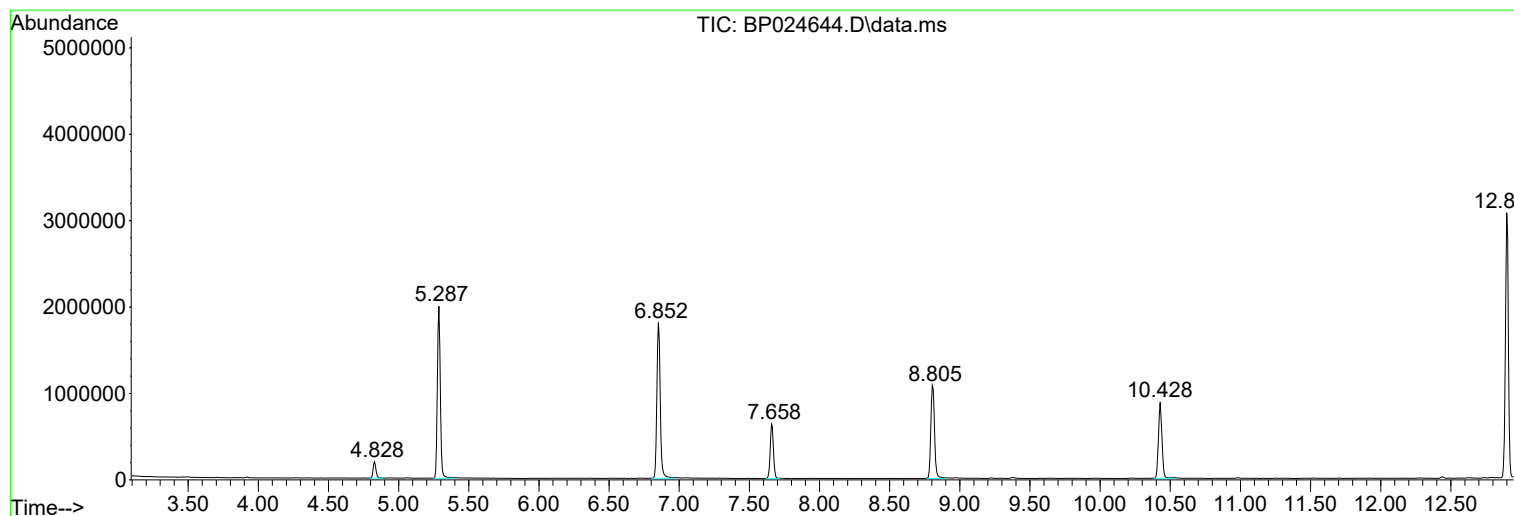

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024644.D
Acq On : 15 May 2025 19:23
Operator : RC/JU
Sample : Q1984-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-26-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024644.D
Acq On : 15 May 2025 19:23
Operator : RC/JU
Sample : Q1984-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-26-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------