

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
 Data File : BP024646.D
 Acq On : 15 May 2025 20:45
 Operator : RC/JU
 Sample : Q1984-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-TS-28-050725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024646.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.828	290	296	305	rBV	243743	339898	5.65%	0.501%
2	5.287	367	374	394	rBV	2897987	4152704	69.05%	6.119%
3	6.858	630	641	656	rBV	2453972	3985694	66.28%	5.873%
4	7.658	770	777	786	rBV	885549	1367677	22.74%	2.015%
5	8.810	965	973	990	rBV	1750202	2921806	48.59%	4.305%
6	10.428	1241	1248	1262	rBV	1156157	1962380	32.63%	2.891%
7	12.904	1660	1669	1679	rBV	3826558	6013713	100.00%	8.861%
8	13.469	1759	1765	1773	rBV2	146893	227674	3.79%	0.335%
9	13.610	1783	1789	1797	rBV2	54531	98759	1.64%	0.146%
10	14.293	1898	1905	1913	rBV	1744562	2609818	43.40%	3.845%
11	14.363	1913	1917	1923	rVB3	46002	80968	1.35%	0.119%
12	14.551	1944	1949	1957	rBV4	62985	110751	1.84%	0.163%
13	15.445	2097	2101	2111	rVB4	30770	76023	1.26%	0.112%
14	15.675	2135	2140	2147	rBV	289338	423438	7.04%	0.624%
15	15.810	2156	2163	2176	rBV	3735769	5275712	87.73%	7.773%
16	16.228	2230	2234	2238	rVV2	44025	79476	1.32%	0.117%
17	16.281	2240	2243	2248	rVB2	81342	122682	2.04%	0.181%
18	16.492	2275	2279	2286	rBV4	56853	99243	1.65%	0.146%
19	17.092	2374	2381	2386	rBV2	1693690	2566732	42.68%	3.782%
20	17.139	2386	2389	2394	rVB2	69384	95723	1.59%	0.141%
21	17.192	2395	2398	2402	rBV2	78425	97814	1.63%	0.144%
22	17.963	2525	2529	2533	rBV3	72573	103812	1.73%	0.153%
23	18.034	2533	2541	2560	rVB	1676157	2820526	46.90%	4.156%
24	18.333	2588	2592	2596	rBV2	298138	372024	6.19%	0.548%
25	18.369	2596	2598	2606	rVB7	68992	108371	1.80%	0.160%
26	18.933	2686	2694	2698	rBV7	102649	302951	5.04%	0.446%
27	19.016	2704	2708	2717	rVB6	214357	421460	7.01%	0.621%
28	19.216	2739	2742	2748	rBV	198581	424601	7.06%	0.626%
29	19.269	2748	2751	2756	rVB4	172308	288085	4.79%	0.424%
30	19.357	2763	2766	2774	rVB2	314848	511998	8.51%	0.754%
31	19.598	2804	2807	2810	rBV	119833	135498	2.25%	0.200%
32	19.816	2838	2844	2849	rBV	5010649	5690547	94.63%	8.385%
33	20.016	2876	2878	2884	rVB3	265917	368808	6.13%	0.543%
34	20.163	2900	2903	2904	rBV2	152041	162048	2.69%	0.239%
35	20.492	2955	2959	2963	rVB2	379369	519962	8.65%	0.766%
36	20.657	2984	2987	2992	rBV	238001	356170	5.92%	0.525%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024646.D
Acq On : 15 May 2025 20:45
Operator : RC/JU
Sample : Q1984-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-28-050725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.198	3075	3079	3088	rVB	520840	871245	14.49%	1.284%
38	21.527	3129	3135	3140	rBV	1458011	2328675	38.72%	3.431%
39	22.304	3260	3267	3279	rVB2	1356117	3964135	65.92%	5.841%
40	22.398	3280	3283	3287	rBV	212654	387151	6.44%	0.570%
41	23.968	3542	3550	3555	rBV2	958726	2230062	37.08%	3.286%
42	24.810	3686	3693	3703	rVB	1053569	2622361	43.61%	3.864%
43	26.104	3905	3913	3921	rVB	637206	1728986	28.75%	2.548%
44	30.274	4613	4622	4623	rBV	968785	1979663	32.92%	2.917%
45	31.750	4867	4873	4894	rVB4	1087963	5128267	85.28%	7.556%
46	32.386	4972	4981	4982	rBV	657540	1332259	22.15%	1.963%




Sum of corrected areas: 67868350

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024646.D
Acq On : 15 May 2025 20:45
Operator : RC/JU
Sample : Q1984-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-28-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

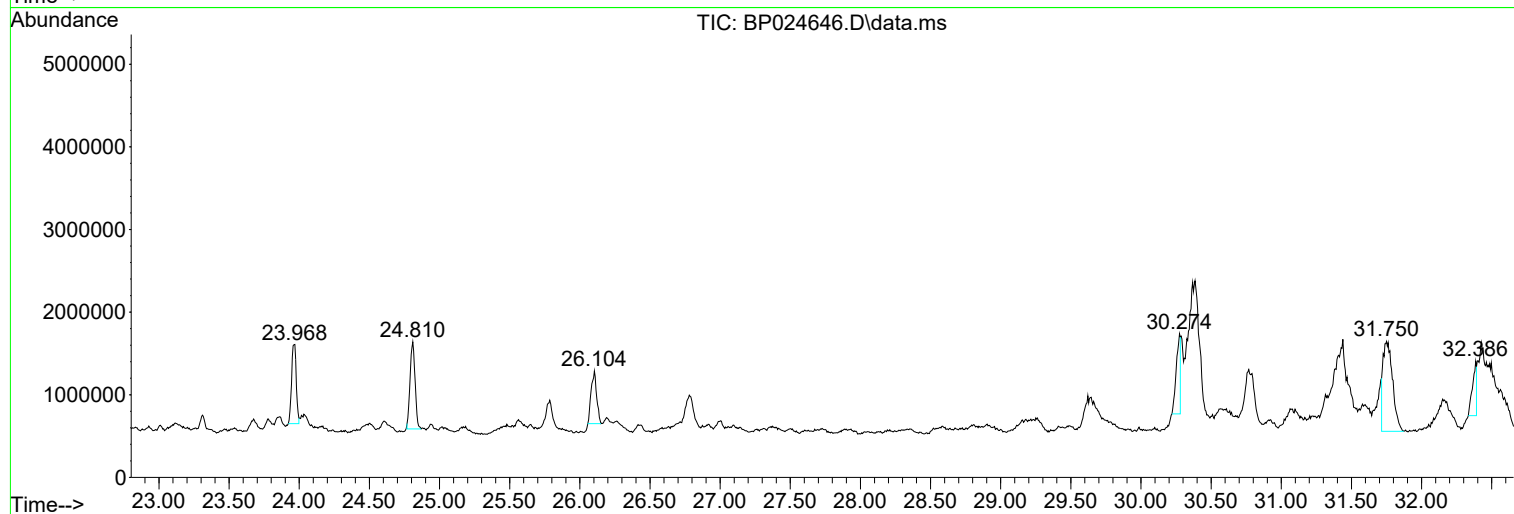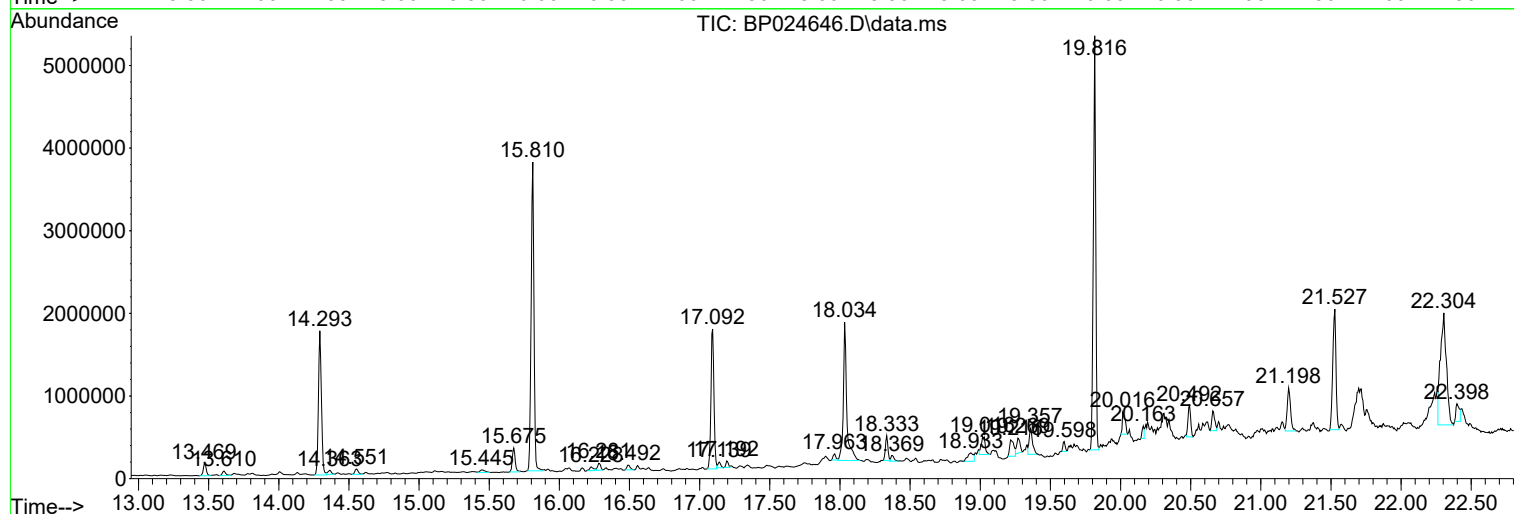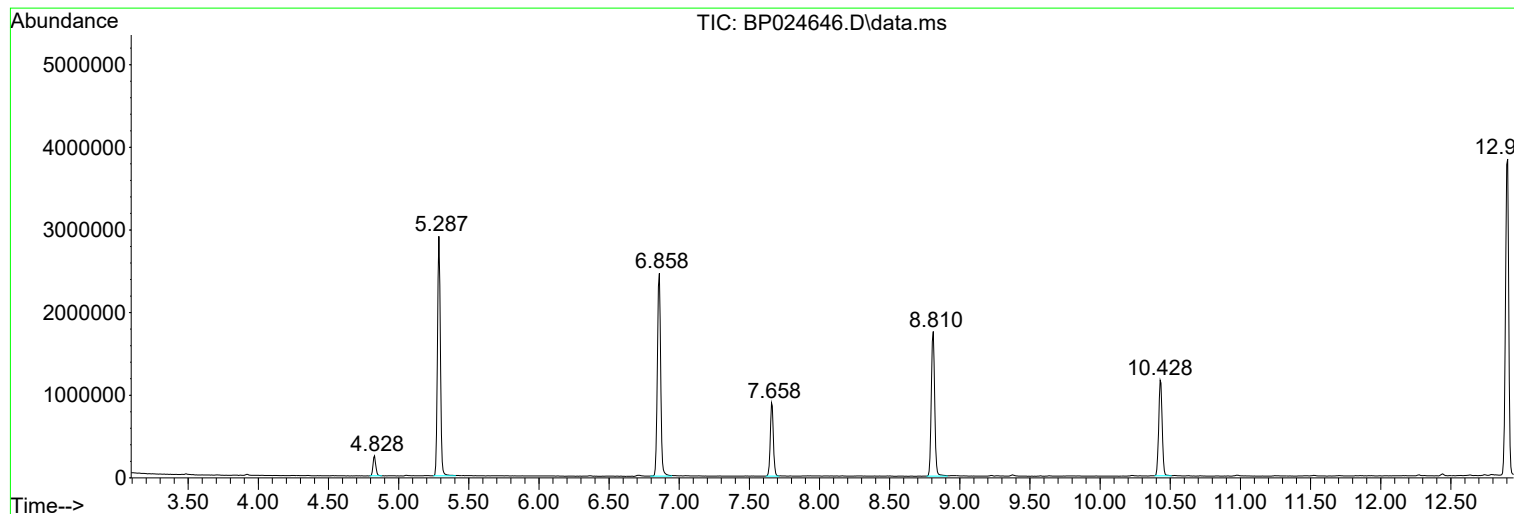

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024646.D
Acq On : 15 May 2025 20:45
Operator : RC/JU
Sample : Q1984-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-28-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024646.D
Acq On : 15 May 2025 20:45
Operator : RC/JU
Sample : Q1984-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-28-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------