

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
 Data File : BP024648.D
 Acq On : 15 May 2025 22:06
 Operator : RC/JU
 Sample : Q1984-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-TS-24-050725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.828	291	296	309	rVB	207693	297041	4.32%	0.622%
2	5.287	368	374	393	rBV	2139567	3129470	45.53%	6.548%
3	6.858	634	641	661	rBV	1919423	3003385	43.70%	6.284%
4	7.658	771	777	787	rBV	757293	1205341	17.54%	2.522%
5	8.810	965	973	985	rBV	1299146	2128082	30.96%	4.453%
6	10.428	1241	1248	1261	rBV	905314	1581179	23.01%	3.308%
7	12.904	1660	1669	1679	rBV	3264136	4811433	70.01%	10.067%
8	13.475	1759	1766	1773	rBV2	91082	140802	2.05%	0.295%
9	14.292	1896	1905	1912	rBV	1340734	1967400	28.63%	4.117%
10	15.675	2134	2140	2152	rBV	254733	369312	5.37%	0.773%
11	15.804	2156	2162	2174	rBV	3072721	4009131	58.33%	8.389%
12	16.269	2234	2241	2247	rVB6	38915	82631	1.20%	0.173%
13	17.086	2374	2380	2385	rBV2	1549782	2136793	31.09%	4.471%
14	17.957	2524	2528	2532	rBV2	61383	81502	1.19%	0.171%
15	18.028	2535	2540	2557	rBV	997861	1587922	23.10%	3.323%
16	18.328	2587	2591	2595	rBV	206176	279849	4.07%	0.586%
17	19.092	2716	2721	2722	rBV3	61598	100499	1.46%	0.210%
18	19.222	2737	2743	2747	rBV	172936	342974	4.99%	0.718%
19	19.357	2762	2766	2775	rBV2	193708	314002	4.57%	0.657%
20	19.592	2803	2806	2809	rVB	106246	118456	1.72%	0.248%
21	19.810	2838	2843	2850	rBV	5839891	6872740	100.00%	14.381%
22	20.027	2878	2880	2884	rVB	64550	71564	1.04%	0.150%
23	20.486	2954	2958	2962	rBV3	347710	456411	6.64%	0.955%
24	20.651	2983	2986	2992	rBV	176264	249797	3.63%	0.523%
25	21.192	3073	3078	3092	rVB	491762	869691	12.65%	1.820%
26	21.516	3127	3133	3139	rBV	1748084	2687042	39.10%	5.622%
27	22.392	3277	3282	3298	rVB2	280078	887772	12.92%	1.858%
28	23.945	3540	3546	3554	rVB	949524	2015443	29.33%	4.217%
29	24.798	3683	3691	3703	rVB	1183900	2818105	41.00%	5.897%
30	26.092	3904	3911	3919	rBV	561846	1575311	22.92%	3.296%
31	30.250	4609	4618	4619	rBV3	482265	1110975	16.16%	2.325%
32	30.327	4629	4631	4632	rBV	291793	228434	3.32%	0.478%
33	31.721	4865	4868	4869	rBV	276684	261275	3.80%	0.547%




Sum of corrected areas: 47791764

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024648.D
Acq On : 15 May 2025 22:06
Operator : RC/JU
Sample : Q1984-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-24-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

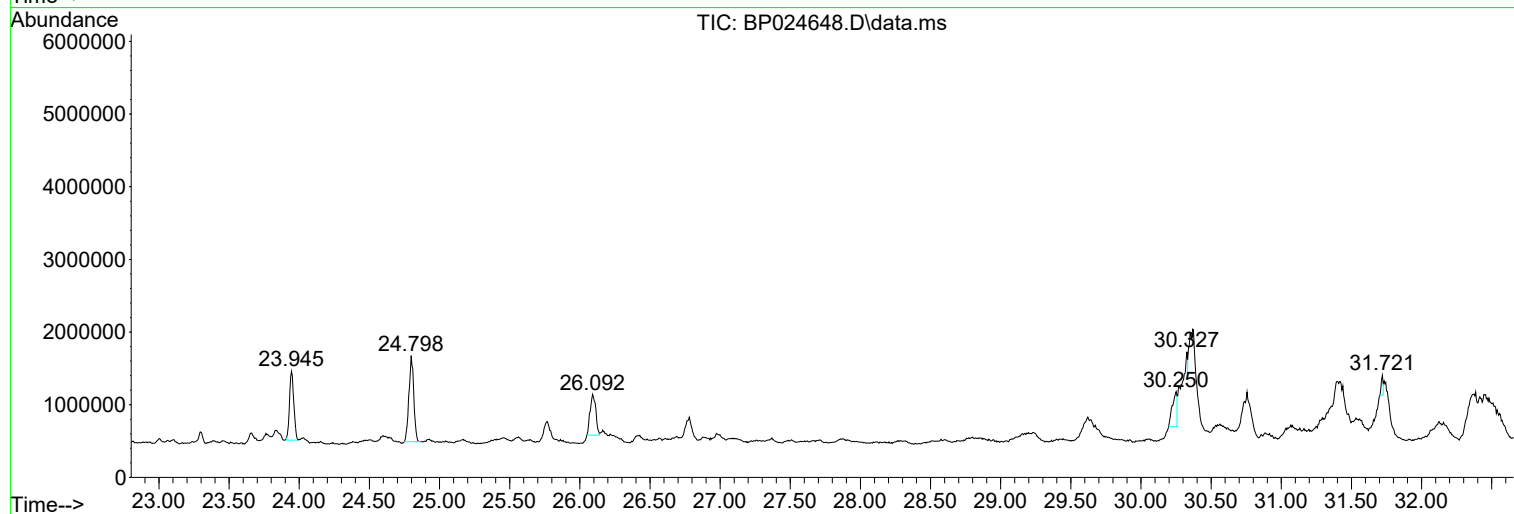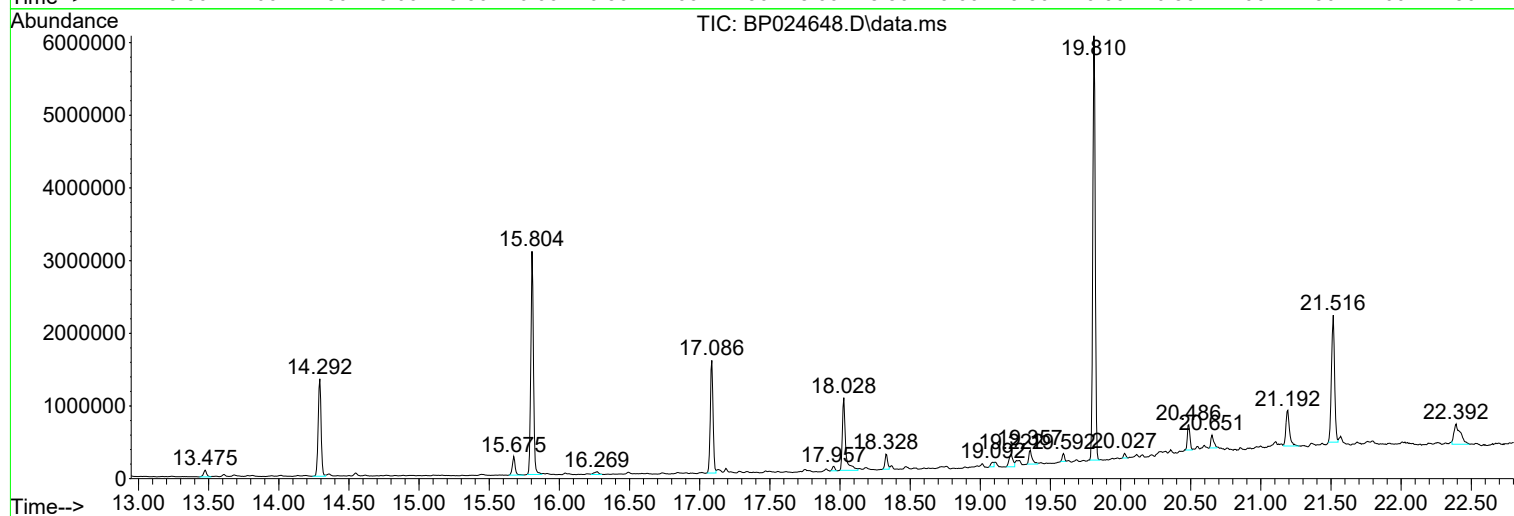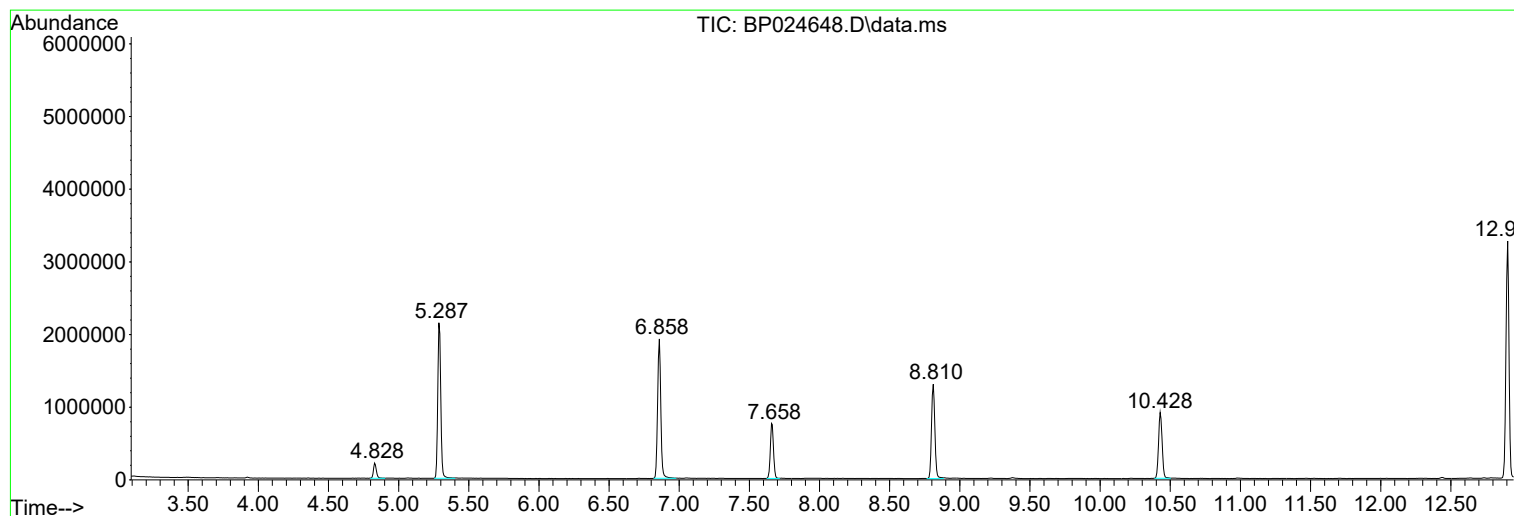

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024648.D
Acq On : 15 May 2025 22:06
Operator : RC/JU
Sample : Q1984-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-24-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051525\
Data File : BP024648.D
Acq On : 15 May 2025 22:06
Operator : RC/JU
Sample : Q1984-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-24-050725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP051325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------