

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
 Data File : BP015106.D
 Acq On : 16 May 2023 12:49
 Operator : CG/JU
 Sample : 02768-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONN3

Quant Time: May 17 00:34:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 16 01:39:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	314072	20.000	ng/ul	0.00
20) Naphthalene-d8	10.963	136	1426667	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.775	164	927225	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.527	188	2041141	20.000	ng/ul	0.00
79) Chrysene-d12	21.604	240	1771595	20.000	ng/ul	0.00
88) Perylene-d12	24.174	264	1756674	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.434	96	39618	4.901	ng/uL	0.00
4) Pyridine-d5	3.881	84	121668	5.310	ng/ul	0.00
7) Phenol-d5	7.451	99	593922	20.367	ng/ul	0.16
9) Bis-(2-Chloroethyl)eth...	7.451	67	600451	35.652	ng/ul	0.00
11) 2-Chlorophenol-d4	7.657	132	411083	19.173	ng/ul	0.00
15) 4-Methylphenol-d8	8.846	113	29946	1.289	ng/ul	0.00
21) Nitrobenzene-d5	9.310	128	398077	35.509	ng/ul	0.00
24) 2-Nitrophenol-d4	10.040	143	371231	29.761	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.581	165	949427	42.180	ng/ul	0.00
31) 4-Chloroaniline-d4	11.116	131	9747	0.293	ng/ul	0.01
46) Dimethylphthalate-d6	14.175	166	2748042	39.221	ng/ul	0.00
49) Acenaphthylene-d8	14.469	160	726801	9.070	ng/ul	0.00
54) 4-Nitrophenol-d4	14.963	143	74851	5.502	ng/ul	0.00
60) Fluorene-d10	15.763	176	1988560	33.634	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.880	200	369056	28.690	ng/ul	0.00
73) Anthracene-d10	17.627	188	1608692	17.212	ng/ul	0.00
81) Pyrene-d10	19.845	212	2647985	25.771	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.004	264	1039309	11.918	ng/ul	-0.02


Target Compounds					Qvalue
10) Bis(2-Chloroethyl)ether	7.534	93	615160	25.713 ng/ul#	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP015106.D
Acq On : 16 May 2023 12:49
Operator : CG/JU
Sample : 02768-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONN3

Quant Time: May 17 00:34:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 16 01:39:21 2023
Response via : Initial Calibration

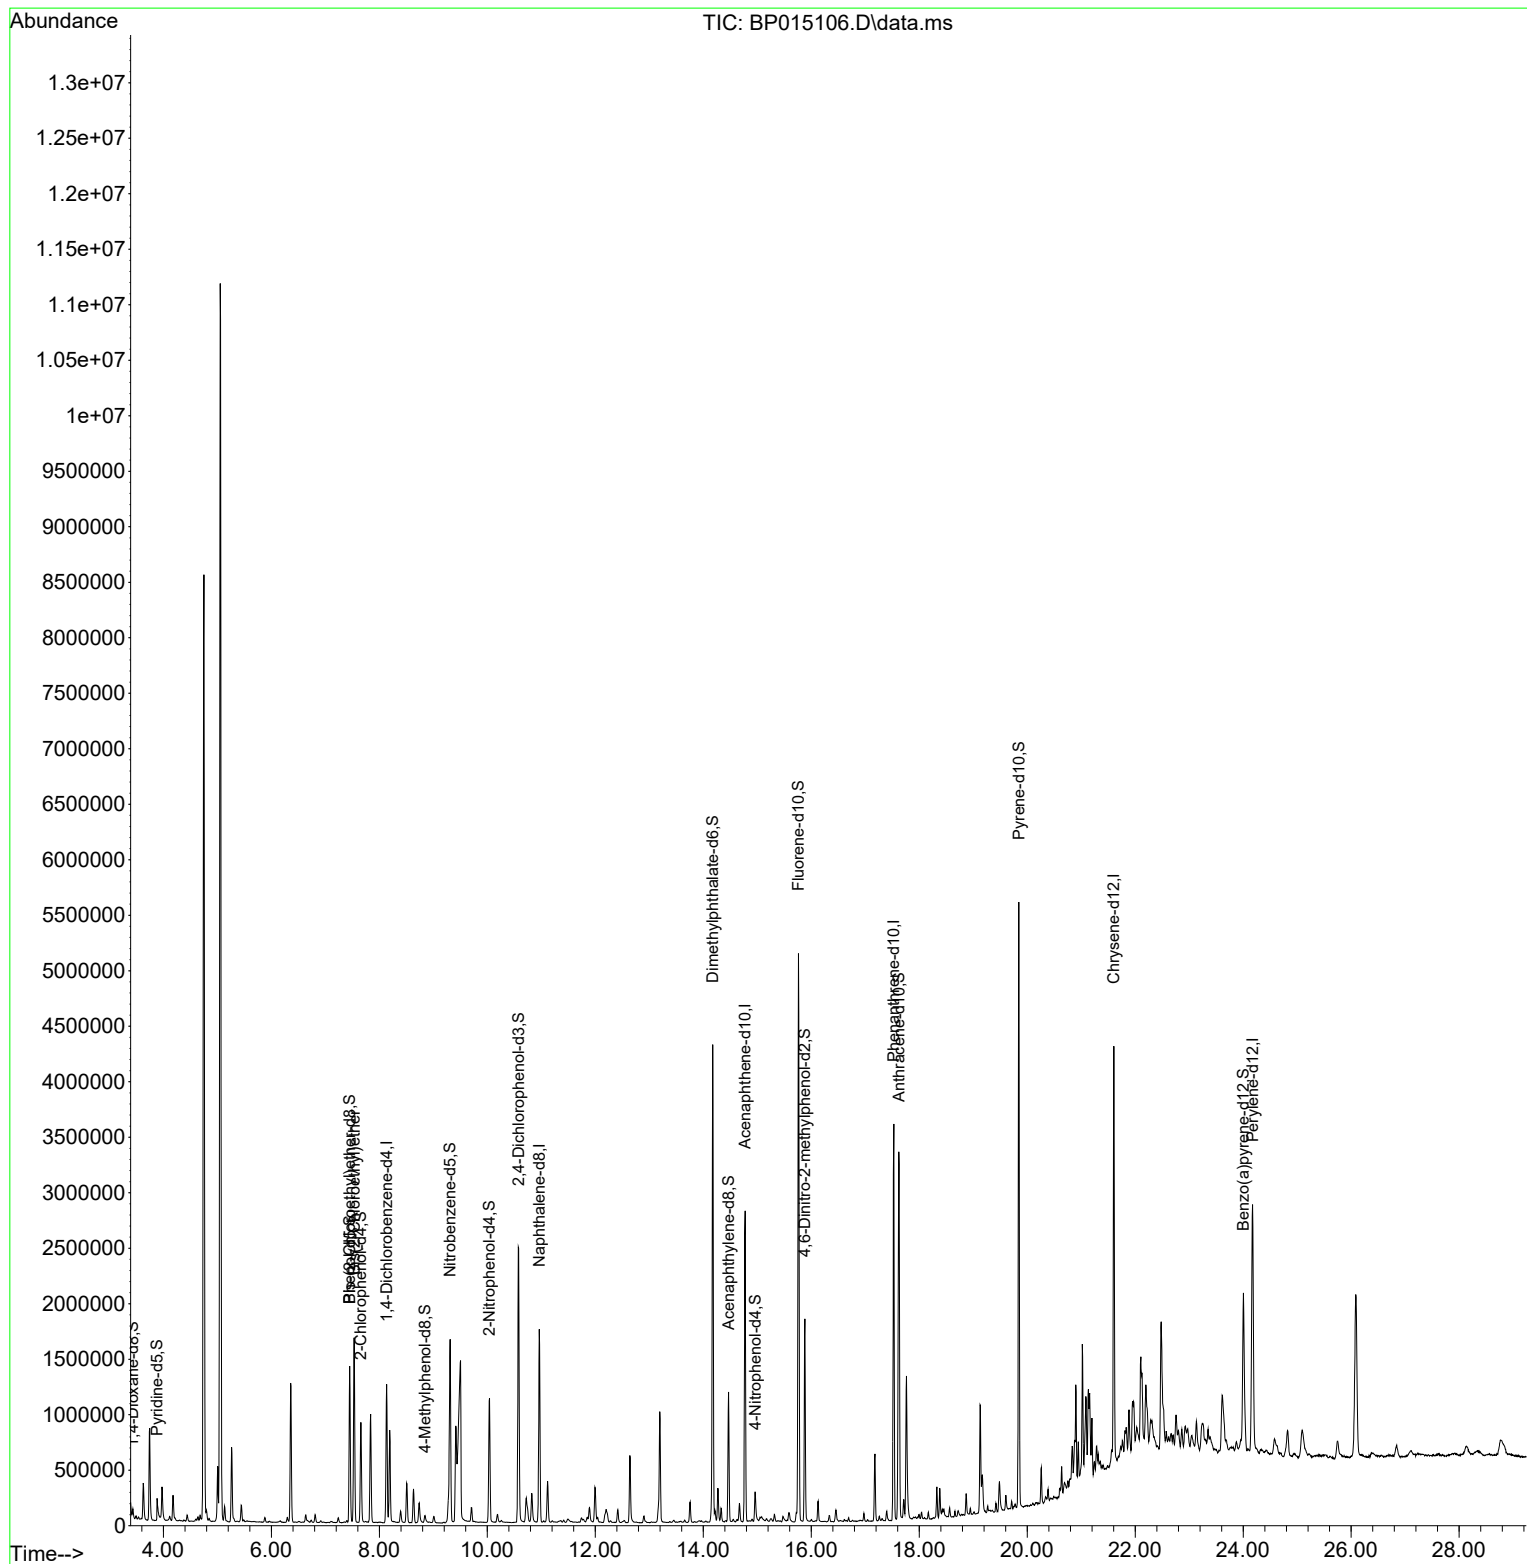

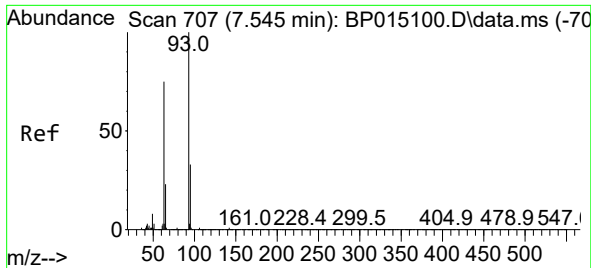

#10
 Bis(2-Chloroethyl)ether
 Concen: 25.713 ng/ul
 RT: 7.534 min Scan# 70
 Delta R.T. -0.018 min
 Lab File: BP015106.D
 Acq: 16 May 2023 12:49

Instrument :
 BNA_P
 ClientSampleId :
 CONN3

Tgt Ion: 93 Resp: 615160
 Ion Ratio Lower Upper
 93 100
 63 6.0 58.0 87.0#
 95 32.2 26.4 39.6

