

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
 Data File : BP015105.D
 Acq On : 16 May 2023 12:16
 Operator : CG/JU
 Sample : 02768-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP015105.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.434	4	8	15	rVB	81888	109808	0.96%	0.108%
2	3.875	81	83	100	rBV	440063	721068	6.28%	0.711%
3	4.117	120	124	130	rVB	40863	64414	0.56%	0.063%
4	4.217	137	141	146	rVB	20031	27672	0.24%	0.027%
5	4.605	204	207	212	rVB7	11503	15729	0.14%	0.016%
6	4.675	215	219	224	rVB	55264	77600	0.68%	0.076%
7	5.169	300	303	310	rVB2	10692	17026	0.15%	0.017%
8	5.664	383	387	392	rVB	15171	21339	0.19%	0.021%
9	5.793	405	409	414	rVB	27947	38808	0.34%	0.038%
10	7.240	649	655	657	rBV	44086	64052	0.56%	0.063%
11	7.281	657	662	678	rVB	348487	568911	4.95%	0.561%
12	7.452	683	691	704	rBV	1411775	2195014	19.11%	2.164%
13	7.658	718	726	737	rBV	1293762	2031339	17.68%	2.002%
14	7.858	755	760	766	rVB5	8245	16089	0.14%	0.016%
15	8.134	799	807	815	rBV	1223972	1942992	16.91%	1.915%
16	8.840	920	927	942	rBV	1070851	1779371	15.49%	1.754%
17	9.310	997	1007	1017	rBV	1588787	2656767	23.13%	2.619%
18	9.410	1019	1024	1030	rVV2	34397	63279	0.55%	0.062%
19	9.469	1030	1034	1038	rVB7	9882	17003	0.15%	0.017%
20	9.705	1068	1074	1081	rBV	129969	196443	1.71%	0.194%
21	10.040	1121	1131	1143	rBV	1227106	2105714	18.33%	2.076%
22	10.269	1164	1170	1175	rBV10	5334	12055	0.10%	0.012%
23	10.575	1214	1222	1234	rBV	1863405	3168895	27.58%	3.124%
24	10.963	1279	1288	1300	rBV	1847304	3048618	26.54%	3.005%
25	11.099	1303	1311	1330	rVV	1669866	2916080	25.38%	2.874%
26	11.746	1414	1421	1424	rBV5	15168	31676	0.28%	0.031%
27	12.199	1493	1498	1505	rVB	88853	137767	1.20%	0.136%
28	12.540	1551	1556	1564	rVB	31071	54218	0.47%	0.053%
29	13.040	1638	1641	1646	rBV7	9630	14621	0.13%	0.014%
30	13.293	1679	1684	1692	rVB7	5485	13137	0.11%	0.013%
31	13.375	1694	1698	1705	rVB8	7476	12104	0.11%	0.012%
32	13.587	1727	1734	1739	rBV6	9719	16449	0.14%	0.016%
33	13.657	1742	1746	1753	rVB4	10357	17314	0.15%	0.017%
34	13.728	1753	1758	1765	rBV8	8874	18340	0.16%	0.018%
35	13.975	1792	1800	1806	rBV8	6045	14183	0.12%	0.014%
36	14.175	1827	1834	1848	rBV	4178467	5809757	50.57%	5.727%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
 Data File : BP015105.D
 Acq On : 16 May 2023 12:16
 Operator : CG/JU
 Sample : 02768-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CONN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
 Title : SVOA CALIBRATION

37	14.293	1851	1854	1859	rVB7	10108	15298	0.13%	0.015%
38	14.410	1870	1874	1877	rBV5	13674	23335	0.20%	0.023%
39	14.469	1877	1884	1900	rVB2	4611119	6816807	59.34%	6.719%
40	14.710	1920	1925	1929	rBV	38074	63833	0.56%	0.063%
41	14.775	1929	1936	1945	rVB	2885094	4288793	37.33%	4.228%
42	14.963	1962	1968	1985	rBV	278949	551015	4.80%	0.543%
43	15.175	1999	2004	2011	rVB9	25404	48947	0.43%	0.048%
44	15.404	2038	2043	2050	rBV6	17019	35218	0.31%	0.035%
45	15.504	2055	2060	2065	rVV	42324	61899	0.54%	0.061%
46	15.551	2065	2068	2070	rVV3	11496	15931	0.14%	0.016%
47	15.581	2070	2073	2080	rVB2	21286	34874	0.30%	0.034%
48	15.722	2092	2097	2099	rBV	74514	104213	0.91%	0.103%
49	15.763	2099	2104	2117	rVV	5971139	8712499	75.84%	8.588%
50	15.881	2117	2124	2140	rVV	2187633	2876034	25.03%	2.835%
51	16.004	2140	2145	2151	rVB3	32601	54260	0.47%	0.053%
52	16.128	2160	2166	2178	rVB	205979	299026	2.60%	0.295%
53	16.463	2216	2223	2225	rBV6	33192	51648	0.45%	0.051%
54	16.975	2305	2310	2314	rBV	76613	99545	0.87%	0.098%
55	17.069	2320	2326	2329	rBV8	8369	18944	0.16%	0.019%
56	17.263	2355	2359	2363	rBV	55097	65767	0.57%	0.065%
57	17.316	2364	2368	2371	rVV2	41344	58817	0.51%	0.058%
58	17.528	2397	2404	2410	rBV	3699797	5223535	45.47%	5.149%
59	17.628	2415	2421	2435	rVV	6995576	9773355	85.07%	9.634%
60	17.798	2447	2450	2456	rBV5	20325	43277	0.38%	0.043%
61	17.916	2468	2470	2474	rBV5	21172	32775	0.29%	0.032%
62	17.998	2481	2484	2488	rVB2	49078	50125	0.44%	0.049%
63	18.045	2488	2492	2495	rBV	62411	80946	0.70%	0.080%
64	18.381	2545	2549	2555	rBV	248890	365774	3.18%	0.361%
65	18.945	2642	2645	2649	rBV2	65384	83228	0.72%	0.082%
66	19.422	2723	2726	2732	rBV	102544	146850	1.28%	0.145%
67	19.492	2735	2738	2745	rVB	104935	154603	1.35%	0.152%
68	19.604	2754	2757	2762	rBV	117399	150103	1.31%	0.148%
69	19.845	2792	2798	2811	rBV	8252701	11488374	100.00%	11.324%
70	21.280	3040	3042	3050	rVB6	130792	184608	1.61%	0.182%
71	21.604	3092	3097	3106	rVB	3741628	4927303	42.89%	4.857%
72	23.351	3391	3394	3403	rVB2	202939	313868	2.73%	0.309%
73	24.010	3498	3506	3518	rBV2	4469728	9635615	83.87%	9.498%
74	24.174	3527	3534	3550	rVB	2051221	4482261	39.02%	4.418%

Sum of corrected areas: 101448955




Instrument :
BNA_P
ClientSampleId :
C0NN9

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP015105.D
Acq On : 16 May 2023 12:16
Operator : CG/JU
Sample : 02768-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONN9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

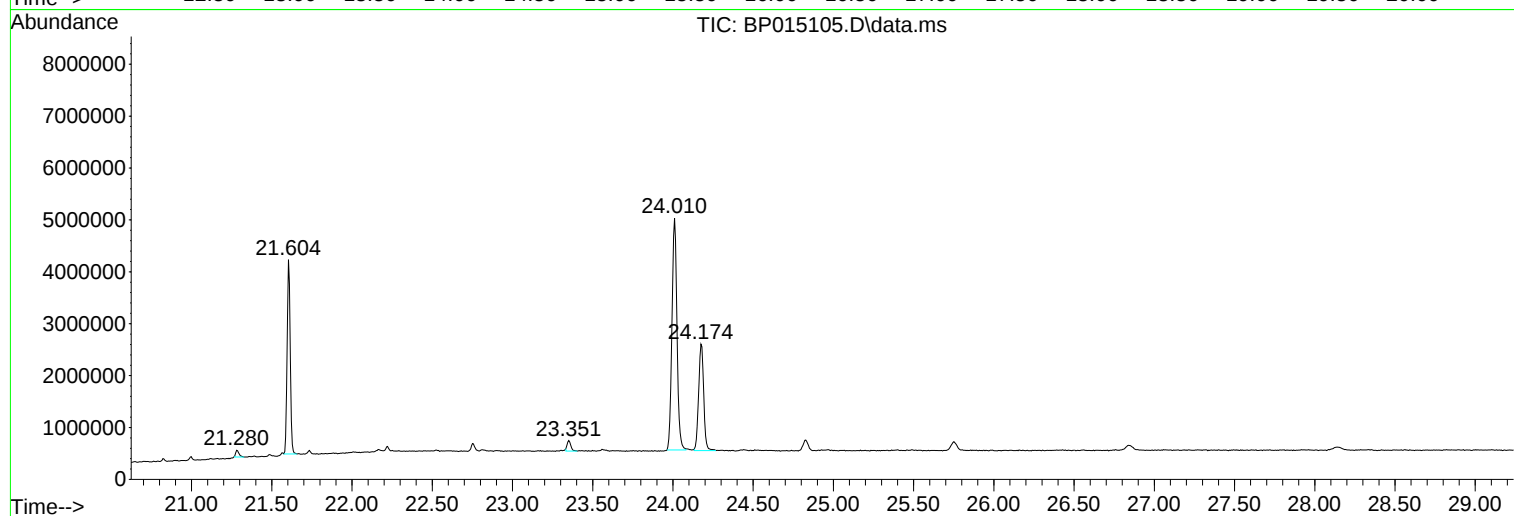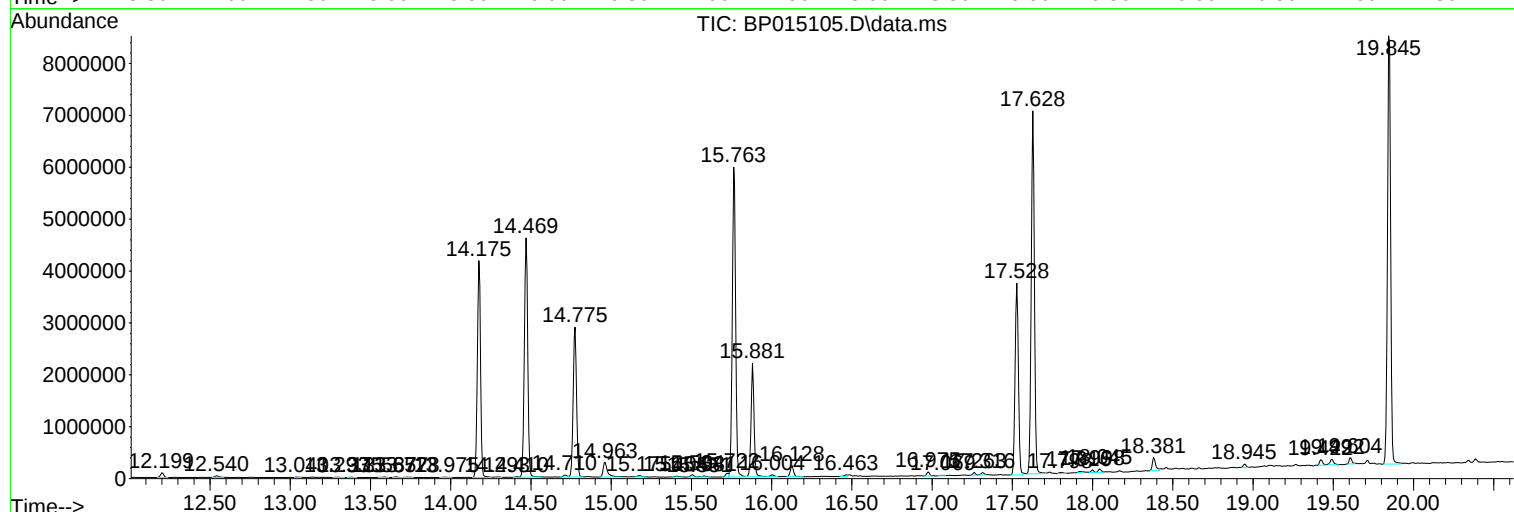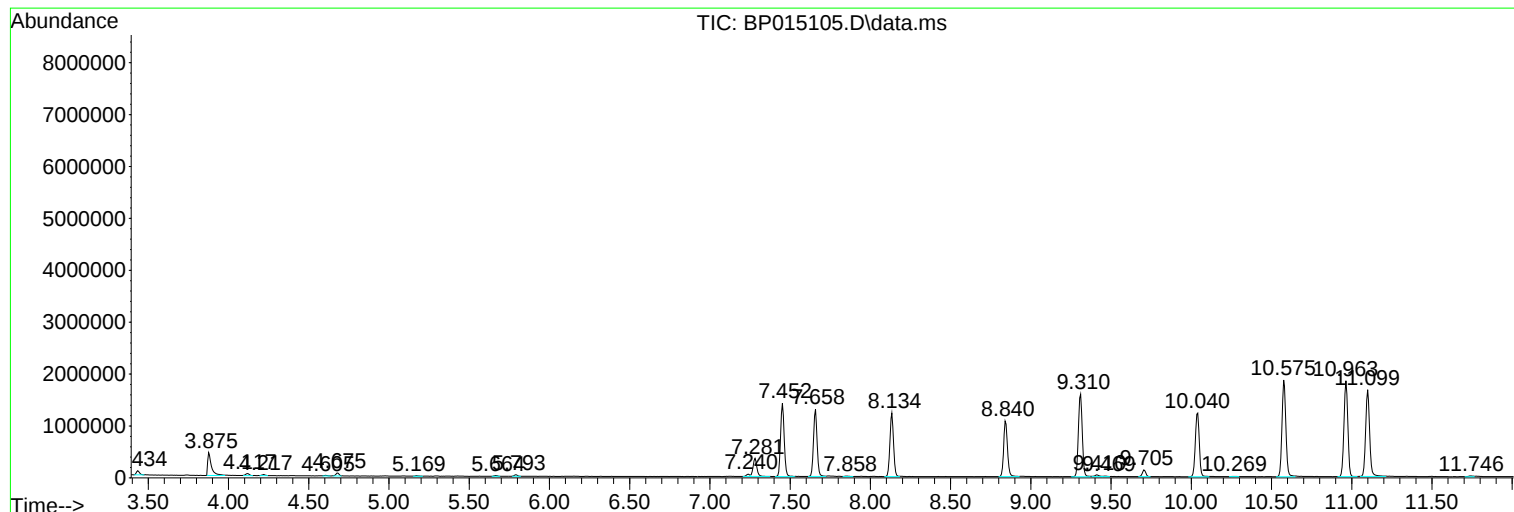

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP015105.D
Acq On : 16 May 2023 12:16
Operator : CG/JU
Sample : 02768-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONN9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP051623\
Data File : BP015105.D
Acq On : 16 May 2023 12:16
Operator : CG/JU
Sample : 02768-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CONN9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP051123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc